

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012515.D
 Acq On : 04 Nov 2022 06:26
 Operator : CG/JU
 Sample : N5353-01
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012515.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	38	41	55	rVB	62751	107704	1.05%	0.113%
2	3.658	112	114	138	rBV	237993	455160	4.43%	0.477%
3	3.864	145	149	157	rVB	22340	36707	0.36%	0.038%
4	3.964	162	166	172	rVB	21403	32187	0.31%	0.034%
5	4.481	251	254	262	rBV4	14555	23051	0.22%	0.024%
6	6.957	668	675	690	rBV	238796	450233	4.38%	0.472%
7	7.116	696	702	718	rBV	1044331	1750267	17.04%	1.835%
8	7.310	728	735	751	rBV	942550	1580133	15.38%	1.657%
9	7.775	806	814	824	rBV	1235960	2013238	19.60%	2.111%
10	8.499	930	937	954	rBV	794543	1408744	13.71%	1.477%
11	8.946	1006	1013	1029	rBV	1298747	2206743	21.48%	2.313%
12	9.322	1073	1077	1084	rVB	26341	41878	0.41%	0.044%
13	9.669	1128	1136	1155	rBV	1001503	1748235	17.02%	1.833%
14	9.940	1178	1182	1189	rBV10	4853	13543	0.13%	0.014%
15	10.204	1218	1227	1248	rBV	1600732	2898184	28.21%	3.038%
16	10.375	1250	1256	1275	rVB2	55967	177077	1.72%	0.186%
17	10.575	1282	1290	1308	rVB	1955832	3391120	33.01%	3.555%
18	10.728	1308	1316	1337	rBV	1386442	2561070	24.93%	2.685%
19	11.410	1425	1432	1436	rBV9	7504	17043	0.17%	0.018%
20	11.998	1526	1532	1537	rVB9	5809	11462	0.11%	0.012%
21	12.175	1555	1562	1570	rVB	25911	45473	0.44%	0.048%
22	13.034	1703	1708	1712	rBV8	6849	10874	0.11%	0.011%
23	13.240	1733	1743	1749	rBV	29440	49655	0.48%	0.052%
24	13.322	1753	1757	1761	rVB3	13253	20981	0.20%	0.022%
25	13.398	1766	1770	1777	rVB5	9494	16501	0.16%	0.017%
26	13.845	1837	1846	1859	rBV	3409046	5057590	49.23%	5.302%
27	14.122	1882	1893	1908	rBV	3788358	5872319	57.16%	6.156%
28	14.322	1923	1927	1936	rVB10	11666	22310	0.22%	0.023%
29	14.428	1939	1945	1954	rBV	3335710	5031988	48.98%	5.275%
30	14.675	1981	1987	2003	rBV	122570	350011	3.41%	0.367%
31	14.851	2015	2017	2029	rVB10	20876	45495	0.44%	0.048%
32	15.016	2036	2045	2046	rBV3	65928	141895	1.38%	0.149%
33	15.275	2086	2089	2094	rVB3	28056	37205	0.36%	0.039%
34	15.428	2109	2115	2122	rBV	5332981	7728528	75.23%	8.102%
35	15.563	2132	2138	2150	rBV	1547209	2301131	22.40%	2.412%
36	15.669	2153	2156	2165	rVB2	29602	50860	0.50%	0.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012515.D
 Acq On : 04 Nov 2022 06:26
 Operator : CG/JU
 Sample : N5353-01
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	16.592	2310	2313	2317	rBV4	22011	29283	0.29%	0.031%
38	17.192	2409	2415	2425	rBV	4178179	6153118	59.90%	6.451%
39	17.292	2426	2432	2444	rVV2	6041516	8810194	85.76%	9.236%
40	17.863	2526	2529	2533	rVB2	38782	42165	0.41%	0.044%
41	18.080	2562	2566	2573	rBV	303060	485834	4.73%	0.509%
42	19.180	2751	2753	2772	rVB2	123270	305328	2.97%	0.320%
43	19.316	2773	2776	2785	rVB	206714	275238	2.68%	0.289%
44	19.533	2807	2813	2827	rBV	7369382	10272623	100.00%	10.769%
45	20.998	3058	3062	3070	rBV2	390501	620932	6.04%	0.651%
46	21.292	3107	3112	3117	rBV	4720538	6254571	60.89%	6.557%
47	23.515	3483	3490	3503	rVB2	4307091	8809463	85.76%	9.235%
48	23.668	3510	3516	3530	rVB2	2708473	5623668	54.74%	5.896%




Sum of corrected areas: 95389012

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012515.D
Acq On : 04 Nov 2022 06:26
Operator : CG/JU
Sample : N5353-01
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWX5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

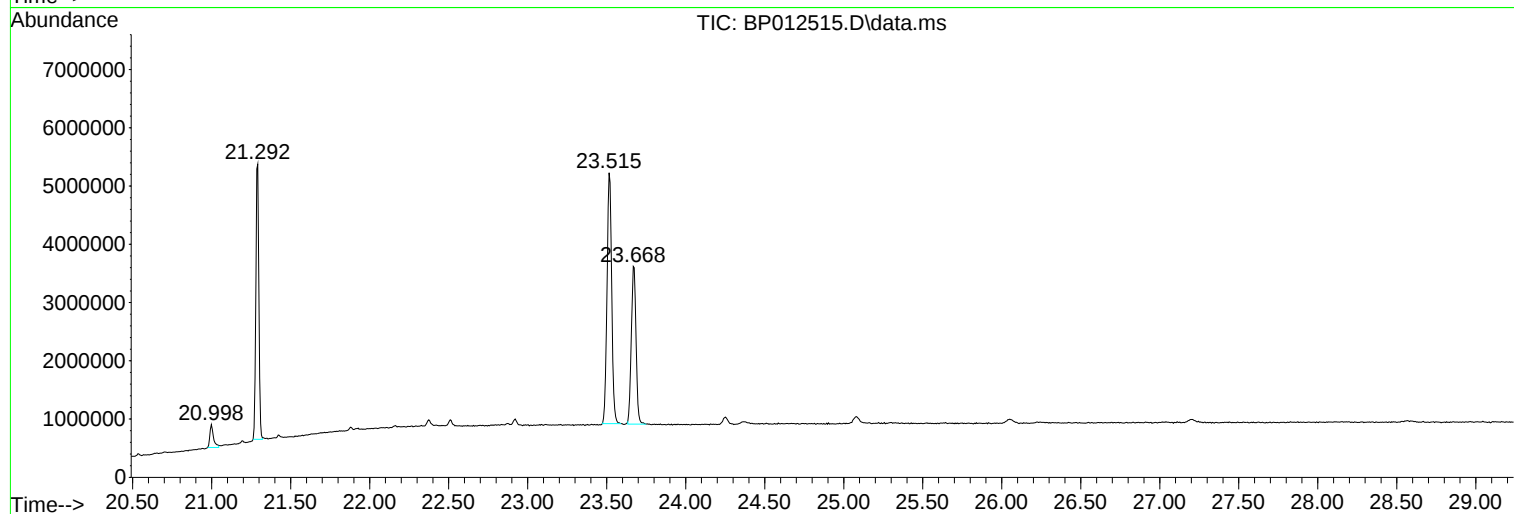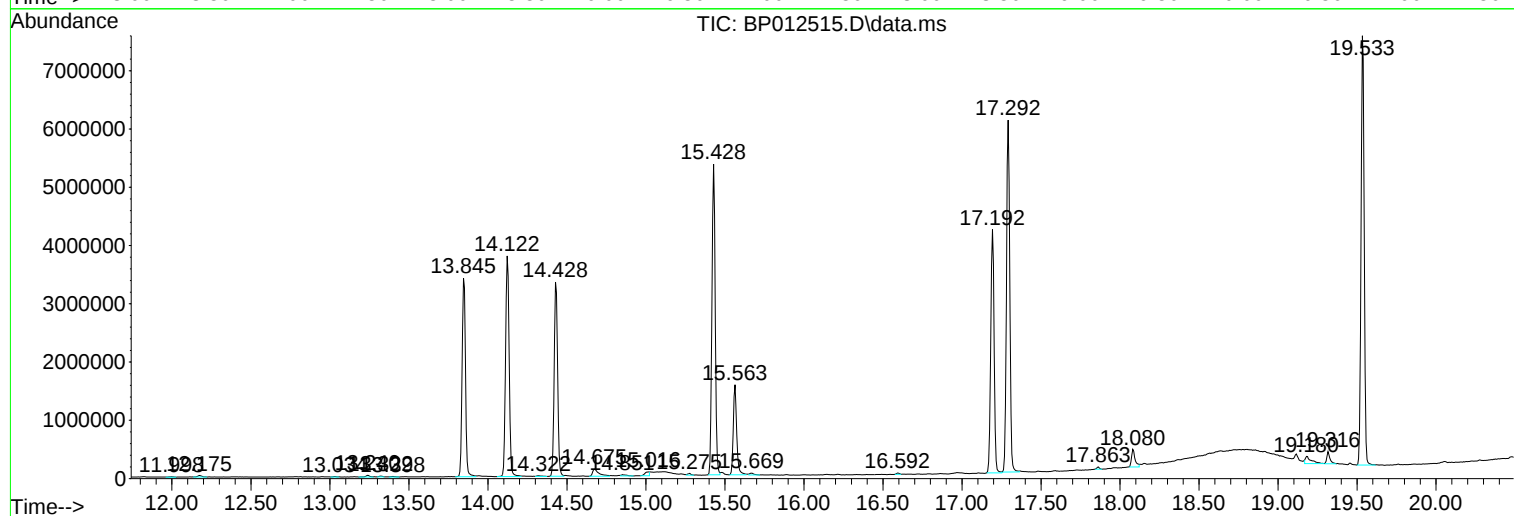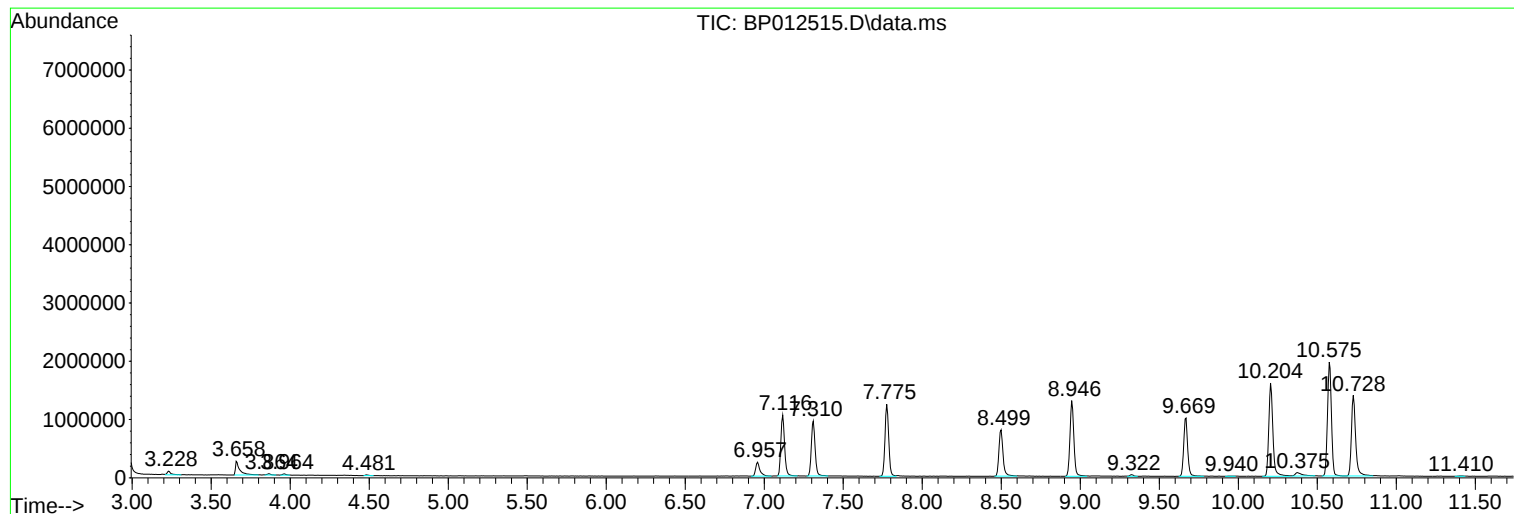

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012515.D
Acq On : 04 Nov 2022 06:26
Operator : CG/JU
Sample : N5353-01
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWX5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012515.D
Acq On : 04 Nov 2022 06:26
Operator : CG/JU
Sample : N5353-01
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWX5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
