

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012516.D
 Acq On : 04 Nov 2022 07:00
 Operator : CG/JU
 Sample : N5353-02
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012516.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	32	35	38	rBV2	13450	17398	0.18%	0.020%
2	3.228	38	41	51	rVB	52487	77624	0.81%	0.090%
3	3.658	113	114	137	rBV	218370	427726	4.49%	0.493%
4	3.864	145	149	159	rVB	18695	32723	0.34%	0.038%
5	3.964	162	166	173	rVB	19894	31409	0.33%	0.036%
6	4.487	250	255	260	rVB	40967	60948	0.64%	0.070%
7	6.887	657	663	667	rVB5	7173	12452	0.13%	0.014%
8	6.958	667	675	687	rBV	245678	452120	4.74%	0.522%
9	7.116	695	702	721	rBV	1068603	1758049	18.44%	2.028%
10	7.311	727	735	745	rBV	965010	1616269	16.96%	1.865%
11	7.775	805	814	825	rBV	1068654	1737921	18.23%	2.005%
12	8.499	929	937	951	rBV	836042	1493861	15.67%	1.723%
13	8.946	1005	1013	1031	rBV	1308065	2217296	23.26%	2.558%
14	9.328	1073	1078	1086	rVB4	13290	27993	0.29%	0.032%
15	9.663	1127	1135	1151	rBV	1021696	1749716	18.36%	2.018%
16	10.205	1219	1227	1251	rBV	1605225	2923641	30.67%	3.373%
17	10.575	1283	1290	1305	rVB	1748762	2928811	30.73%	3.379%
18	10.728	1309	1316	1342	rBV	1171685	2278268	23.90%	2.628%
19	11.263	1401	1407	1412	rBV3	6160	15185	0.16%	0.018%
20	11.822	1499	1502	1506	rVB6	6333	9835	0.10%	0.011%
21	12.175	1556	1562	1572	rVB	25196	47216	0.50%	0.054%
22	13.034	1702	1708	1714	rBV7	9949	15235	0.16%	0.018%
23	13.151	1723	1728	1732	rBV8	5277	9927	0.10%	0.011%
24	13.322	1751	1757	1763	rVB5	13313	23385	0.25%	0.027%
25	13.846	1836	1846	1860	rBV	3408976	4921901	51.64%	5.678%
26	14.122	1884	1893	1909	rBV	3834482	5867183	61.56%	6.768%
27	14.428	1938	1945	1954	rBV	2831188	4286276	44.97%	4.945%
28	14.504	1954	1958	1981	rVV	106783	293212	3.08%	0.338%
29	14.675	1982	1987	2005	rVV	110646	318342	3.34%	0.367%
30	15.181	2069	2073	2077	rBV	43529	62347	0.65%	0.072%
31	15.222	2077	2080	2083	rVV	38394	52733	0.55%	0.061%
32	15.257	2083	2086	2096	rVB	75377	106944	1.12%	0.123%
33	15.428	2108	2115	2132	rBV	5074092	7590122	79.63%	8.756%
34	15.563	2132	2138	2152	rVV	1433744	2123832	22.28%	2.450%
35	15.669	2152	2156	2162	rVB	30127	50281	0.53%	0.058%
36	17.192	2408	2415	2425	rBV	3640913	5308079	55.69%	6.123%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012516.D
 Acq On : 04 Nov 2022 07:00
 Operator : CG/JU
 Sample : N5353-02
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	17.292	2425	2432	2450	rVV	5522222	8378862	87.91%	9.666%
38	18.081	2562	2566	2574	rBV2	131234	225808	2.37%	0.260%
39	19.110	2738	2741	2744	rBV	74171	82208	0.86%	0.095%
40	19.181	2750	2753	2758	rBV	64569	83870	0.88%	0.097%
41	19.316	2773	2776	2781	rBV2	116085	172509	1.81%	0.199%
42	19.533	2807	2813	2823	rBV2	6709188	9531523	100.00%	10.995%
43	21.286	3106	3111	3121	rBV	4112315	5139792	53.92%	5.929%
44	23.516	3483	3490	3507	rVB2	3665993	7769934	81.52%	8.963%
45	23.669	3510	3516	3531	rVB2	2093567	4355581	45.70%	5.025%




Sum of corrected areas: 86686347

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012516.D
Acq On : 04 Nov 2022 07:00
Operator : CG/JU
Sample : N5353-02
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

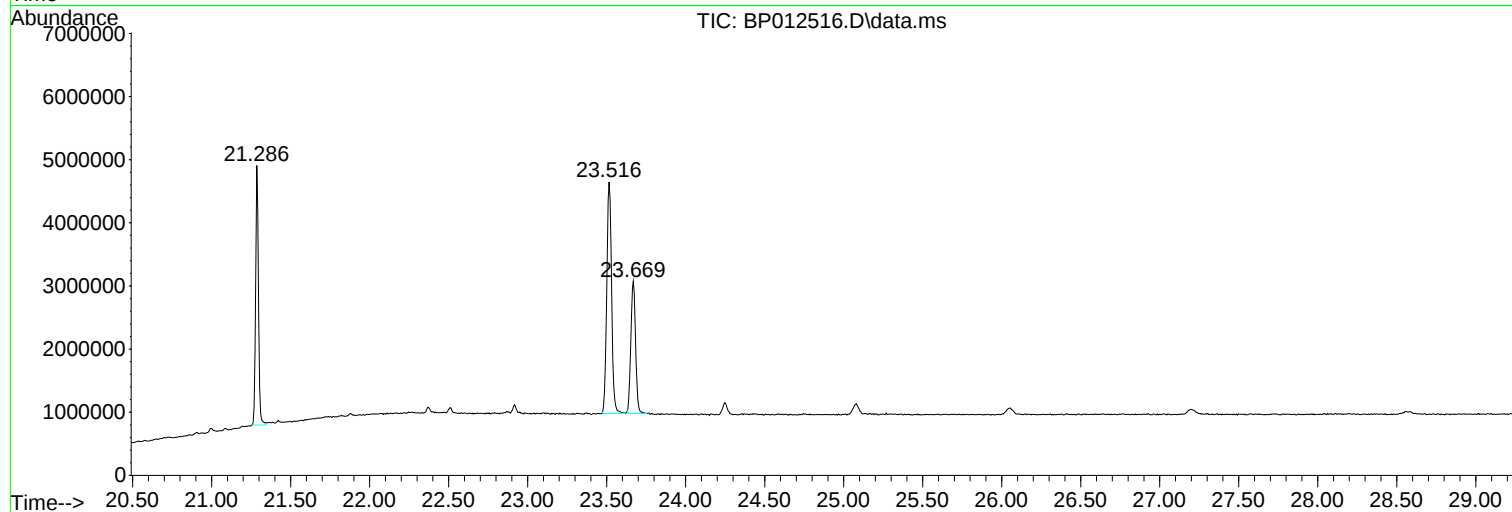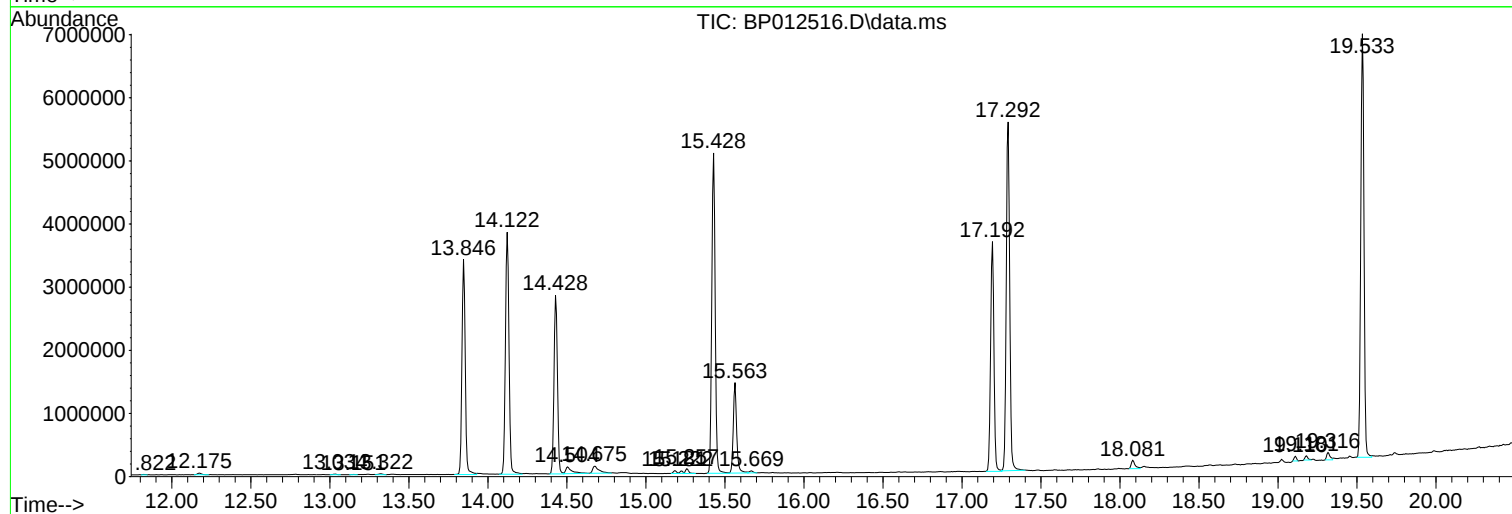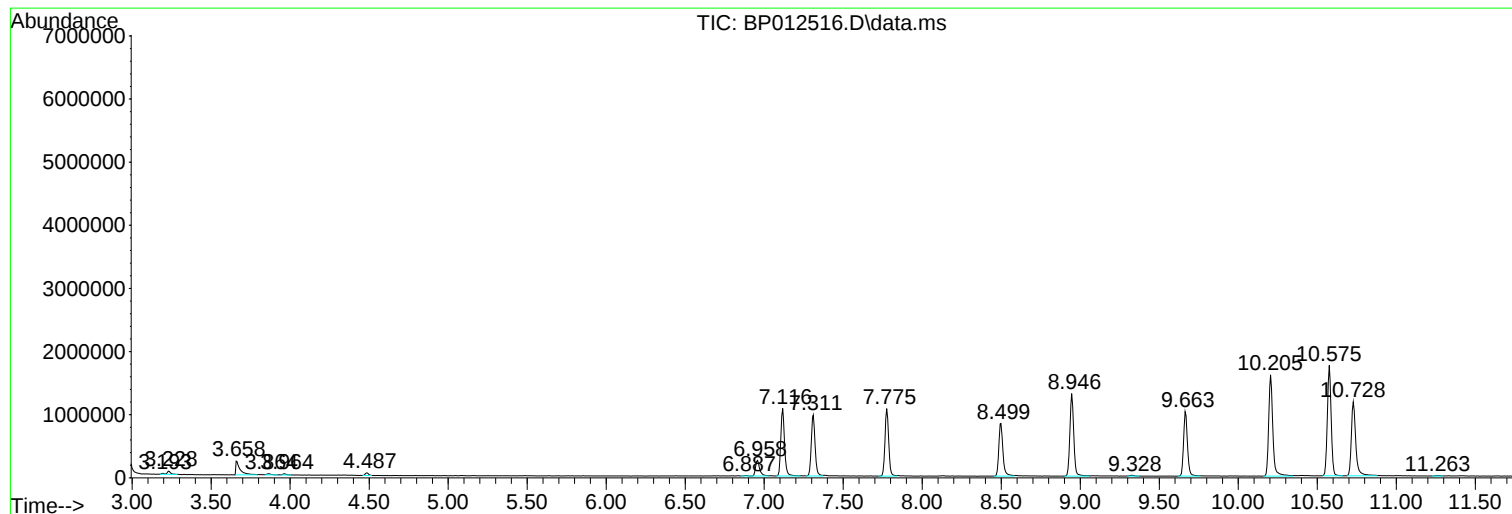

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012516.D
Acq On : 04 Nov 2022 07:00
Operator : CG/JU
Sample : N5353-02
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012516.D
Acq On : 04 Nov 2022 07:00
Operator : CG/JU
Sample : N5353-02
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
