

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012518.D
 Acq On : 04 Nov 2022 08:08
 Operator : CG/JU
 Sample : N5353-05
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	39	rBV	59408	89097	0.79%	0.090%
2	3.228	39	41	53	rVB	61273	94067	0.83%	0.095%
3	3.658	111	114	129	rBV	275738	486831	4.31%	0.490%
4	3.864	145	149	155	rVB	24856	35063	0.31%	0.035%
5	3.964	162	166	173	rVB	20965	29345	0.26%	0.030%
6	6.958	668	675	688	rBV	284608	522282	4.63%	0.526%
7	7.116	695	702	713	rBV	1213306	1968334	17.44%	1.982%
8	7.311	728	735	753	rBV	1102738	1831038	16.22%	1.844%
9	7.775	807	814	823	rBV	1177100	1905098	16.88%	1.918%
10	8.493	929	936	953	rBV	917331	1655321	14.66%	1.667%
11	8.946	1005	1013	1031	rBV	1492294	2526224	22.38%	2.543%
12	9.322	1072	1077	1083	rVB	17289	27048	0.24%	0.027%
13	9.663	1125	1135	1151	rBV	1178814	2044035	18.11%	2.058%
14	10.204	1219	1227	1255	rBV	1728502	3160849	28.00%	3.182%
15	10.410	1256	1262	1268	rVV9	7376	17625	0.16%	0.018%
16	10.575	1281	1290	1303	rBV	1921563	3209126	28.43%	3.231%
17	10.728	1308	1316	1345	rBV	1512427	2850597	25.25%	2.870%
18	11.422	1426	1434	1440	rBV	5838	16840	0.15%	0.017%
19	12.175	1556	1562	1570	rBV3	27914	55700	0.49%	0.056%
20	13.234	1736	1742	1750	rBV3	15554	26487	0.23%	0.027%
21	13.322	1752	1757	1761	rVV6	9314	15126	0.13%	0.015%
22	13.393	1761	1769	1776	rVB5	7681	14341	0.13%	0.014%
23	13.845	1837	1846	1861	rBV	3920416	5674792	50.27%	5.714%
24	14.122	1884	1893	1912	rBV	4326827	6623393	58.67%	6.669%
25	14.428	1938	1945	1959	rBV	3192895	4780626	42.35%	4.813%
26	14.675	1980	1987	2004	rBV	133254	423487	3.75%	0.426%
27	14.857	2012	2018	2019	rBV6	12213	19360	0.17%	0.019%
28	15.222	2076	2080	2084	rBV	15555	20991	0.19%	0.021%
29	15.269	2084	2088	2094	rVB3	16853	28081	0.25%	0.028%
30	15.428	2104	2115	2132	rBV	5840550	8752819	77.54%	8.813%
31	15.563	2132	2138	2151	rVV	1654474	2501143	22.16%	2.518%
32	15.663	2152	2155	2165	rVB	37854	70031	0.62%	0.071%
33	16.134	2232	2235	2243	rVV9	9007	19099	0.17%	0.019%
34	16.210	2243	2248	2254	rVB8	12435	24080	0.21%	0.024%
35	17.192	2408	2415	2425	rBV	3934854	5907879	52.33%	5.948%
36	17.292	2425	2432	2448	rVV	6697952	9972893	88.34%	10.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012518.D
 Acq On : 04 Nov 2022 08:08
 Operator : CG/JU
 Sample : N5353-05
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	17.481	2461	2464	2471	rVB2	12517	20188	0.18%	0.020%
38	18.081	2561	2566	2574	rBV3	110185	190003	1.68%	0.191%
39	19.110	2736	2741	2746	rBV	100393	150634	1.33%	0.152%
40	19.180	2749	2753	2756	rBV	80852	117673	1.04%	0.118%
41	19.316	2773	2776	2785	rBV3	76731	121278	1.07%	0.122%
42	19.533	2807	2813	2826	rBV	8391824	11288741	100.00%	11.366%
43	21.286	3106	3111	3120	rBV	4360763	5659020	50.13%	5.698%
44	23.516	3482	3490	3502	rBV2	4552628	9377362	83.07%	9.441%
45	23.668	3509	3516	3528	rVB2	2445561	4997358	44.27%	5.032%




Sum of corrected areas: 99321405

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012518.D
Acq On : 04 Nov 2022 08:08
Operator : CG/JU
Sample : N5353-05
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

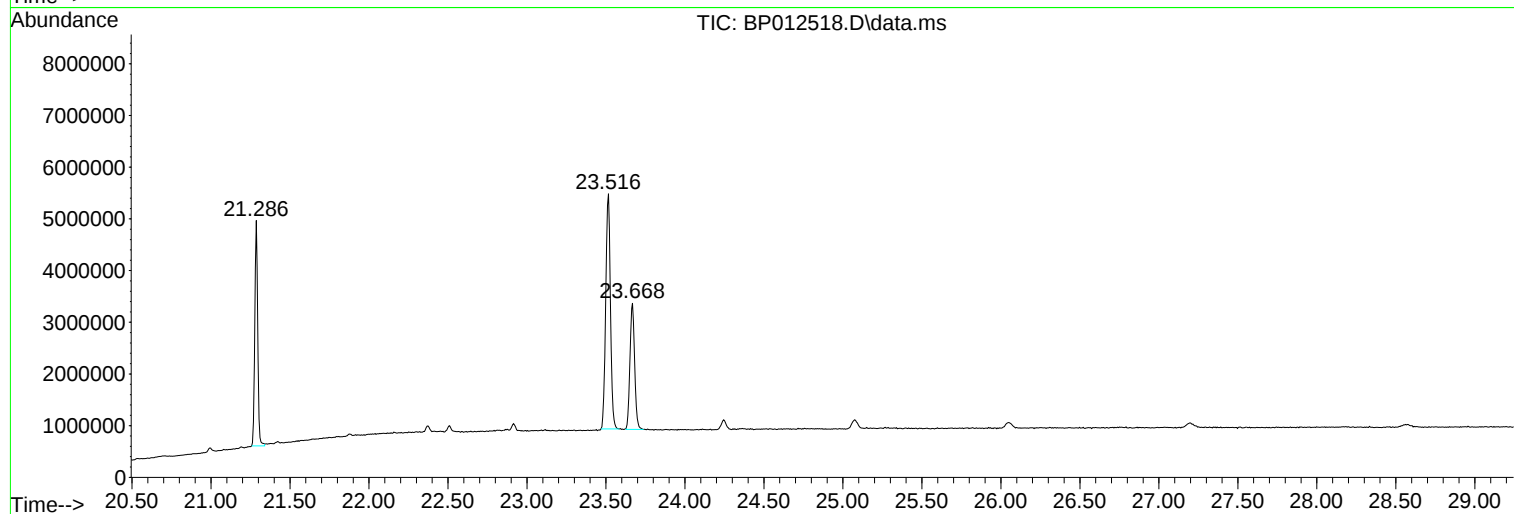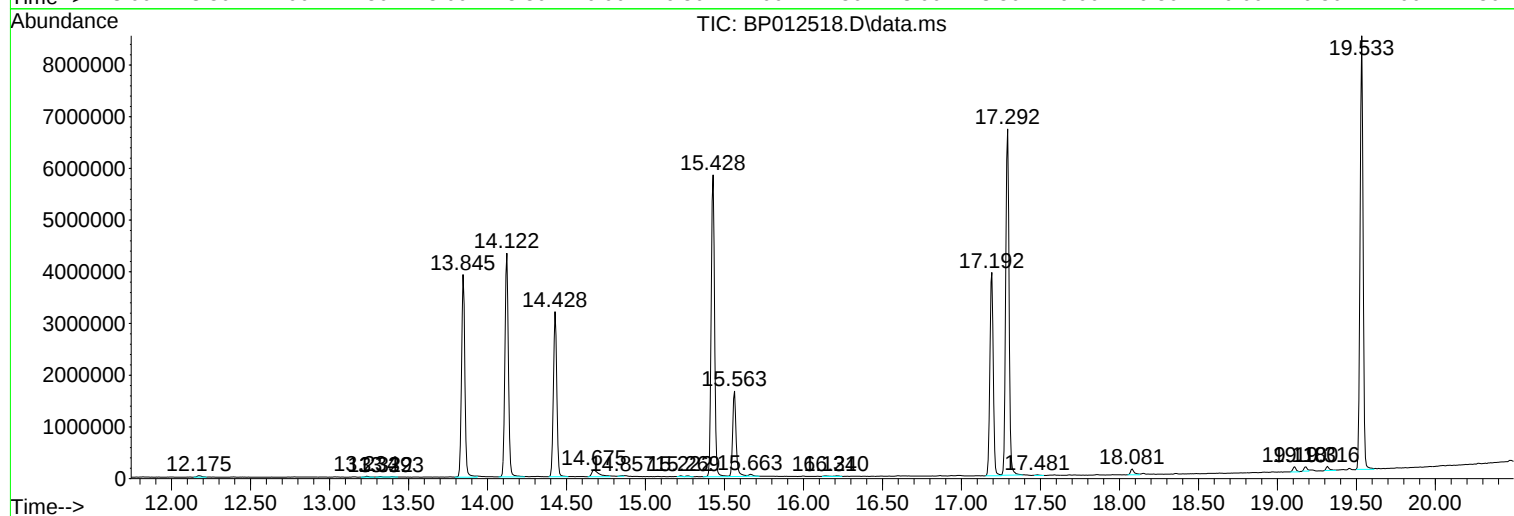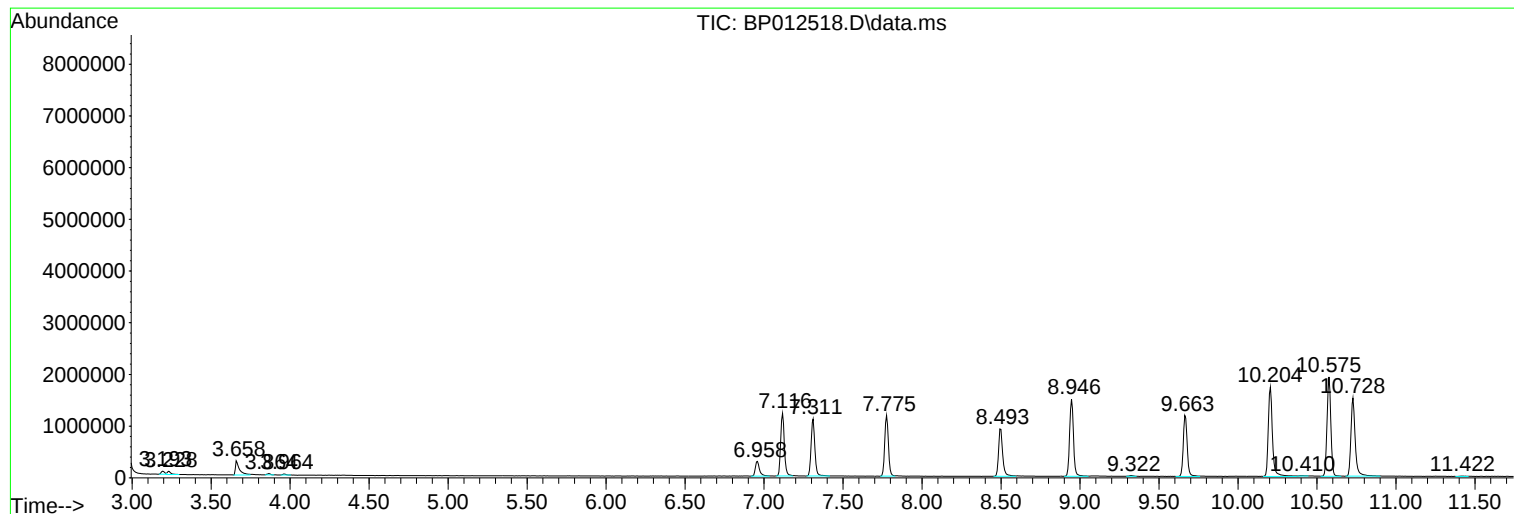

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012518.D
Acq On : 04 Nov 2022 08:08
Operator : CG/JU
Sample : N5353-05
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012518.D
Acq On : 04 Nov 2022 08:08
Operator : CG/JU
Sample : N5353-05
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc