

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012520.D
 Acq On : 04 Nov 2022 09:17
 Operator : CG/JU
 Sample : N5353-08
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	38	41	51	rVB	47607	72673	0.72%	0.084%
2	3.664	112	115	130	rBV	192773	385203	3.81%	0.445%
3	3.864	145	149	156	rVB	21522	33267	0.33%	0.038%
4	3.964	162	166	178	rVB	21932	38271	0.38%	0.044%
5	6.893	656	664	667	rVB6	6163	12210	0.12%	0.014%
6	6.958	669	675	691	rVV	212533	400585	3.96%	0.463%
7	7.116	696	702	716	rBV	1015067	1653147	16.35%	1.910%
8	7.310	728	735	747	rBV	909299	1495540	14.79%	1.728%
9	7.775	807	814	824	rBV	989585	1636386	16.18%	1.890%
10	8.499	930	937	954	rBV	746250	1311518	12.97%	1.515%
11	8.887	994	1003	1007	rBV	49466	83084	0.82%	0.096%
12	8.946	1007	1013	1031	rVB	1251543	2117041	20.94%	2.446%
13	9.328	1073	1078	1084	rVB2	15623	26846	0.27%	0.031%
14	9.669	1128	1136	1147	rBV	950645	1677827	16.59%	1.938%
15	10.204	1219	1227	1250	rBV	1437360	2676835	26.47%	3.093%
16	10.387	1254	1258	1272	rVB2	19114	61843	0.61%	0.071%
17	10.575	1282	1290	1307	rVB	1593429	2715311	26.86%	3.137%
18	10.728	1309	1316	1337	rBV	1255143	2368005	23.42%	2.736%
19	11.428	1429	1435	1441	rBV	4367	11005	0.11%	0.013%
20	11.551	1450	1456	1468	rBV2	53593	151077	1.49%	0.175%
21	11.828	1495	1503	1508	rBV10	4952	11503	0.11%	0.013%
22	12.098	1544	1549	1555	rBV7	5320	10689	0.11%	0.012%
23	12.175	1557	1562	1569	rVV2	25594	45245	0.45%	0.052%
24	13.034	1703	1708	1714	rBV9	7276	14050	0.14%	0.016%
25	13.240	1735	1743	1749	rBV3	14777	26068	0.26%	0.030%
26	13.322	1751	1757	1764	rVV6	12637	20970	0.21%	0.024%
27	13.392	1764	1769	1773	rBV7	7187	10957	0.11%	0.013%
28	13.845	1839	1846	1861	rBV	3471808	4864131	48.11%	5.619%
29	13.951	1862	1864	1869	rVB6	14199	18322	0.18%	0.021%
30	14.122	1886	1893	1911	rBV	3658346	5592026	55.31%	6.460%
31	14.316	1922	1926	1930	rVB5	7116	11670	0.12%	0.013%
32	14.428	1938	1945	1959	rBV	2712308	4042171	39.98%	4.670%
33	14.675	1982	1987	2008	rBV2	92336	336195	3.33%	0.388%
34	14.875	2019	2021	2028	rVB7	14369	23830	0.24%	0.028%
35	15.187	2070	2074	2078	rBV	15572	22862	0.23%	0.026%
36	15.222	2078	2080	2083	rVV	10100	13316	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
 Data File : BP012520.D
 Acq On : 04 Nov 2022 09:17
 Operator : CG/JU
 Sample : N5353-08
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBWR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
 Title : SVOA CALIBRATION

37	15.263	2083	2087	2092	rVB2	42875	63193	0.62%	0.073%
38	15.428	2106	2115	2132	rBV	4967722	7626727	75.43%	8.811%
39	15.563	2132	2138	2151	rVV	1428889	2061896	20.39%	2.382%
40	15.669	2153	2156	2162	rVB2	30133	45194	0.45%	0.052%
41	16.216	2246	2249	2255	rVB6	10553	17488	0.17%	0.020%
42	17.057	2387	2392	2396	rBV7	10605	19139	0.19%	0.022%
43	17.192	2408	2415	2425	rBV	3410529	5111596	50.56%	5.905%
44	17.292	2425	2432	2455	rVB	5965177	8830818	87.34%	10.202%
45	17.798	2514	2518	2522	rBV	16534	24923	0.25%	0.029%
46	18.080	2562	2566	2575	rBV	123459	200343	1.98%	0.231%
47	19.110	2737	2741	2746	rBV	88001	113063	1.12%	0.131%
48	19.180	2749	2753	2757	rBV	82837	123089	1.22%	0.142%
49	19.316	2773	2776	2782	rBV2	83446	134364	1.33%	0.155%
50	19.533	2807	2813	2827	rBV	7467651	10110935	100.00%	11.681%
51	20.992	3059	3061	3068	rVB2	116542	160777	1.59%	0.186%
52	21.286	3106	3111	3119	rBV	3950945	5088886	50.33%	5.879%
53	23.510	3483	3489	3504	rVB2	4060841	8483094	83.90%	9.800%
54	23.668	3509	3516	3526	rVB2	2063652	4351350	43.04%	5.027%




Sum of corrected areas: 86558554

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012520.D
Acq On : 04 Nov 2022 09:17
Operator : CG/JU
Sample : N5353-08
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWR2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

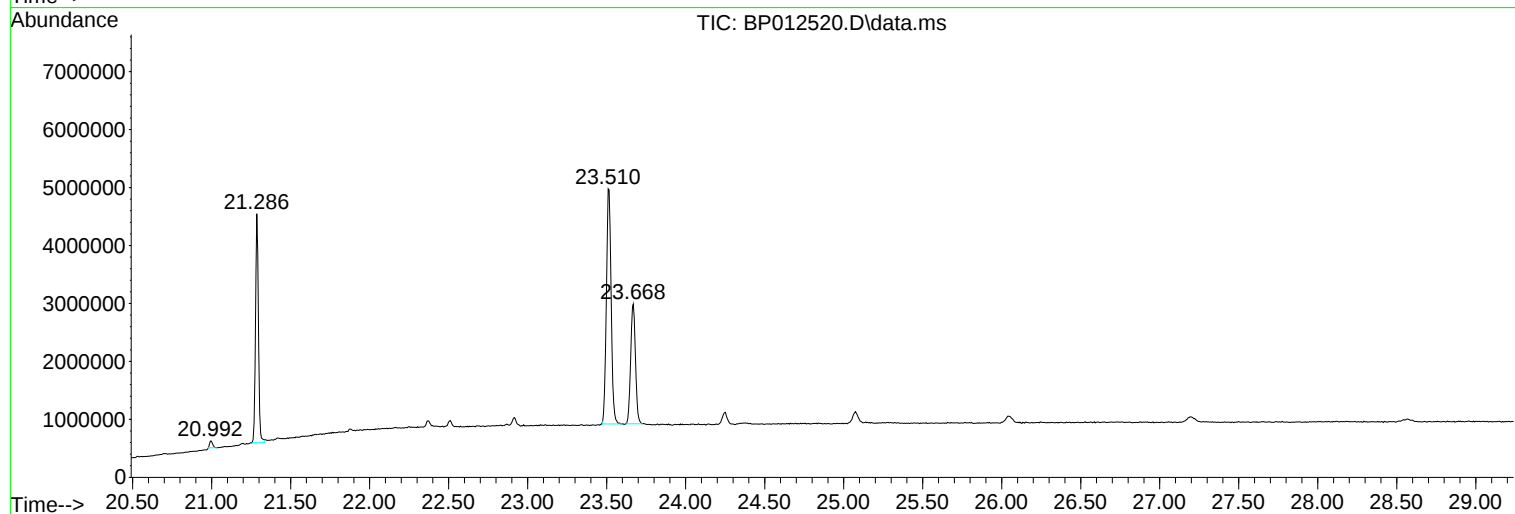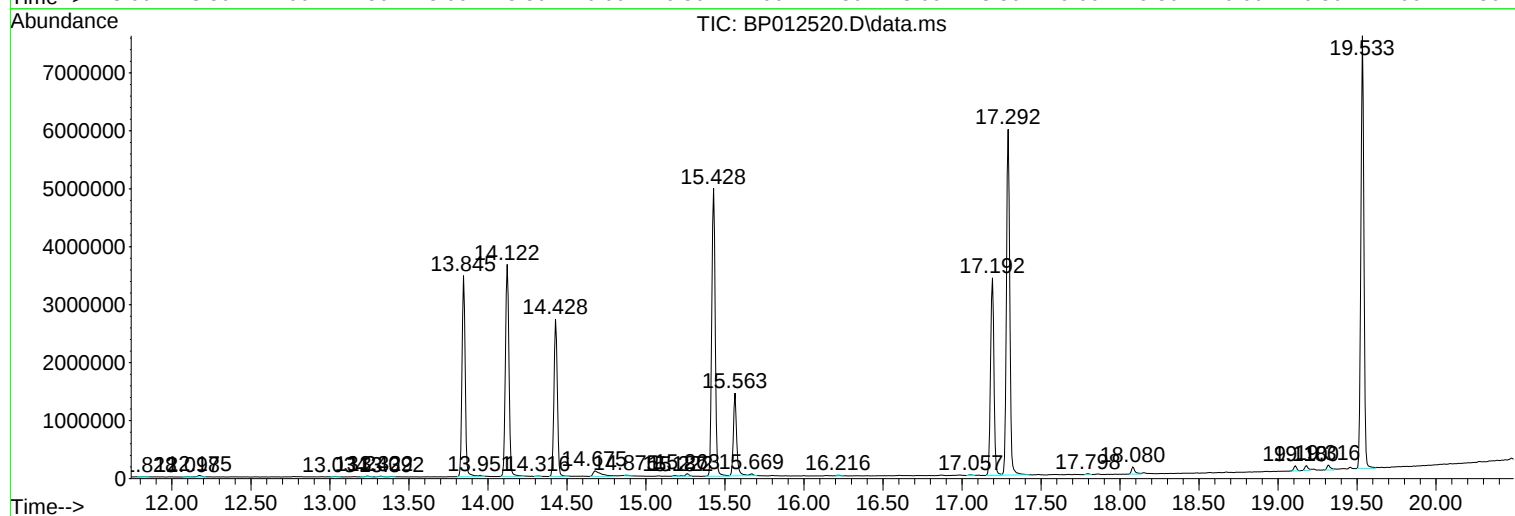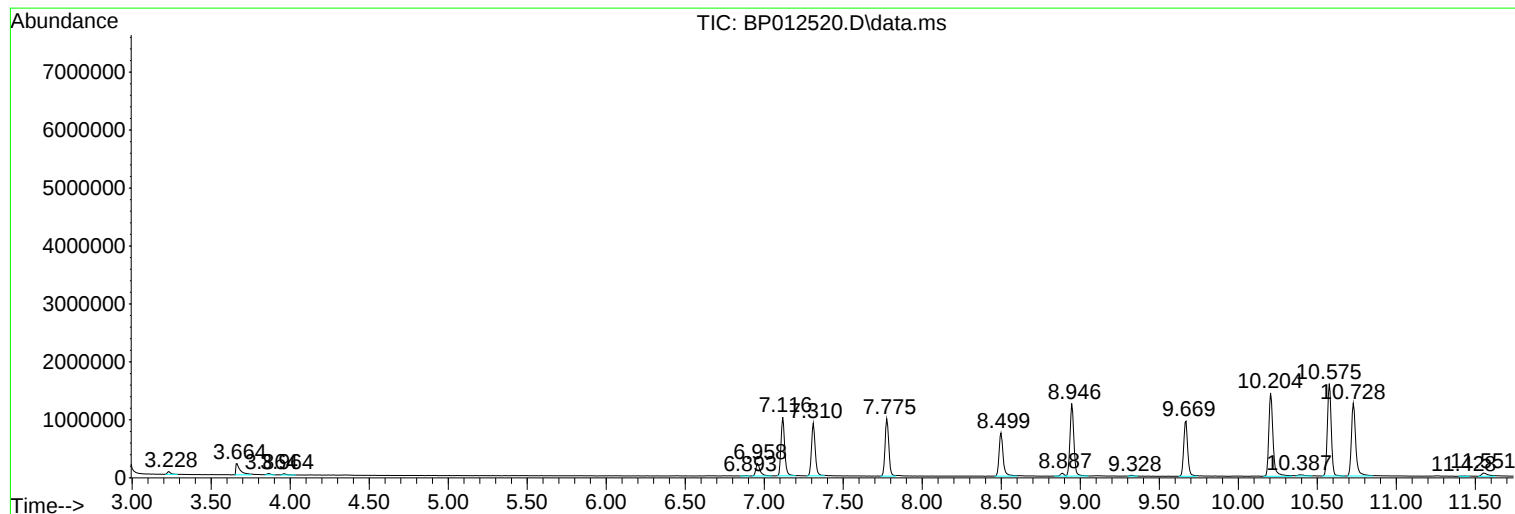

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012520.D
Acq On : 04 Nov 2022 09:17
Operator : CG/JU
Sample : N5353-08
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWR2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110222\
Data File : BP012520.D
Acq On : 04 Nov 2022 09:17
Operator : CG/JU
Sample : N5353-08
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBWR2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP102522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
