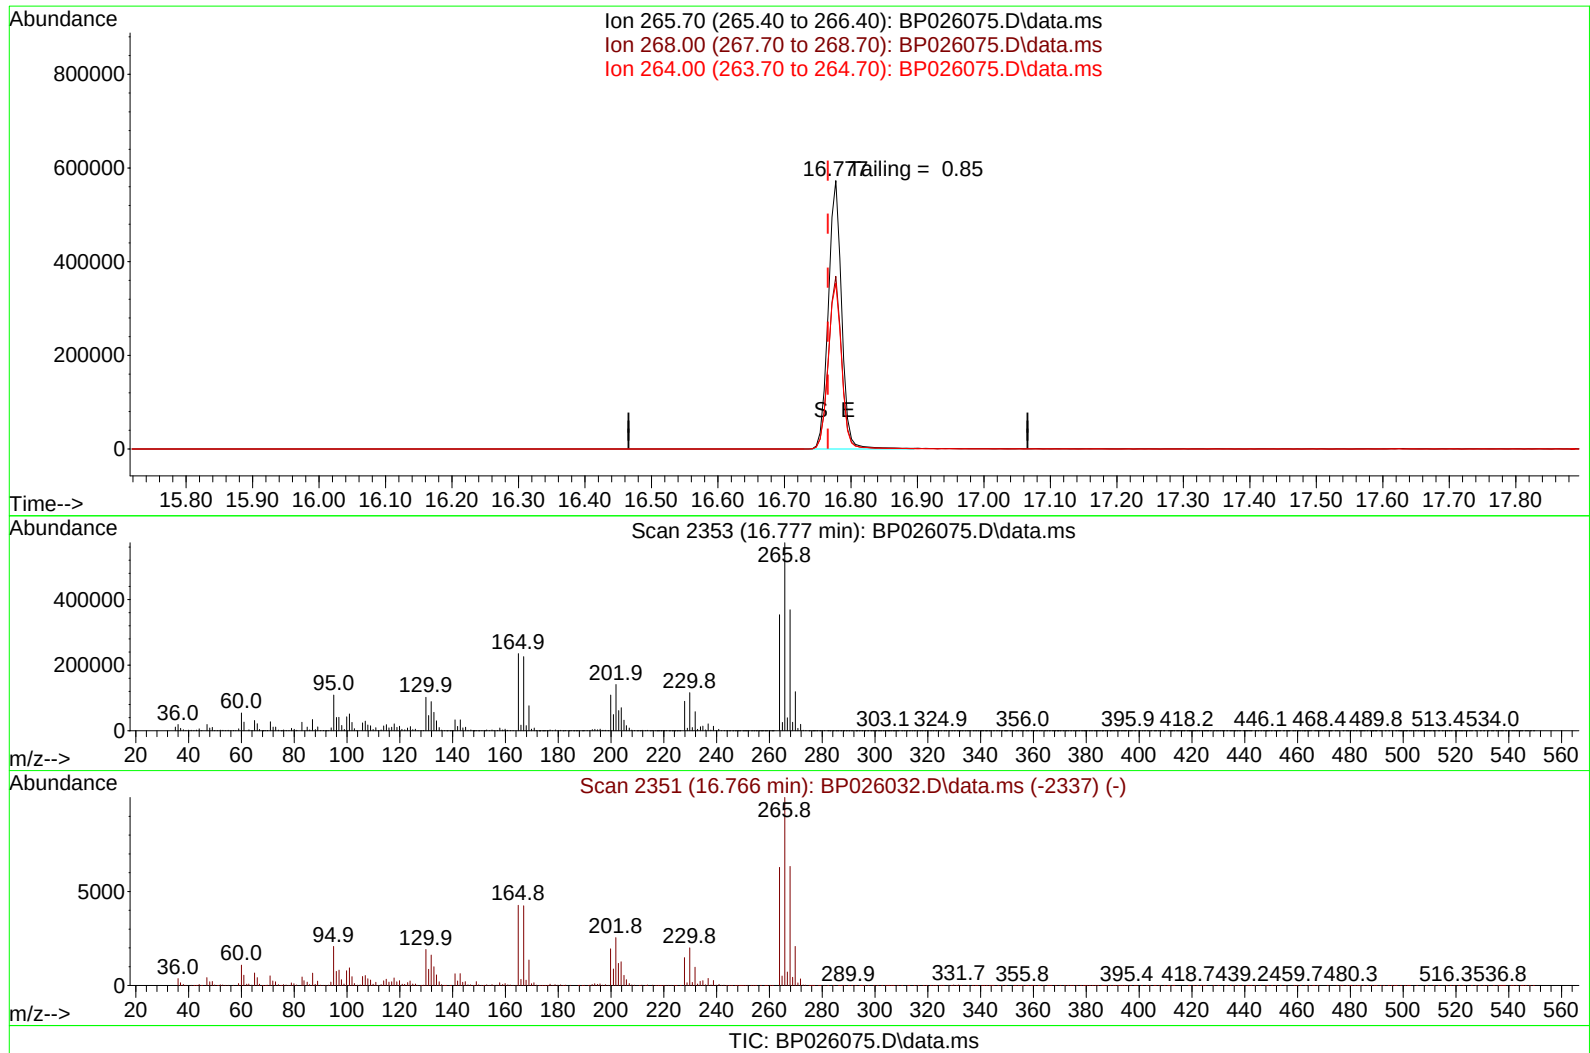


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110625\
Data File : BP026075.D
Acq On : 06 Nov 2025 12:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1




Quant Time: Nov 06 14:04:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

**(70) Pentachlorophenol (C)****16.777min (+ 0.012) 88742.13 ng****response 797426**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	64.36
264.00	62.80	61.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP110625\
Data File : BP026075.D
Acq On : 06 Nov 2025 12:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 06 14:04:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

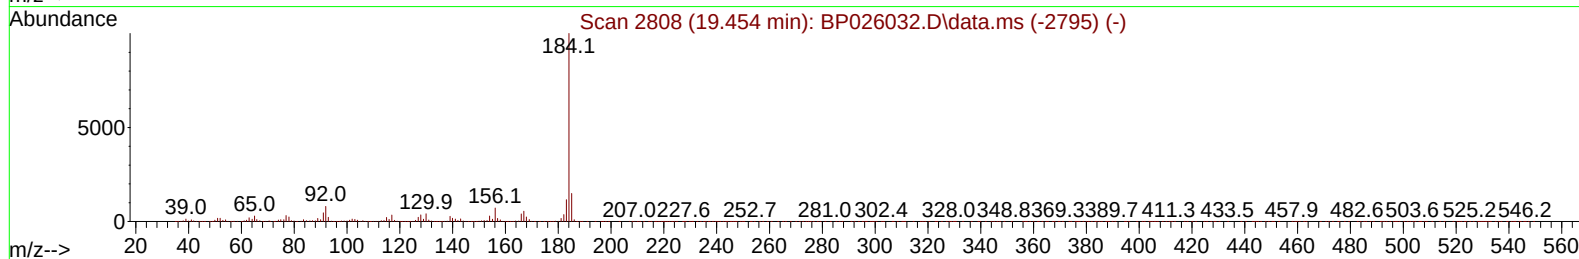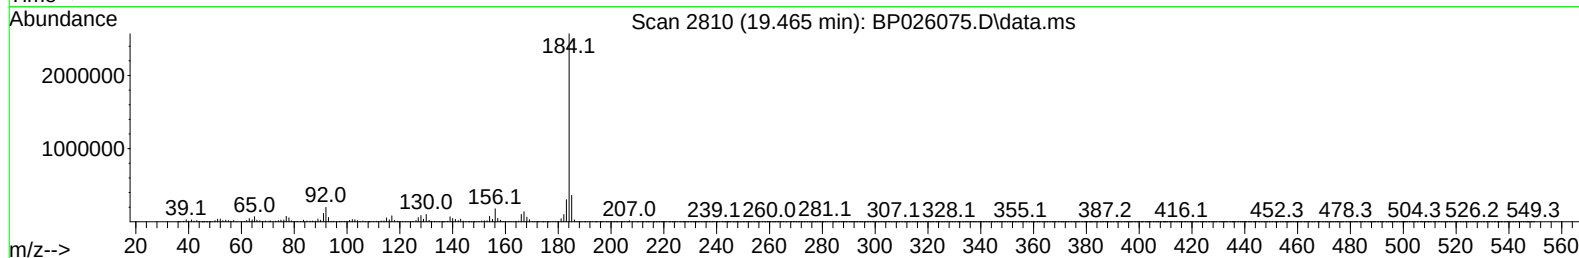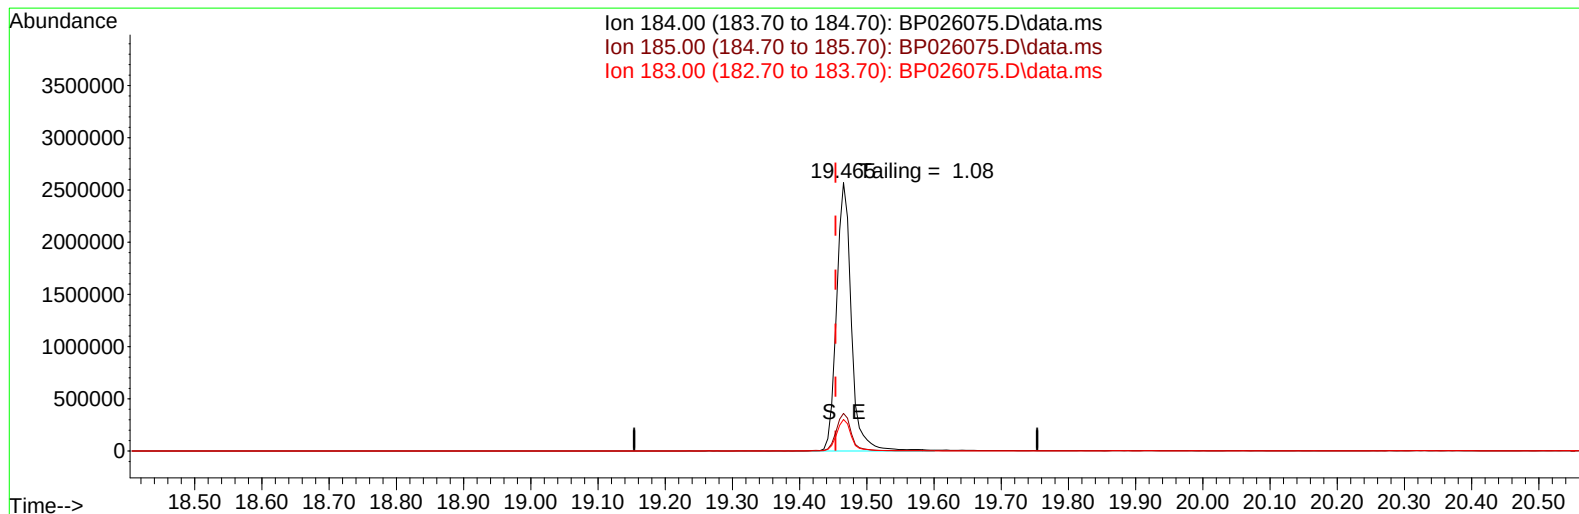

TIC: BP026075.D\data.ms

(77) Benzidine

19.465min (+ 0.012) 35734.65 ng

response 3913872

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.04
183.00	11.50	11.78
0.00	0.00	0.00