
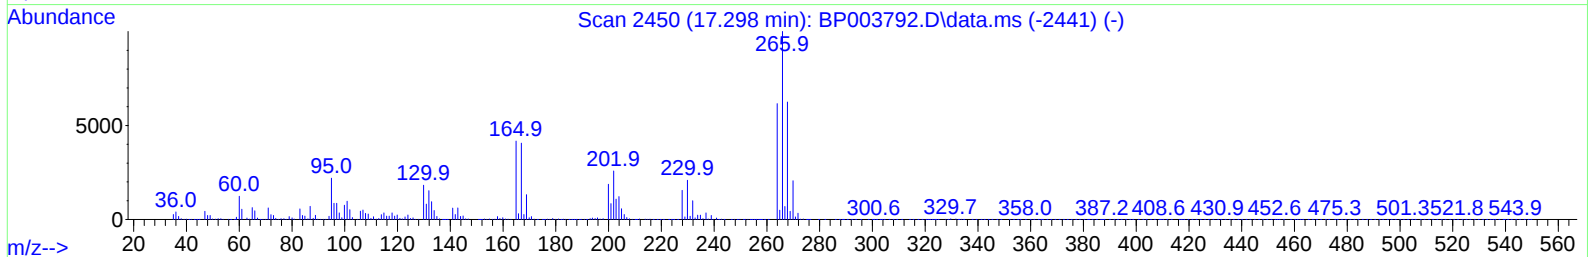
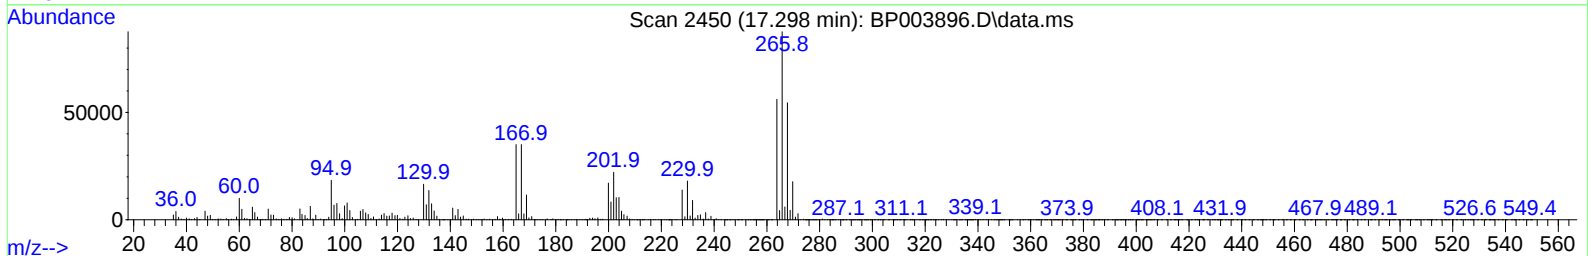


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111020\
Data File : BP003896.D
Acq On : 10 Nov 2020 11:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 03:55:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 13:41:24 2020
Response via : Initial Calibration

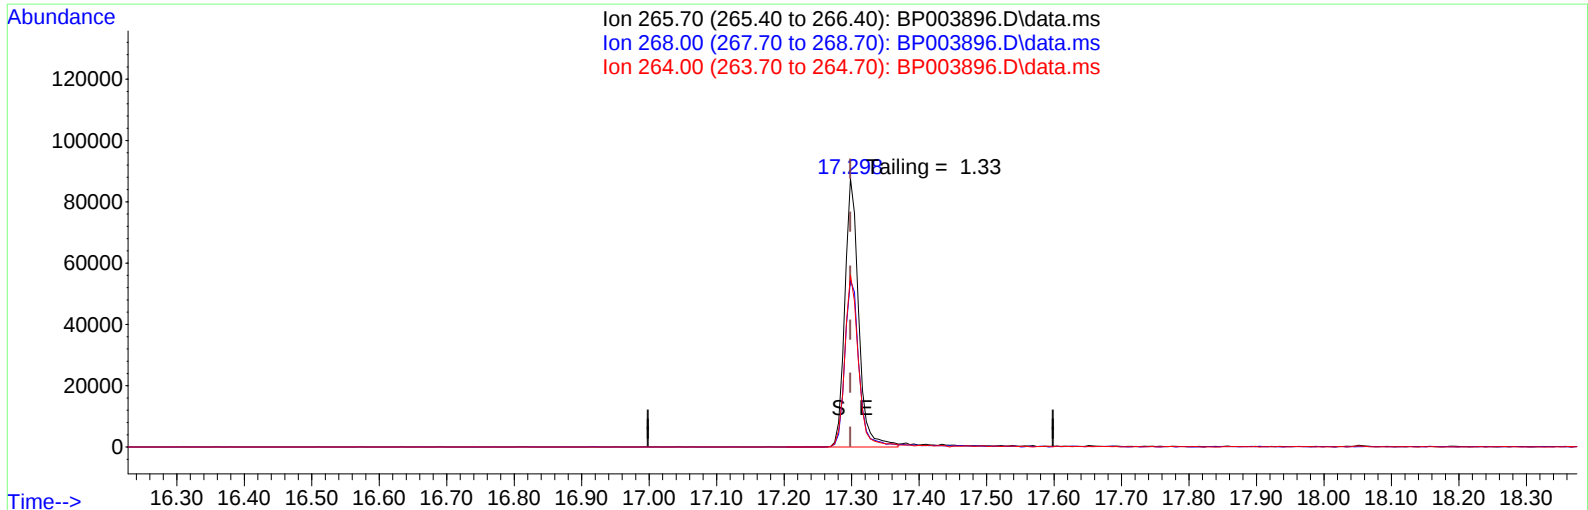

TIC: BP003896.D\data.ms

(70) Pentachlorophenol (C)




17.298min (0.000) 29967.91 ng

response 125359

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	62.21
264.00	63.30	64.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111020\
Data File : BP003896.D
Acq On : 10 Nov 2020 11:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 03:55:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 13:41:24 2020
Response via : Initial Calibration

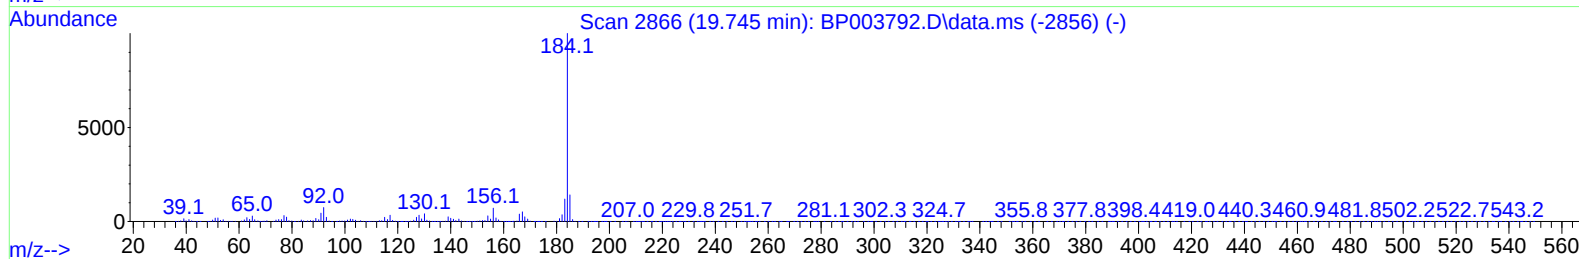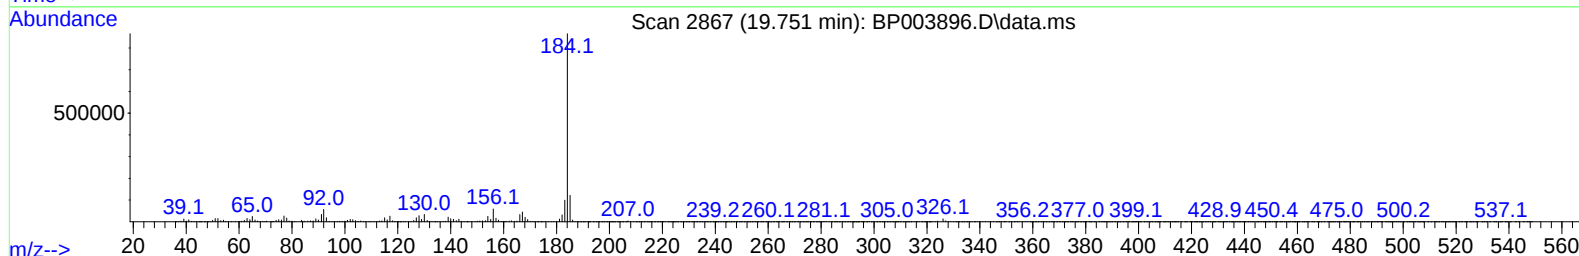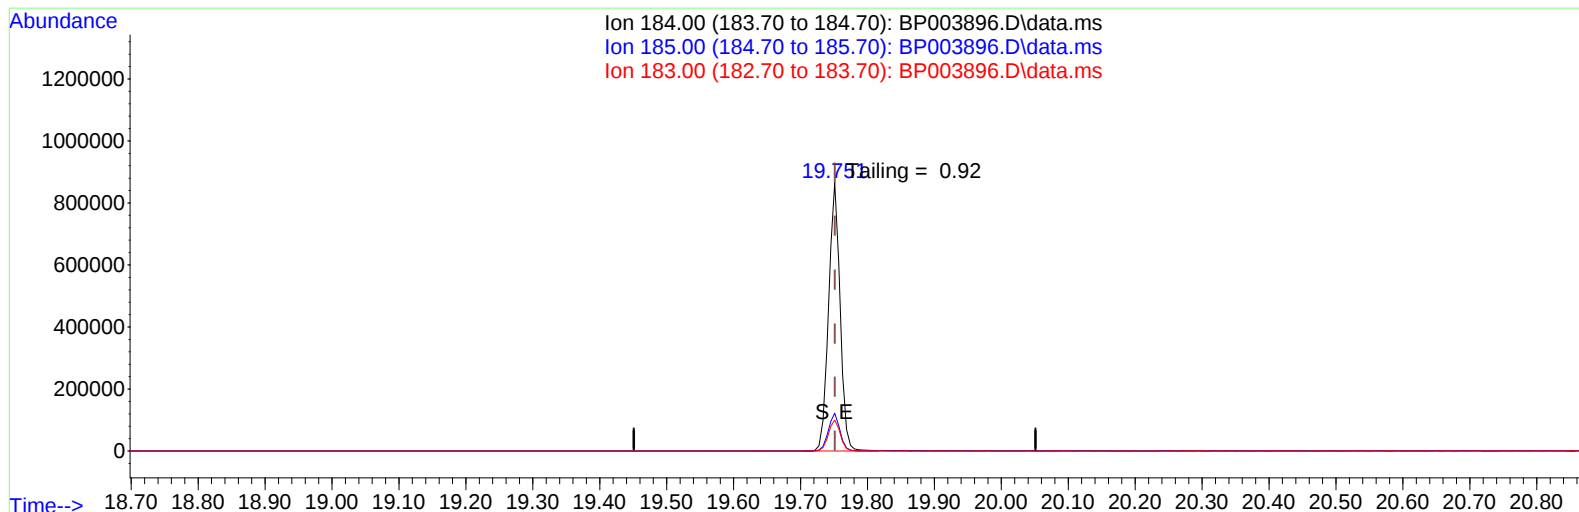

TIC: BP003896.D\data.ms

(77) Benzidine

19.751min (0.000) 48931.66 ng

response 1041070

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.08
183.00	12.00	11.52
0.00	0.00	0.00