

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111020\
Data File : BP003898.D
Acq On : 10 Nov 2020 12:38
Operator : CG/JU
Sample : PB132891BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132891BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003898.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.928	3	7	25	rVB	8913080	10040489	100.00%	20.688%
2	5.798	488	495	512	rBV	2797037	4235936	42.19%	8.728%
3	7.451	766	776	788	rBV	2669540	4302573	42.85%	8.865%
4	8.275	909	916	924	rVB	524648	837184	8.34%	1.725%
5	9.439	1105	1114	1125	rBV	1696983	2790762	27.80%	5.750%
6	11.110	1389	1398	1409	rBV	679846	1133143	11.29%	2.335%
7	13.522	1801	1808	1815	rBV	4157654	5926518	59.03%	12.212%
8	14.898	2034	2042	2050	rBV	1012683	1467383	14.61%	3.024%
9	16.380	2286	2294	2310	rBV	3074378	4473554	44.56%	9.218%
10	17.627	2499	2506	2513	rBV	1254863	1702405	16.96%	3.508%
11	20.127	2925	2931	2936	rBV	6882560	8254891	82.22%	17.009%
12	21.656	3186	3191	3197	rBV	1310468	1689053	16.82%	3.480%
13	24.127	3604	3611	3621	rVB	832945	1678204	16.71%	3.458%




Sum of corrected areas: 48532095

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111020\
Data File : BP003898.D
Acq On : 10 Nov 2020 12:38
Operator : CG/JU
Sample : PB132891BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132891BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

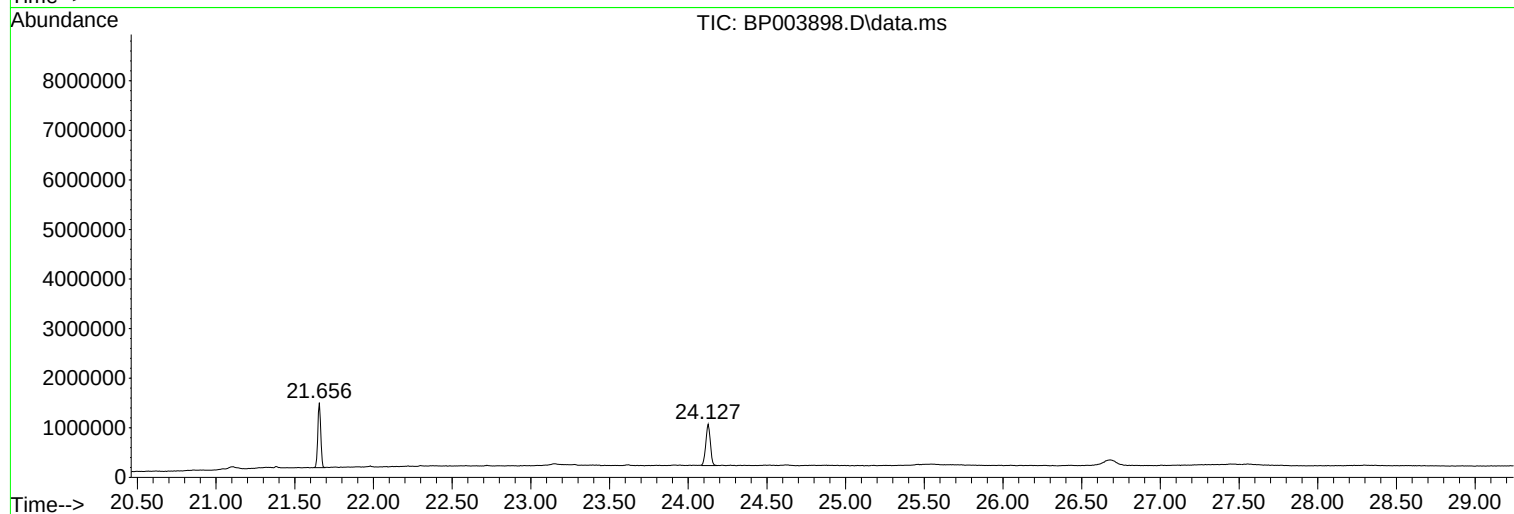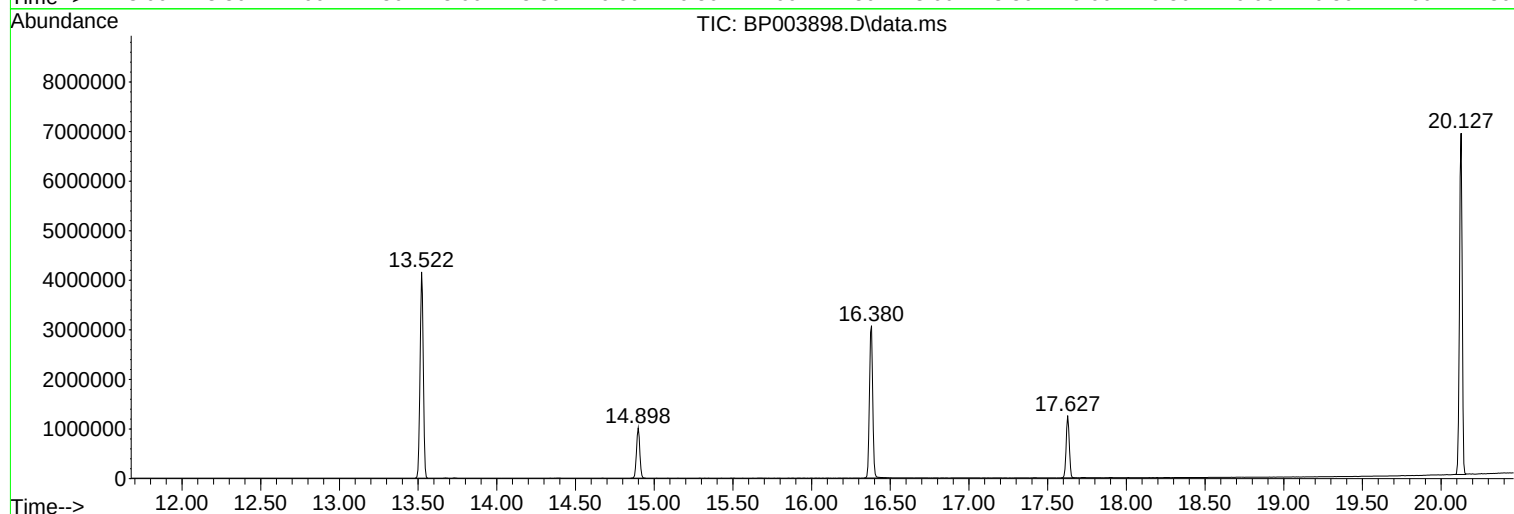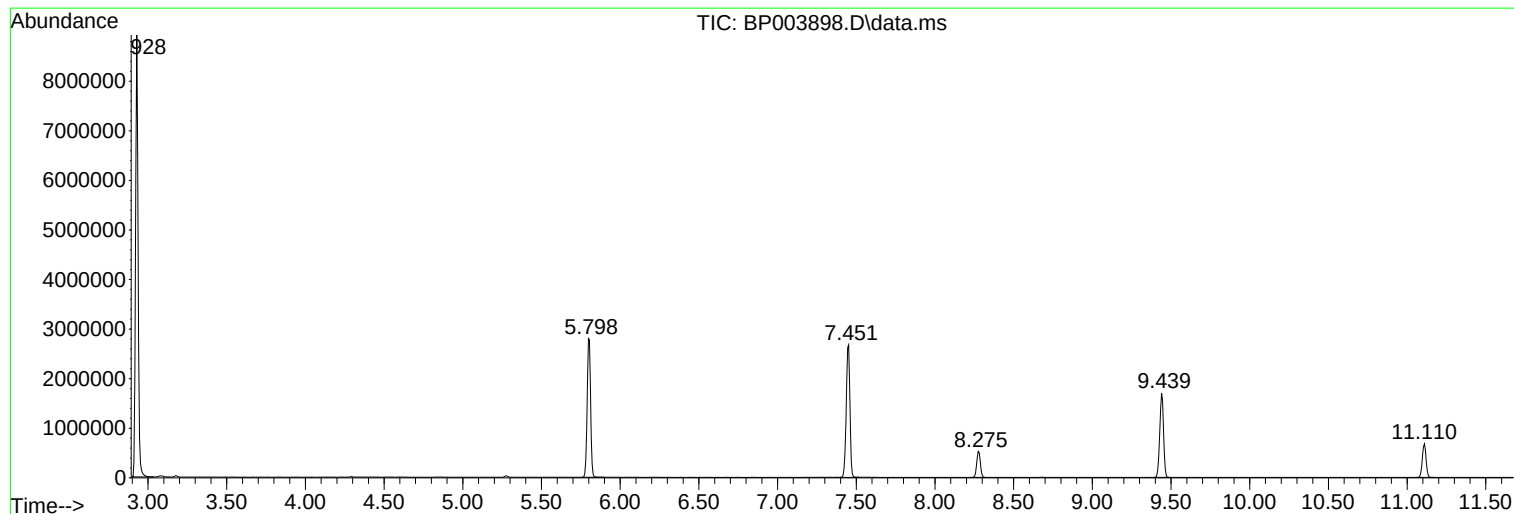

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111020\
Data File : BP003898.D
Acq On : 10 Nov 2020 12:38
Operator : CG/JU
Sample : PB132891BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132891BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111020\
Data File : BP003898.D
Acq On : 10 Nov 2020 12:38
Operator : CG/JU
Sample : PB132891BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132891BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------