

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111020\
 Data File : BP003899.D
 Acq On : 10 Nov 2020 13:12
 Operator : CG/JU
 Sample : PB132892BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB132892BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003899.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.928	3	7	27	rVB	8562273	9740774	100.00%	20.563%
2	5.799	488	495	510	rBV	2806993	4108737	42.18%	8.674%
3	7.446	767	775	786	rBV	2561898	4161951	42.73%	8.786%
4	8.275	909	916	927	rVB	523384	818059	8.40%	1.727%
5	9.440	1106	1114	1122	rBV	1665031	2701999	27.74%	5.704%
6	11.110	1389	1398	1407	rVB	650044	1091780	11.21%	2.305%
7	13.522	1801	1808	1816	rBV	4086594	5756464	59.10%	12.152%
8	14.898	2035	2042	2051	rBV	993077	1419005	14.57%	2.996%
9	16.381	2286	2294	2311	rBV	2984217	4305196	44.20%	9.089%
10	17.628	2499	2506	2518	rBV	1200117	1653501	16.98%	3.491%
11	20.127	2925	2931	2936	rBV	6808734	8216711	84.35%	17.346%
12	21.657	3186	3191	3196	rBV	1331148	1684199	17.29%	3.555%
13	24.127	3604	3611	3622	rVB	858291	1711169	17.57%	3.612%


Sum of corrected areas: 47369545

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111020\
Data File : BP003899.D
Acq On : 10 Nov 2020 13:12
Operator : CG/JU
Sample : PB132892BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132892BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

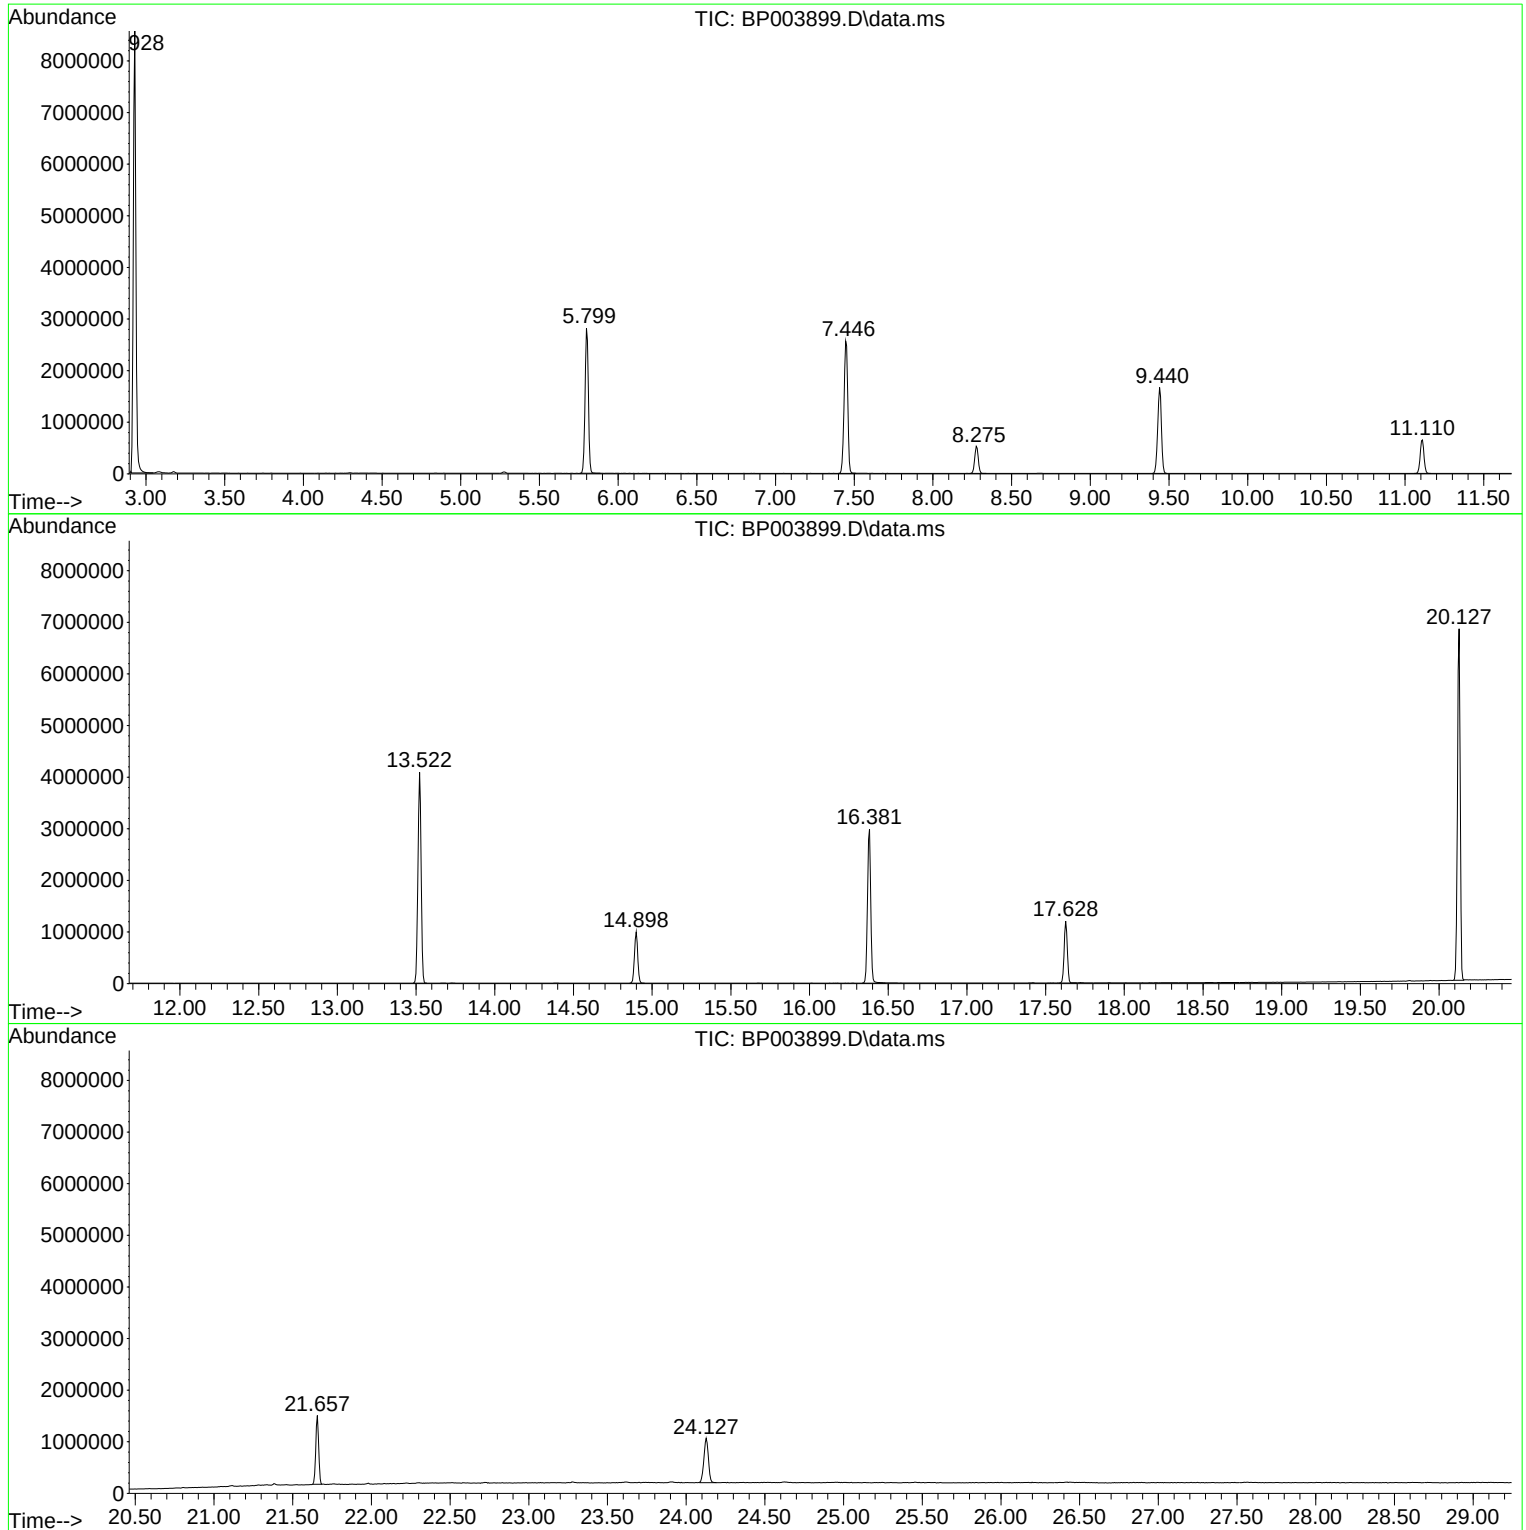

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111020\
Data File : BP003899.D
Acq On : 10 Nov 2020 13:12
Operator : CG/JU
Sample : PB132892BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132892BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111020\
Data File : BP003899.D
Acq On : 10 Nov 2020 13:12
Operator : CG/JU
Sample : PB132892BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB132892BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------