

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111020\
 Data File : BP003903.D
 Acq On : 10 Nov 2020 15:36
 Operator : CG/JU
 Sample : L4668-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MW-16

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP003903.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.087	27	34	44	rBV	212525	434000	6.17%	1.270%
2	3.181	44	50	65	rVB	1085829	1415560	20.12%	4.142%
3	5.805	488	496	505	rBV	1133998	1713892	24.36%	5.015%
4	7.446	767	775	785	rBV	725332	1149975	16.35%	3.365%
5	8.275	907	916	924	rBV	562056	908945	12.92%	2.660%
6	9.440	1106	1114	1122	rBV	1872276	3010718	42.79%	8.809%
7	11.110	1390	1398	1406	rBV	675300	1159367	16.48%	3.392%
8	13.522	1801	1808	1815	rBV	4274919	6039794	85.85%	17.672%
9	14.322	1939	1944	1949	rVB	163731	227390	3.23%	0.665%
10	14.898	2036	2042	2049	rVB	937082	1372973	19.52%	4.017%
11	16.381	2287	2294	2304	rBV	3070650	4402642	62.58%	12.882%
12	17.628	2501	2506	2513	rVB	1087521	1476127	20.98%	4.319%
13	18.469	2646	2649	2657	rBV	132655	217698	3.09%	0.637%
14	20.127	2926	2931	2936	rVB	5853998	7035341	100.00%	20.585%
15	21.316	3129	3133	3142	rVB	285802	379499	5.39%	1.110%
16	21.657	3186	3191	3196	rBV	1247655	1627690	23.14%	4.763%
17	24.133	3606	3612	3621	rBV	796521	1605220	22.82%	4.697%




Sum of corrected areas: 34176831

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111020\
Data File : BP003903.D
Acq On : 10 Nov 2020 15:36
Operator : CG/JU
Sample : L4668-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW-16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

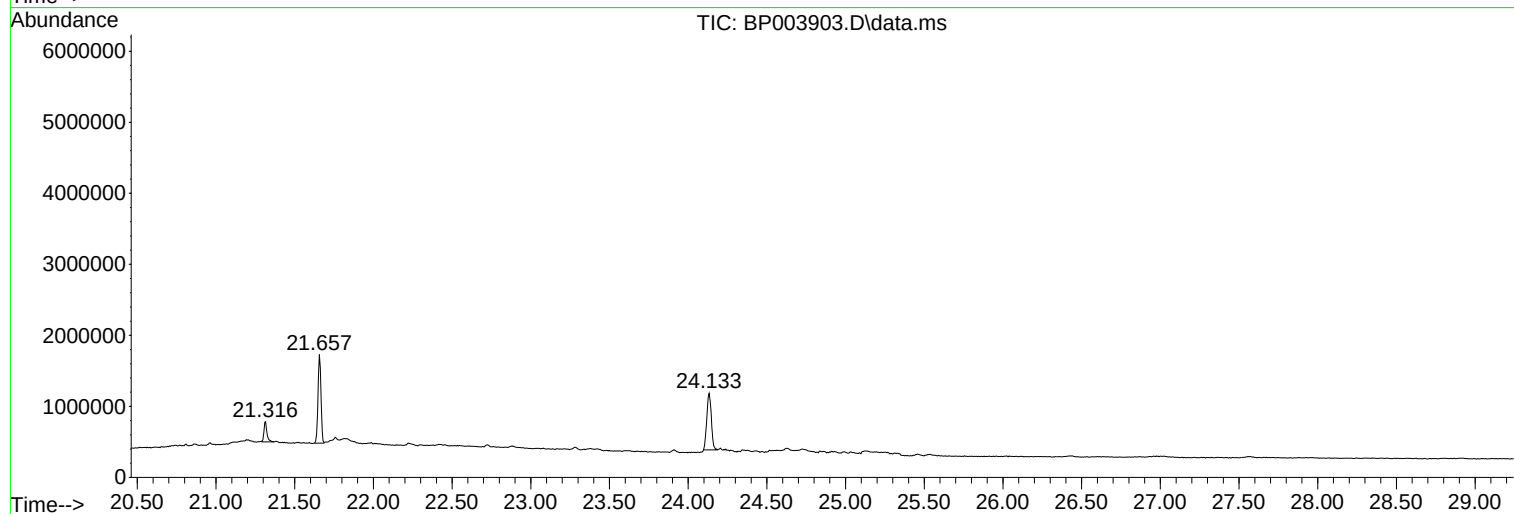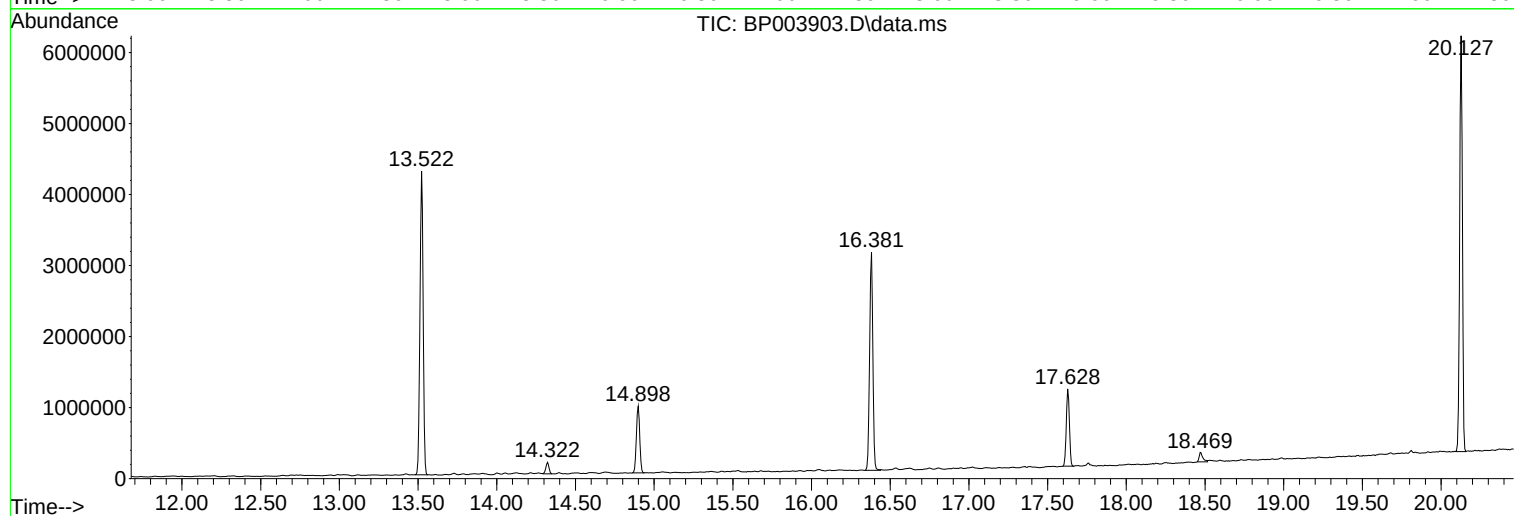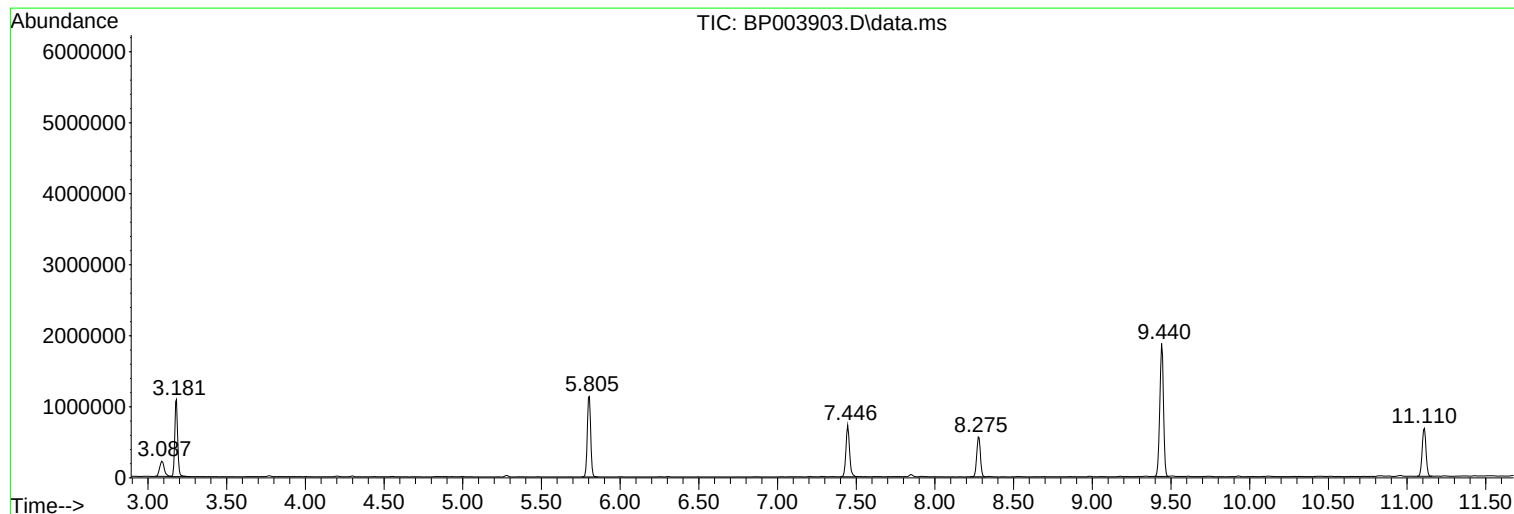

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111020\
Data File : BP003903.D
Acq On : 10 Nov 2020 15:36
Operator : CG/JU
Sample : L4668-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW-16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111020\
Data File : BP003903.D
Acq On : 10 Nov 2020 15:36
Operator : CG/JU
Sample : L4668-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW-16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
