
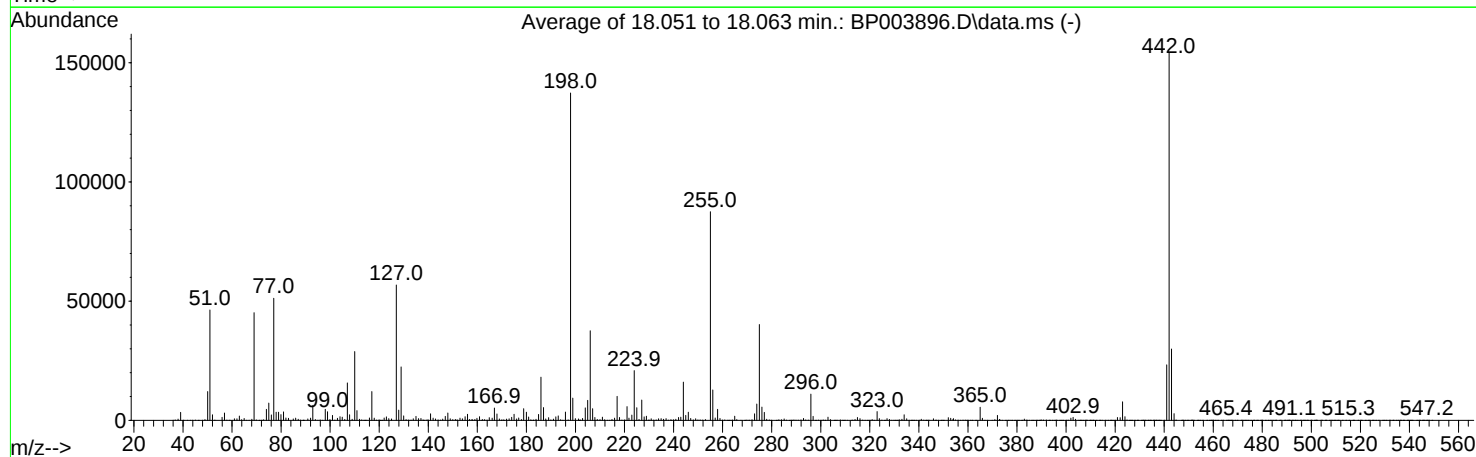


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111020\
 Data File : BP003896.D
 Acq On : 10 Nov 2020 11:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP110320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 10 13:41:24 2020

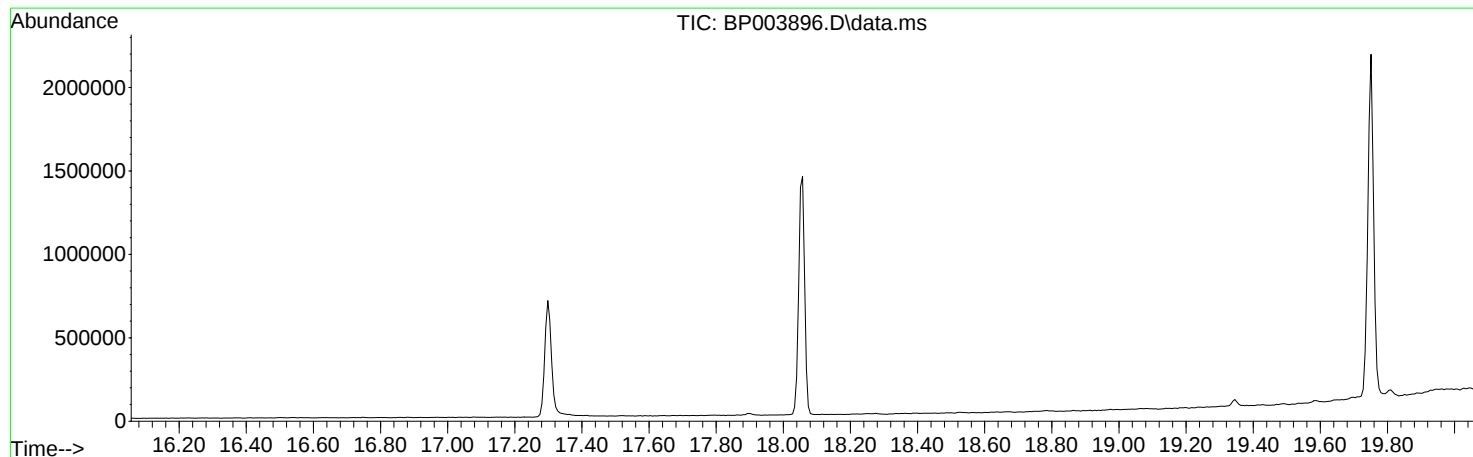

AutoFind: Scans 2578, 2579, 2580; Background Corrected with Scan 2571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	46304	PASS
68	69	0.00	2	1.1	492	PASS
69	198	0.00	100	32.9	45192	PASS
70	69	0.00	2	0.5	239	PASS
127	198	10	80	41.4	56804	PASS
197	198	0.00	2	0.2	221	PASS
198	198	100	100	100.0	137306	PASS
199	198	5	9	6.8	9341	PASS
275	198	10	60	29.3	40195	PASS
365	198	1	100	4.0	5474	PASS
441	198	0.01	100	17.0	23279	PASS
442	442	100	100	100.0	154281	PASS
443	442	15	24	19.4	29941	PASS