
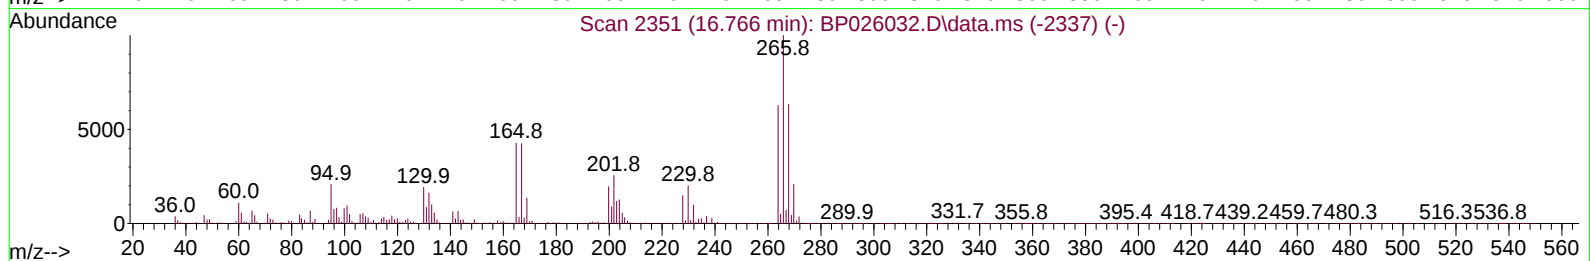
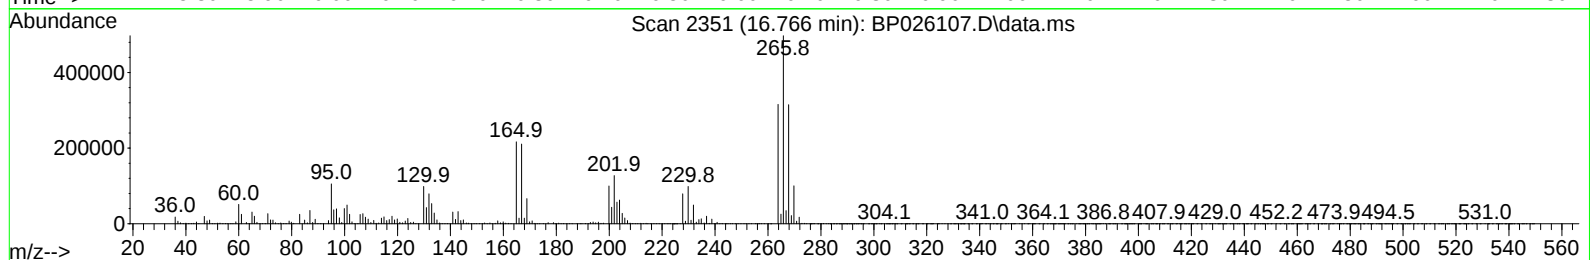


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111225\
Data File : BP026107.D
Acq On : 12 Nov 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 11:18:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

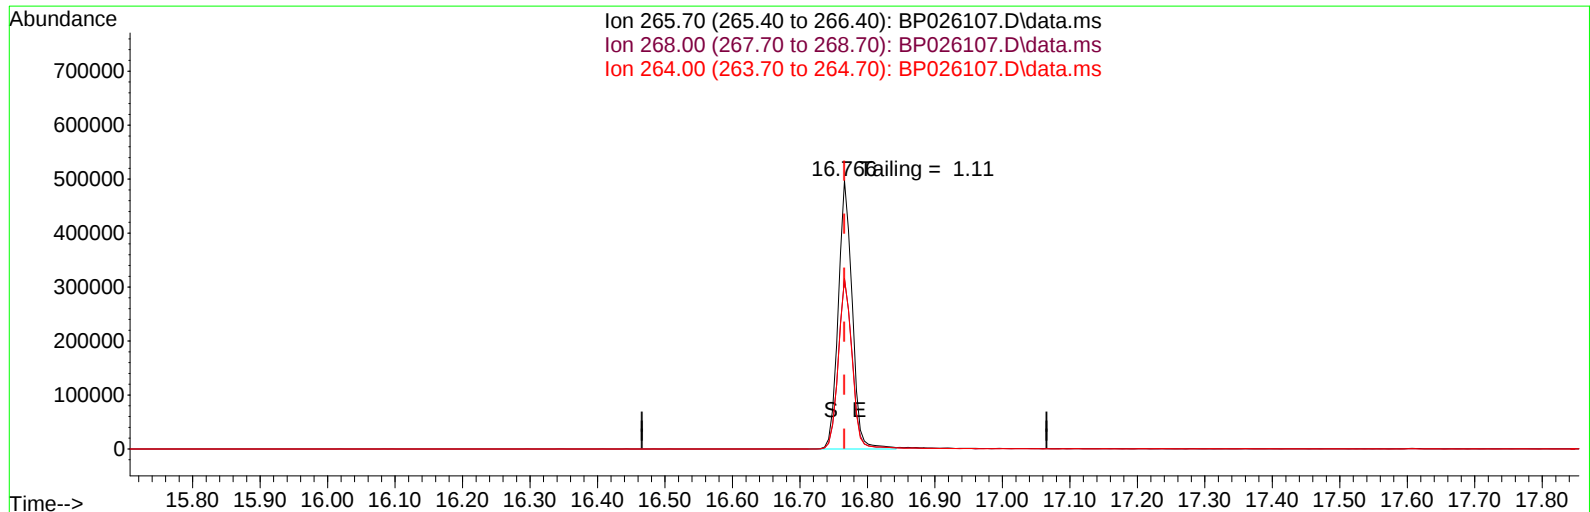

TIC: BP026107.D\data.ms

(70) Pentachlorophenol (C)




16.766min (+ 0.000) 116733.38 ng

response 714908

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	63.29
264.00	62.80	63.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111225\
Data File : BP026107.D
Acq On : 12 Nov 2025 10:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 11:18:07 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP102925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 30 11:51:34 2025
Response via : Initial Calibration

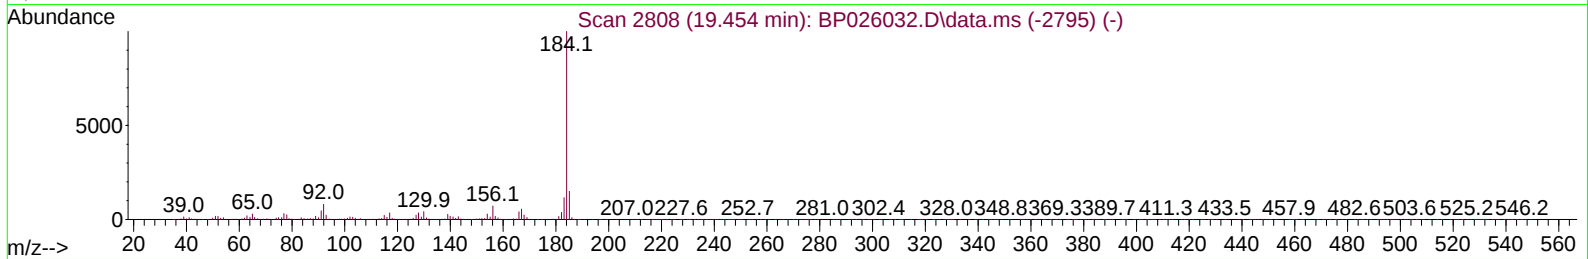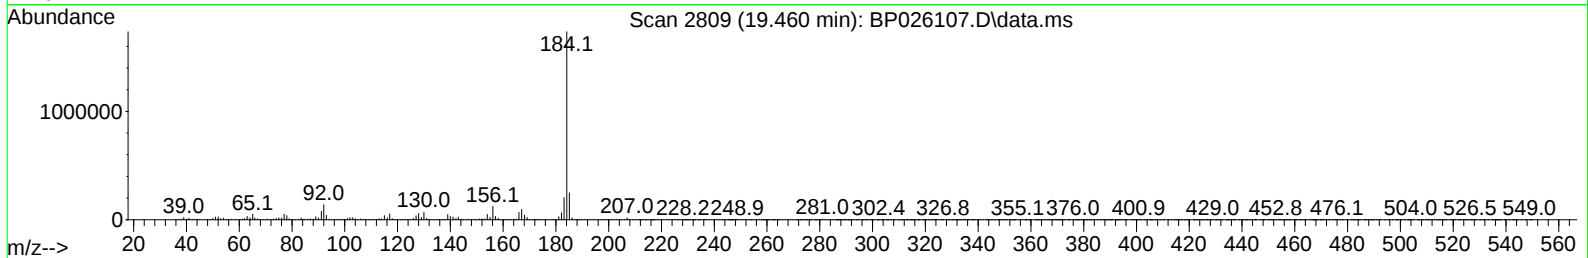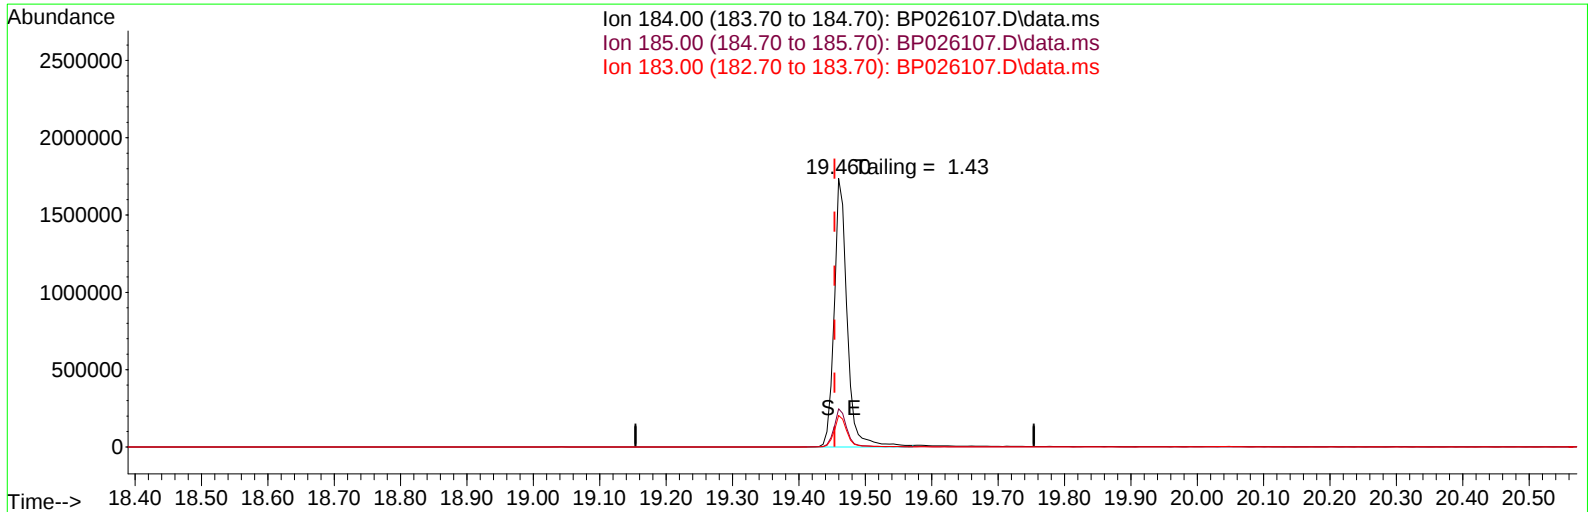

TIC: BP026107.D\data.ms

(77) Benzidine

19.460min (+ 0.006) 27750.80 ng

response 2359699

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.25
183.00	11.50	11.71
0.00	0.00	0.00