




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023102.D
Acq On : 14 Nov 2024 10:59
Operator : RC/JU
Sample : P4724-19
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9D2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 14 22:58:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

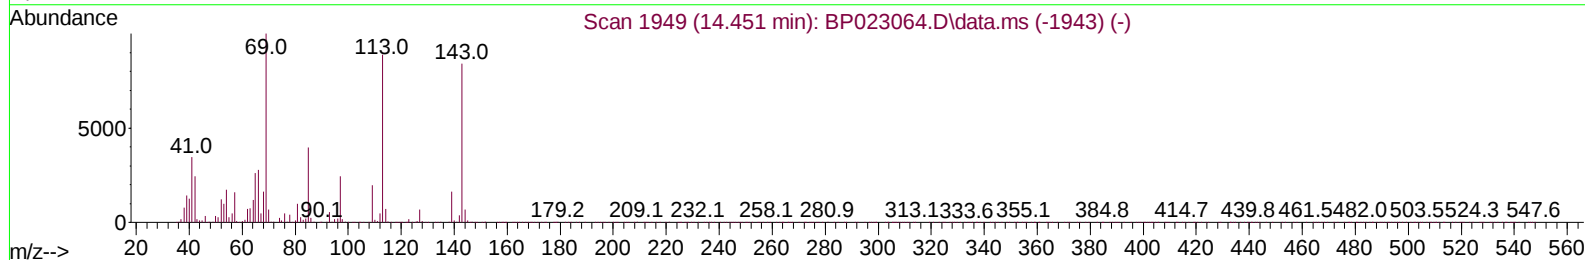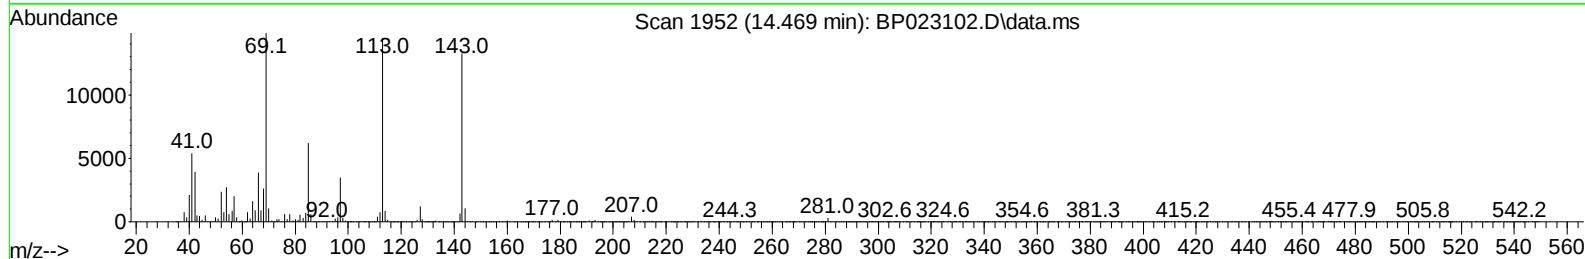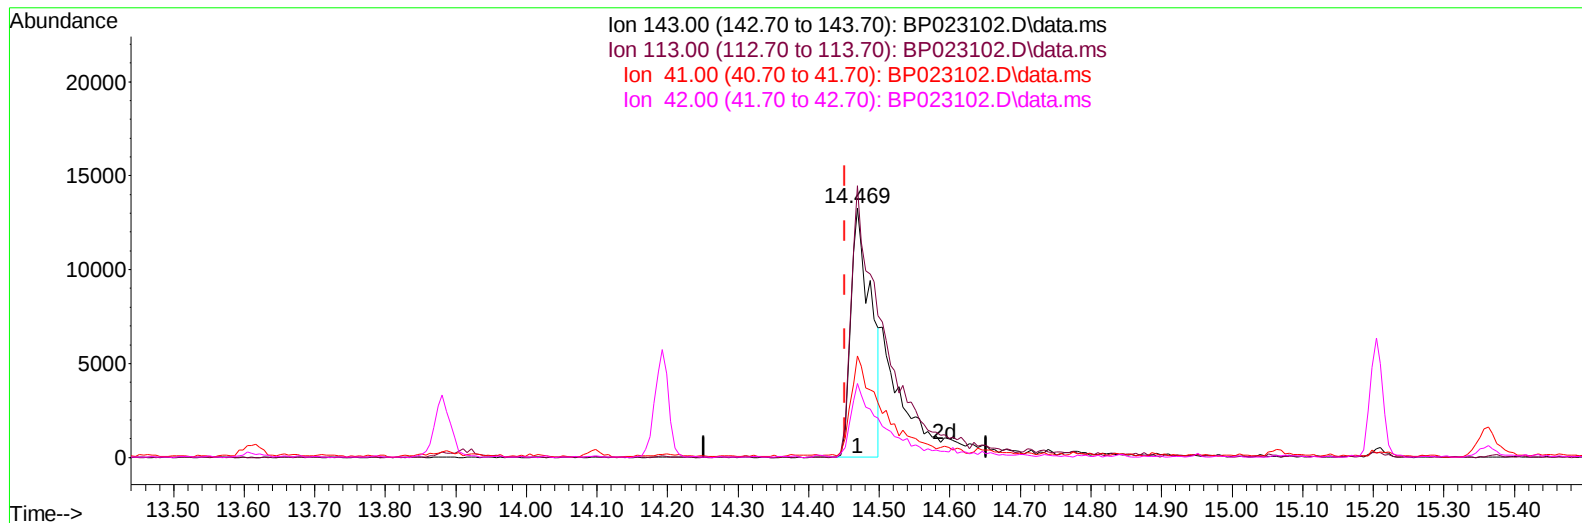

TIC: BP023102.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.469min (+ 0.018) 9.75 ng/u1

response 26244

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	108.83
41.00	39.20	40.80
42.00	25.90	29.61




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023102.D
Acq On : 14 Nov 2024 10:59
Operator : RC/JU
Sample : P4724-19
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9D2

Manual IntegrationsAPPROVED

Quant Time: Nov 14 22:58:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

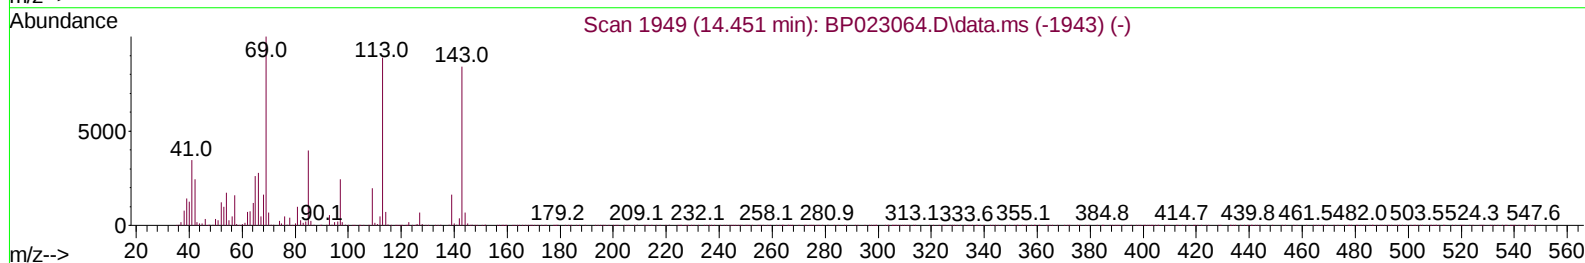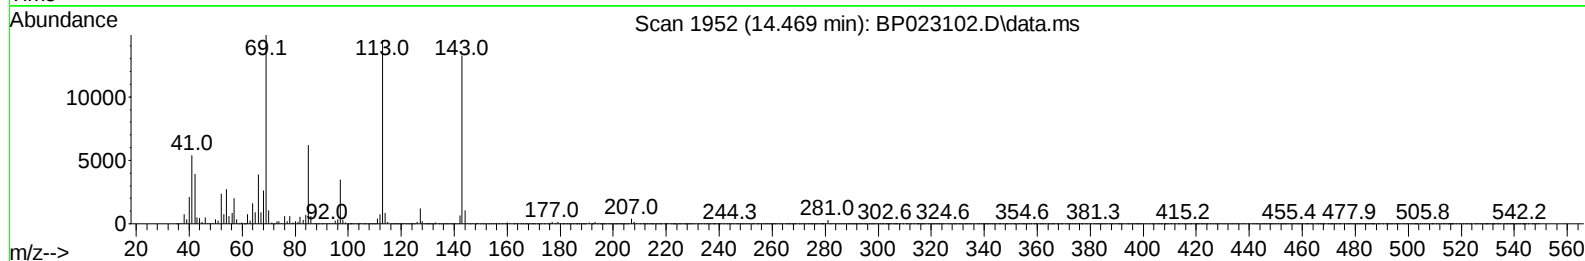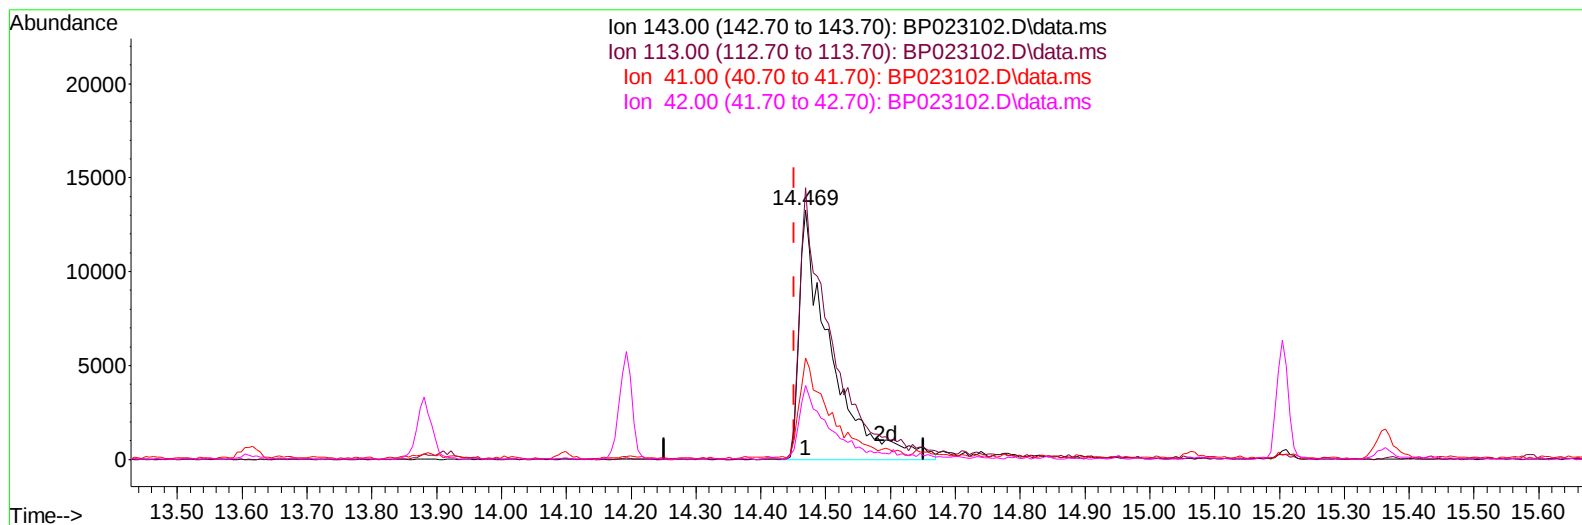

TIC: BP023102.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.469min (+ 0.018) 16.39 ng/ul m

response 44122

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	108.83
41.00	39.20	40.80
42.00	25.90	29.61

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023102.D
 Acq On : 14 Nov 2024 10:59
 Operator : RC/JU
 Sample : P4724-19
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH9D2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 14 22:58:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.575	152	78959	20.000	ng/ul	0.00
20) Naphthalene-d8	10.328	136	304092	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.193	164	248480	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.004	188	631583	20.000	ng/ul	-0.01
79) Chrysene-d12	21.445	240	711180	20.000	ng/ul	0.00
88) Perylene-d12	24.663	264	853294	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	5287	3.219	ng/uL	0.00
4) Pyridine-d5	3.552	84	65884	13.500	ng/ul	0.00
7) Phenol-d5	6.787	99	99405	17.028	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.928	67	61229	17.852	ng/ul	0.00
11) 2-Chlorophenol-d4	7.128	132	74610	17.451	ng/ul	0.00
15) 4-Methylphenol-d8	8.293	113	83862	17.457	ng/ul	0.00
21) Nitrobenzene-d5	8.728	128	38452	18.163	ng/ul	0.00
24) 2-Nitrophenol-d4	9.440	143	46609	18.467	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.975	165	93986	17.782	ng/ul	0.00
31) 4-Chloroaniline-d4	10.487	131	112497	17.841	ng/ul	0.00
46) Dimethylphthalate-d6	13.616	166	370553	20.691	ng/ul	0.00
49) Acenaphthylene-d8	13.881	160	378821	20.273	ng/ul	-0.02
54) 4-Nitrophenol-d4	14.469	143	44122m	16.394	ng/ul	0.02
60) Fluorene-d10	15.204	176	336214	21.413	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.363	200	47801	12.634	ng/ul	0.00
73) Anthracene-d10	17.098	188	572945	21.425	ng/ul	-0.02
81) Pyrene-d10	19.498	212	736412	22.481	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.439	264	902560	22.206	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023102.D
Acq On : 14 Nov 2024 10:59
Operator : RC/JU
Sample : P4724-19
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH9D2

Manual IntegrationsAPPROVED

Quant Time: Nov 14 22:58:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

