




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023111.D
Acq On : 14 Nov 2024 18:26
Operator : RC/JU
Sample : P4803-07DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 14 23:46:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

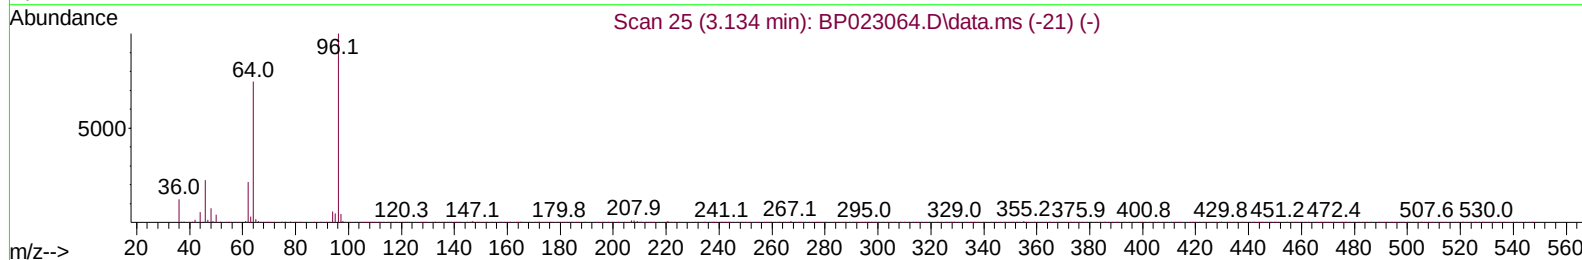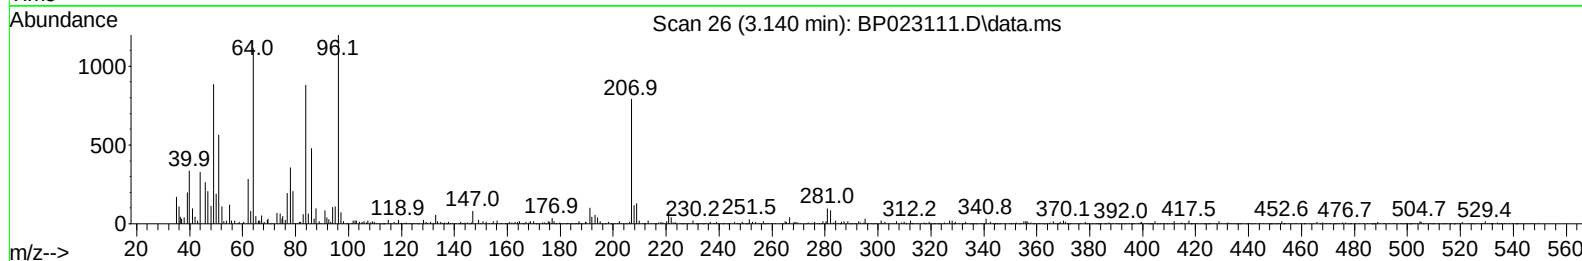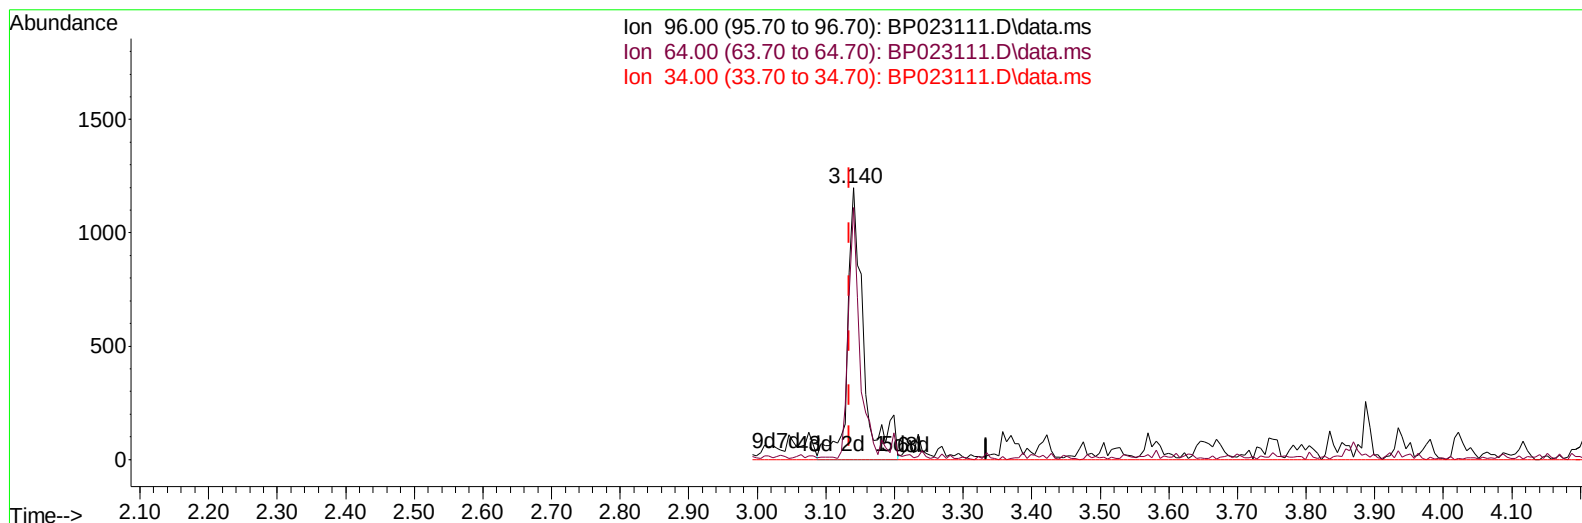

TIC: BP023111.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.140min (+ 0.006) 1.70 ng/uL m

response 1949

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	67.80	92.82#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023111.D
Acq On : 14 Nov 2024 18:26
Operator : RC/JU
Sample : P4803-07DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 14 23:46:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

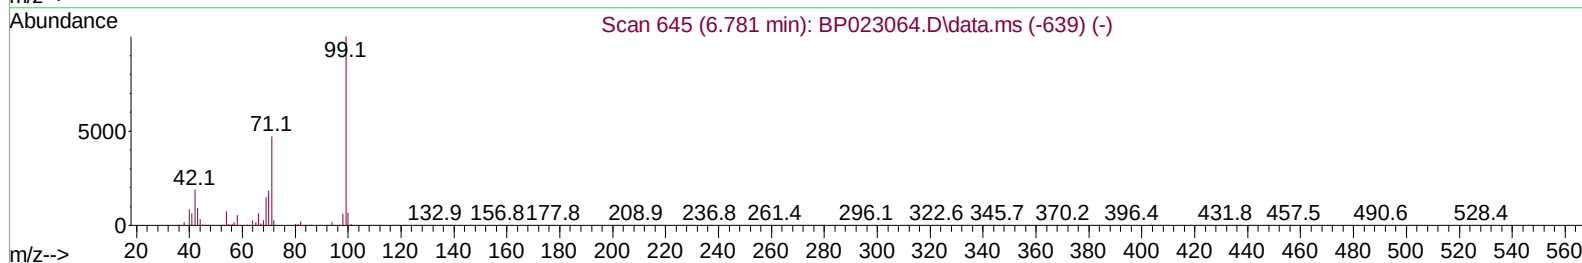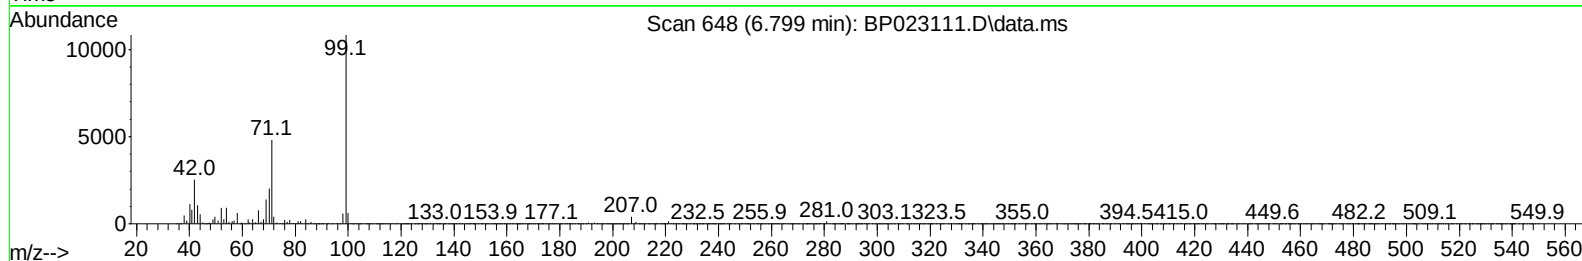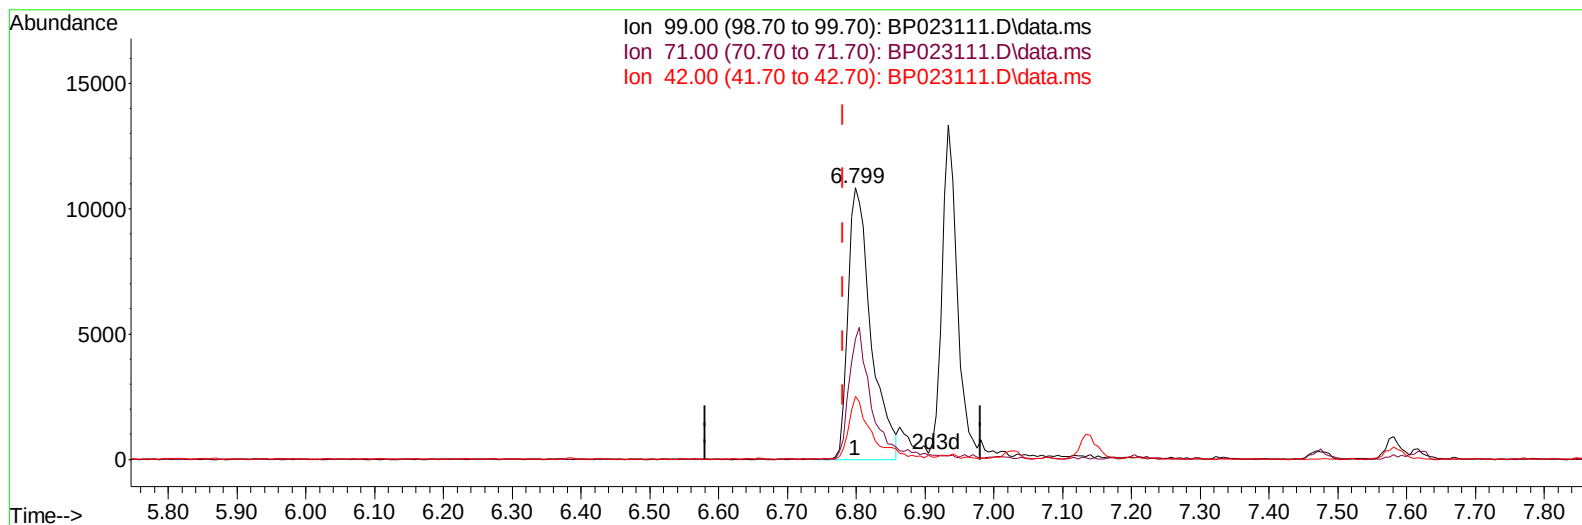

TIC: BP023111.D\data.ms

(7) Phenol-d5 (S)

6.799min (+ 0.018) 6.18 ng/u1

response 25172

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	44.70	44.35
42.00	21.10	23.24
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023111.D
Acq On : 14 Nov 2024 18:26
Operator : RC/JU
Sample : P4803-07DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 14 23:46:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

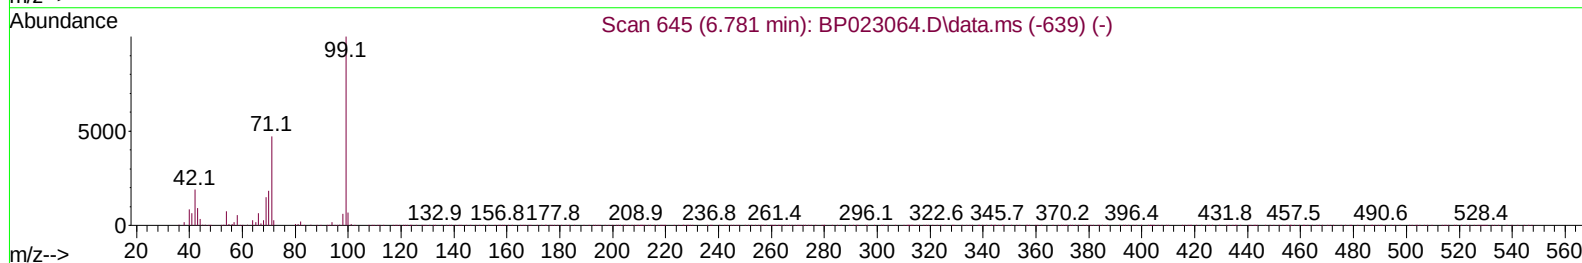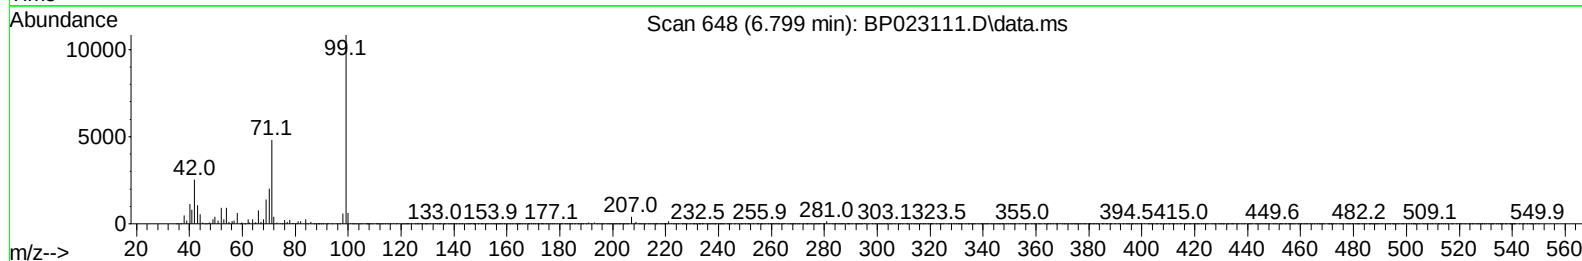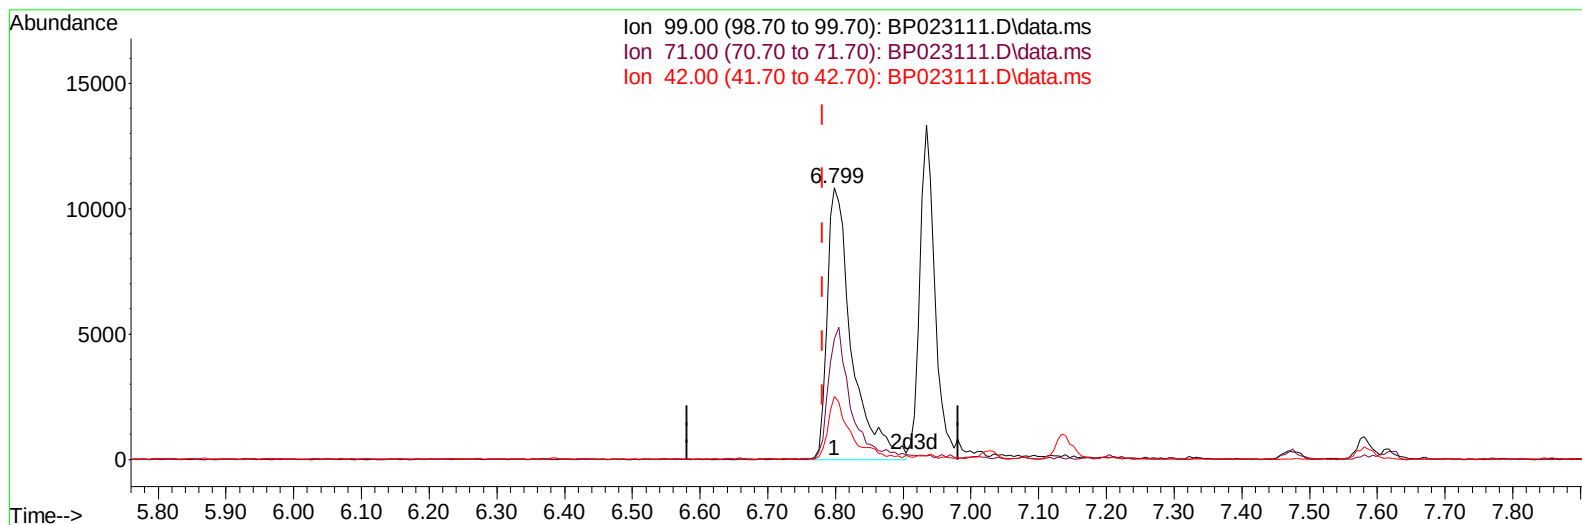

TIC: BP023111.D\data.ms

(7) Phenol-d5 (S)

6.799min (+ 0.018) 6.65 ng/ul m

response 27089

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	44.70	44.35
42.00	21.10	23.24
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023111.D
Acq On : 14 Nov 2024 18:26
Operator : RC/JU
Sample : P4803-07DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 14 23:46:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

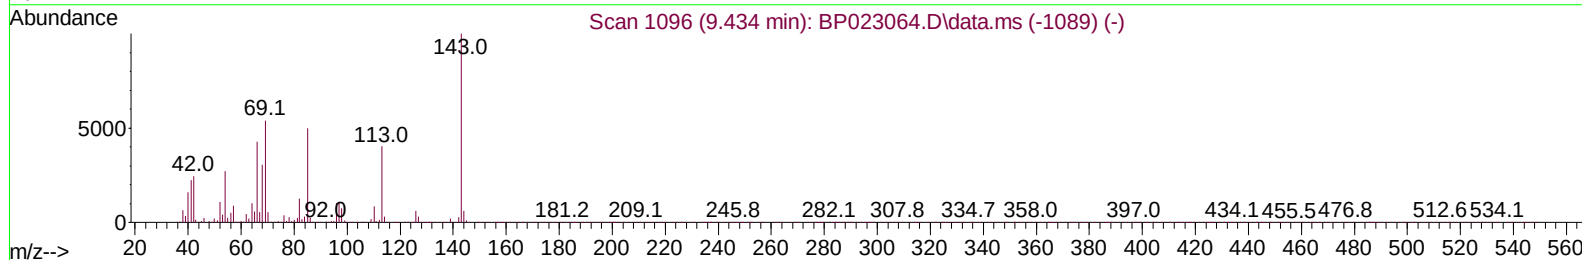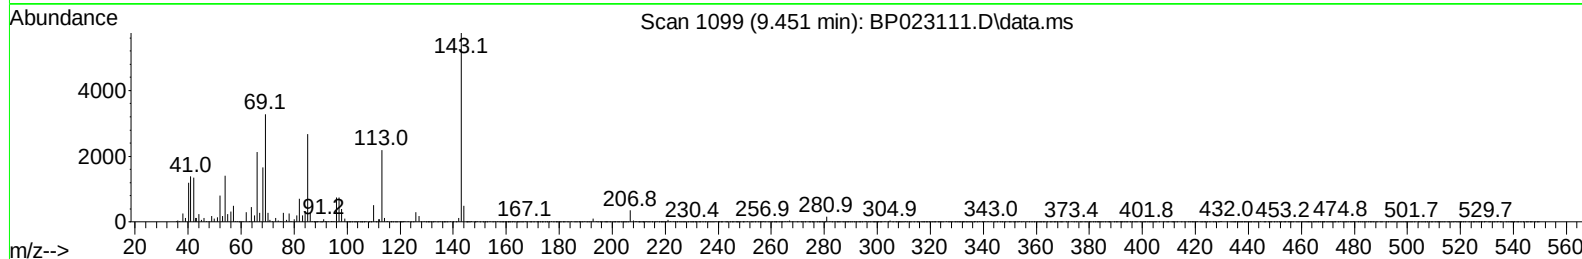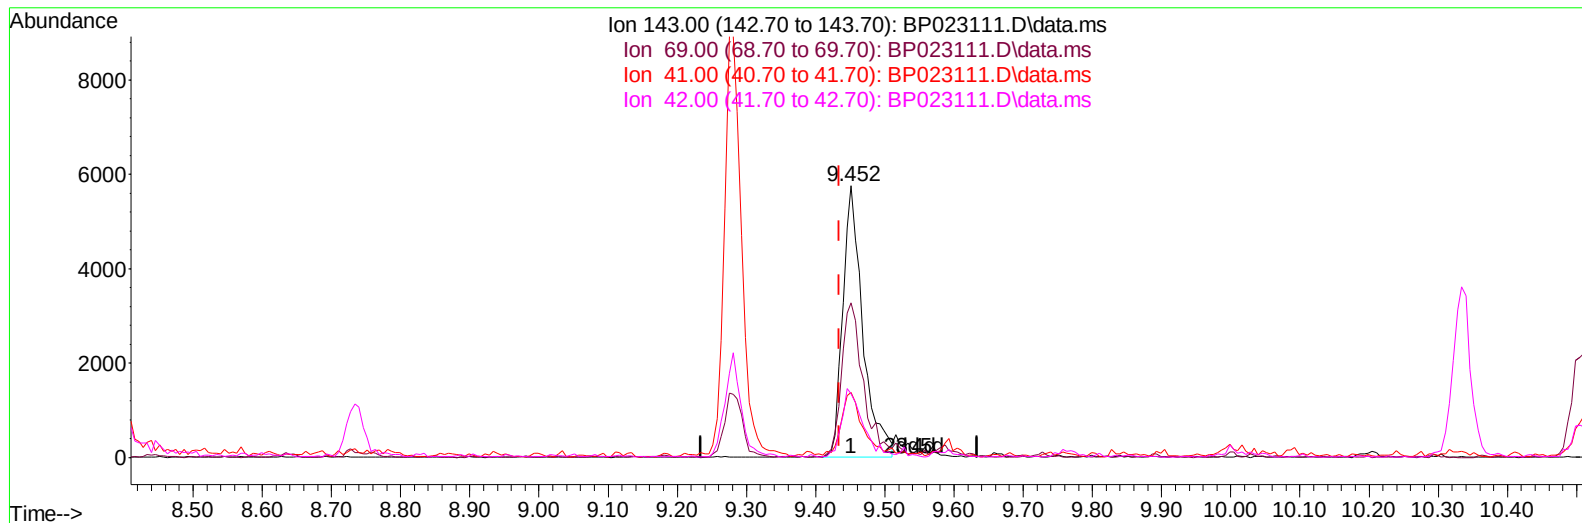

TIC: BP023111.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.451min (+ 0.018) 6.67 ng/uL

response 11518

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	66.00	56.96
41.00	25.10	24.00
42.00	27.40	23.39




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023111.D
Acq On : 14 Nov 2024 18:26
Operator : RC/JU
Sample : P4803-07DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 14 23:46:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

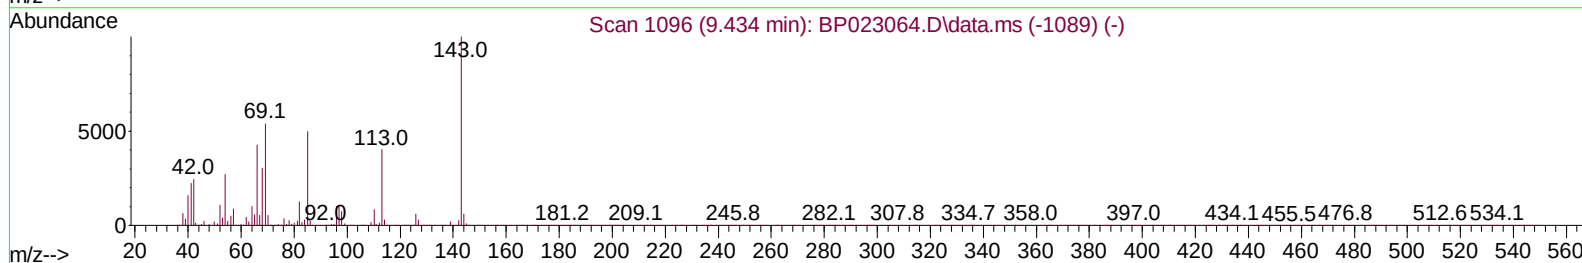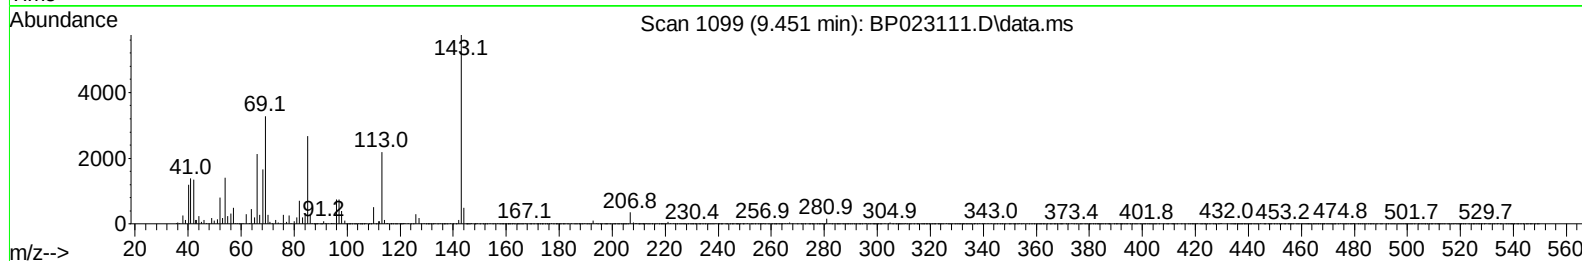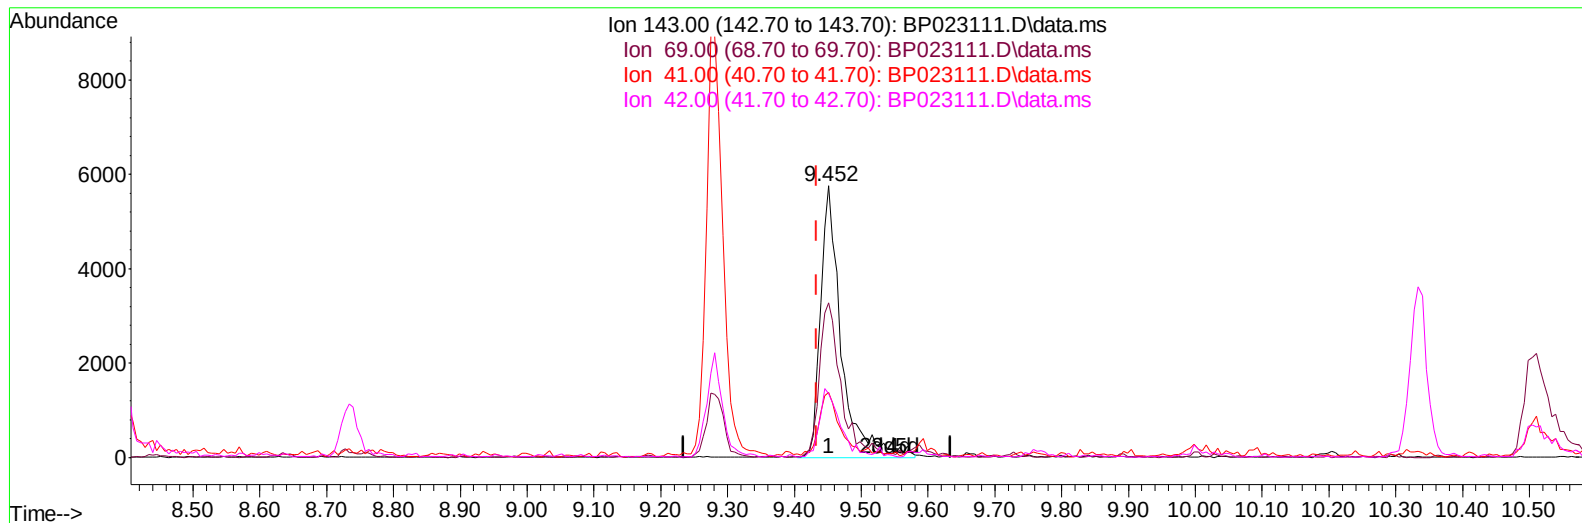

TIC: BP023111.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.451min (+ 0.018) 7.18 ng/ul m

response 12387

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	66.00	56.96
41.00	25.10	24.00
42.00	27.40	23.39




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023111.D
Acq On : 14 Nov 2024 18:26
Operator : RC/JU
Sample : P4803-07DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 14 23:46:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

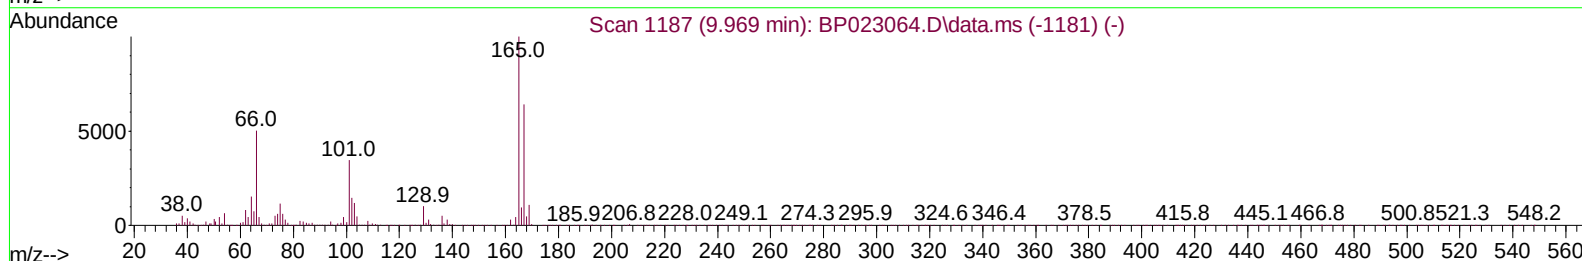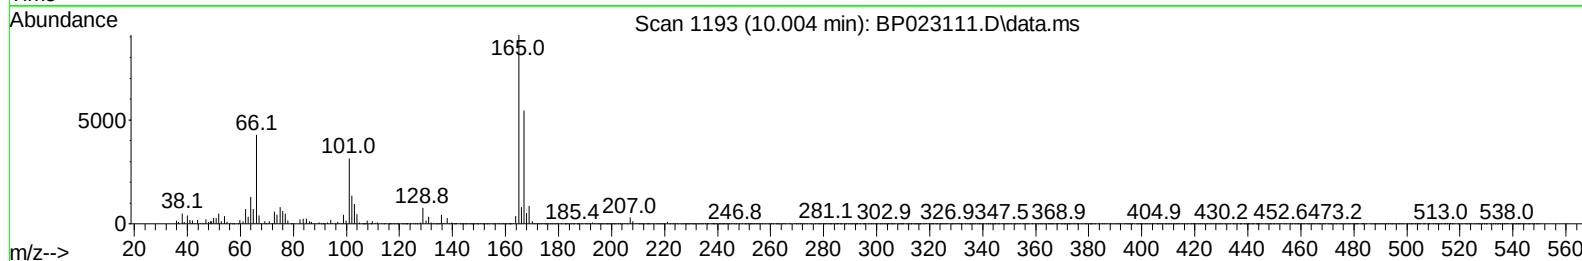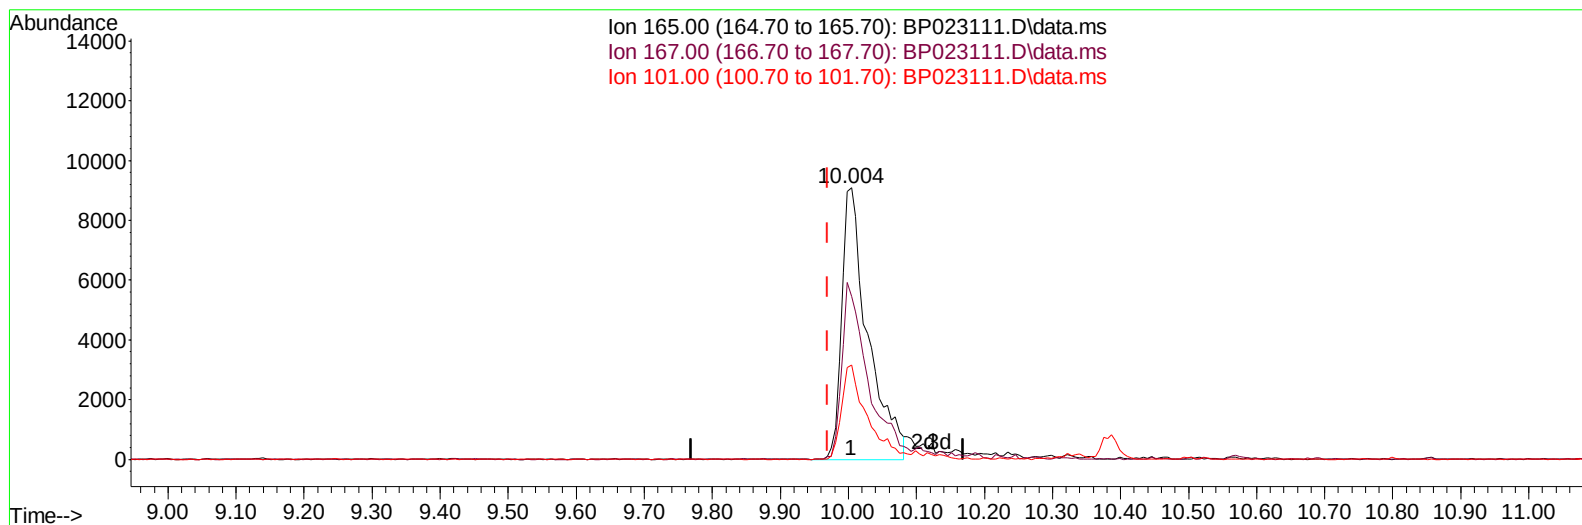

TIC: BP023111.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.004min (+ 0.035) 6.70 ng/ul

response 24223

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.80	60.05
101.00	32.60	34.70
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023111.D
Acq On : 14 Nov 2024 18:26
Operator : RC/JU
Sample : P4803-07DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 14 23:46:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

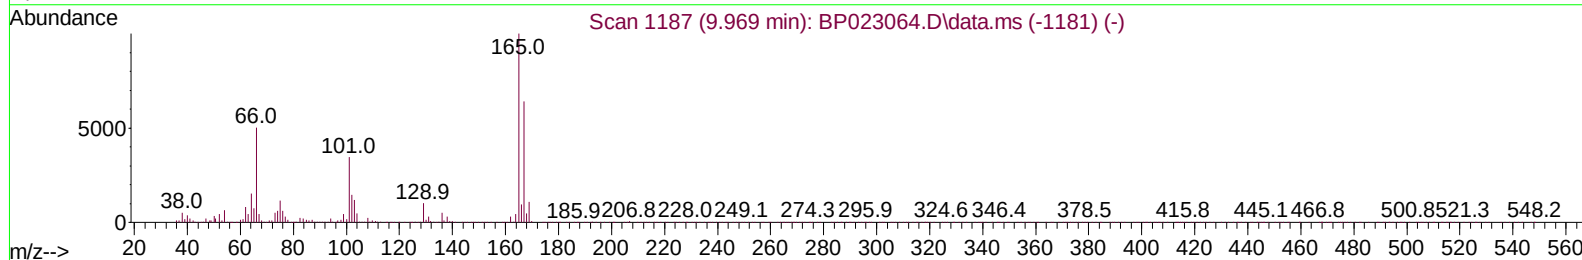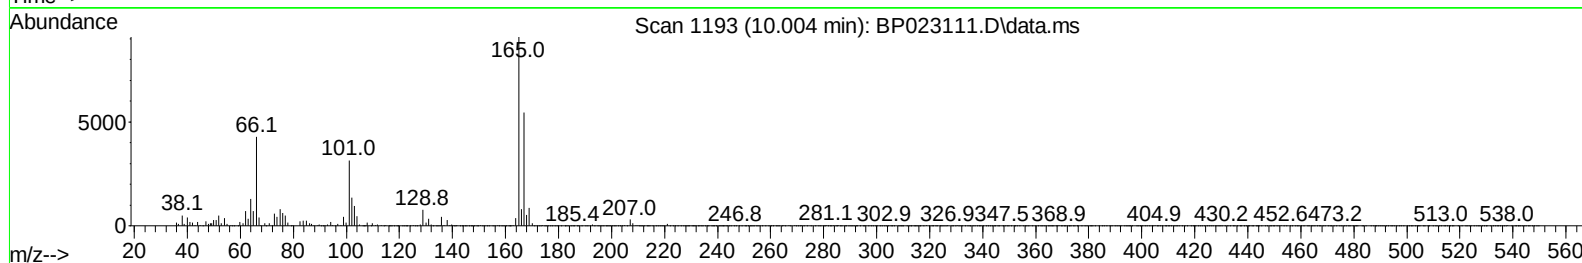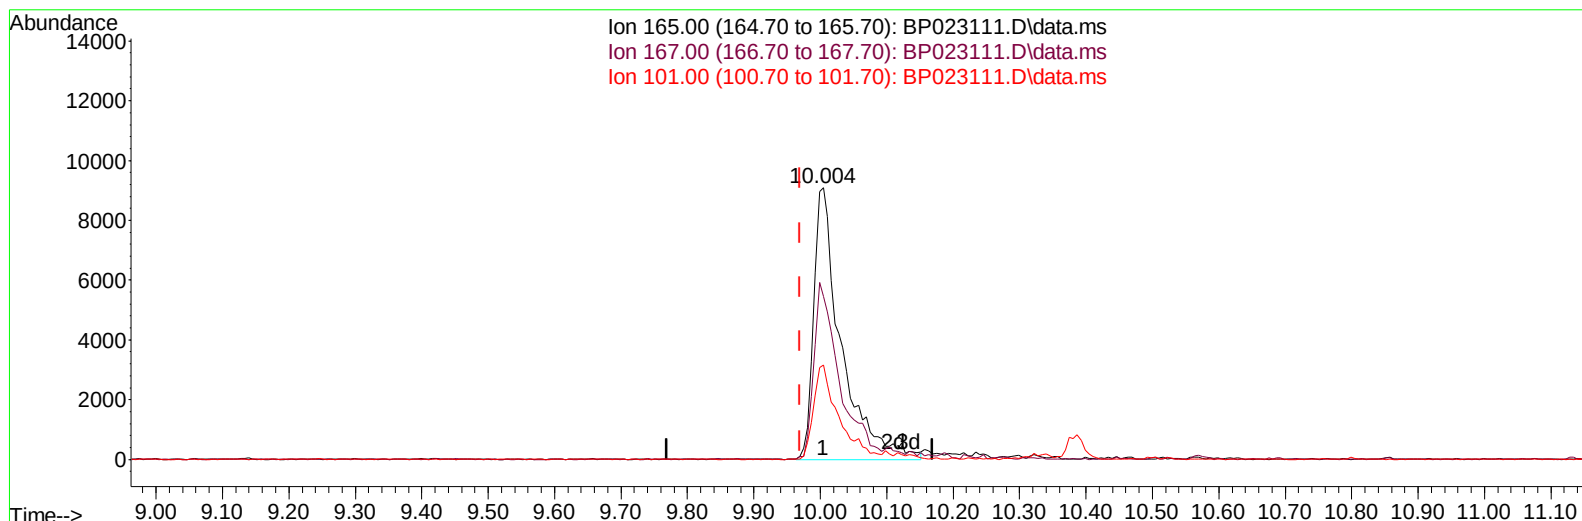

TIC: BP023111.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.004min (+ 0.035) 7.19 ng/ul m

response 25978

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.80	60.05
101.00	32.60	34.70
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023111.D
Acq On : 14 Nov 2024 18:26
Operator : RC/JU
Sample : P4803-07DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 14 23:46:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

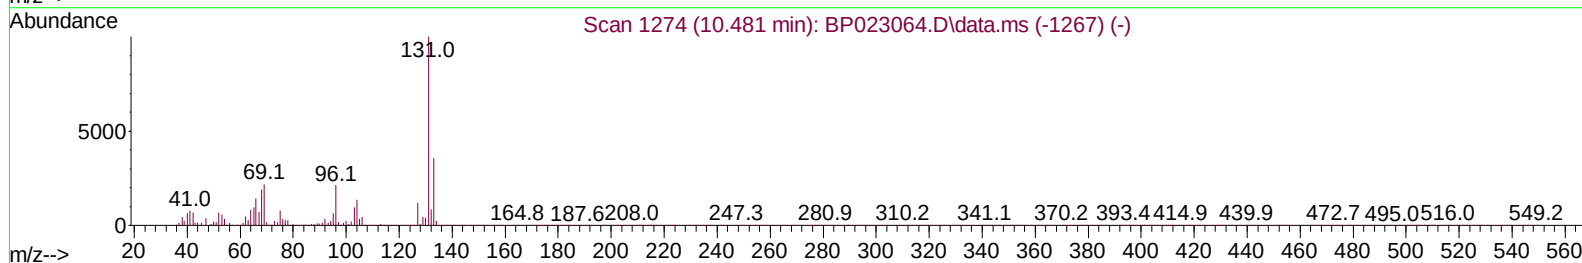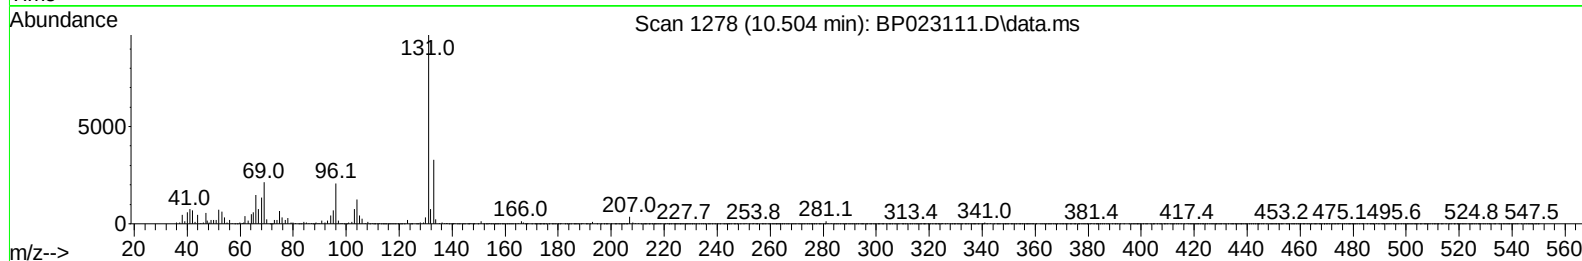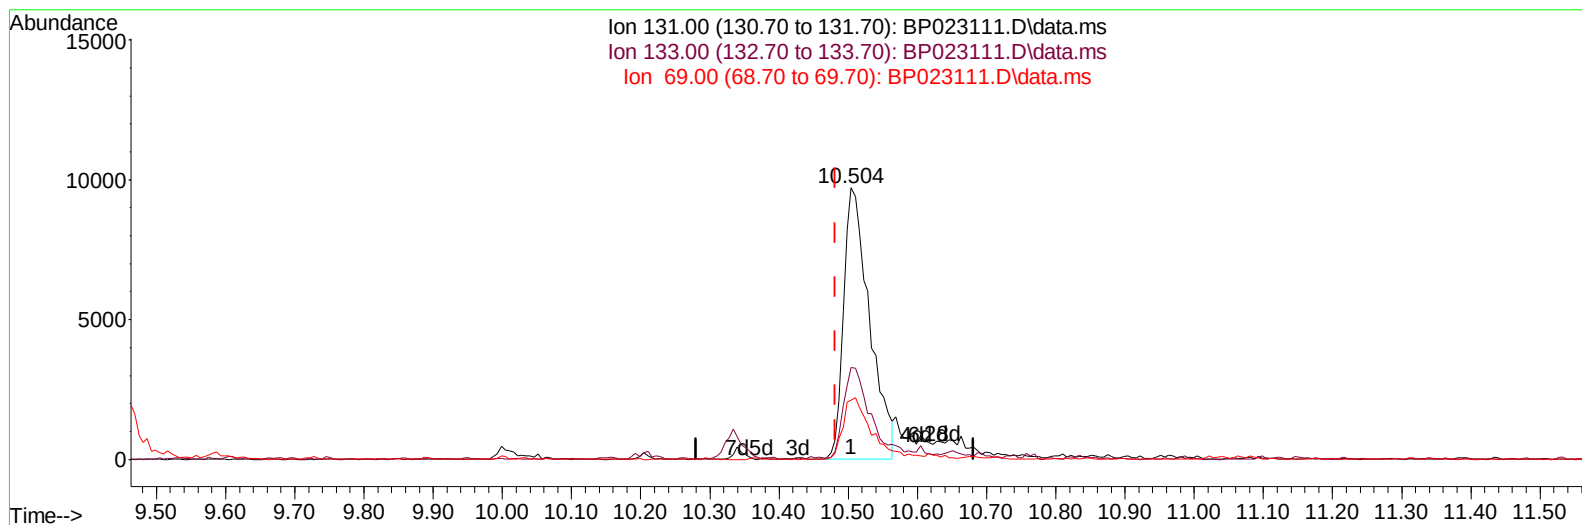

TIC: BP023111.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.504min (+ 0.023) 5.85 ng/u1

response 25215

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	33.90	33.93
69.00	23.10	21.90
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023111.D
 Acq On : 14 Nov 2024 18:26
 Operator : RC/JU
 Sample : P4803-07DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 14 23:46:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

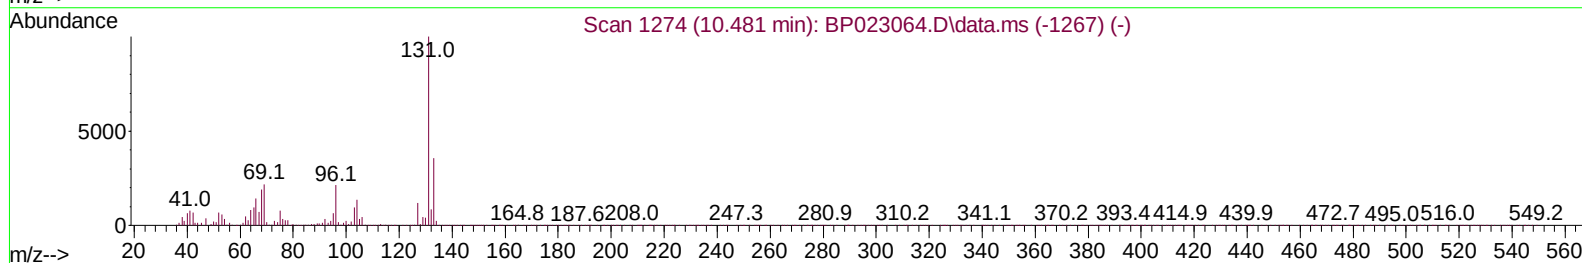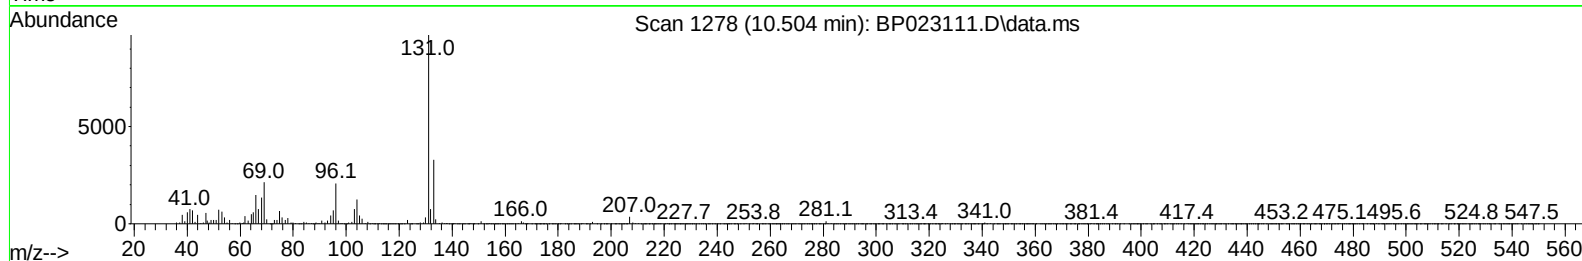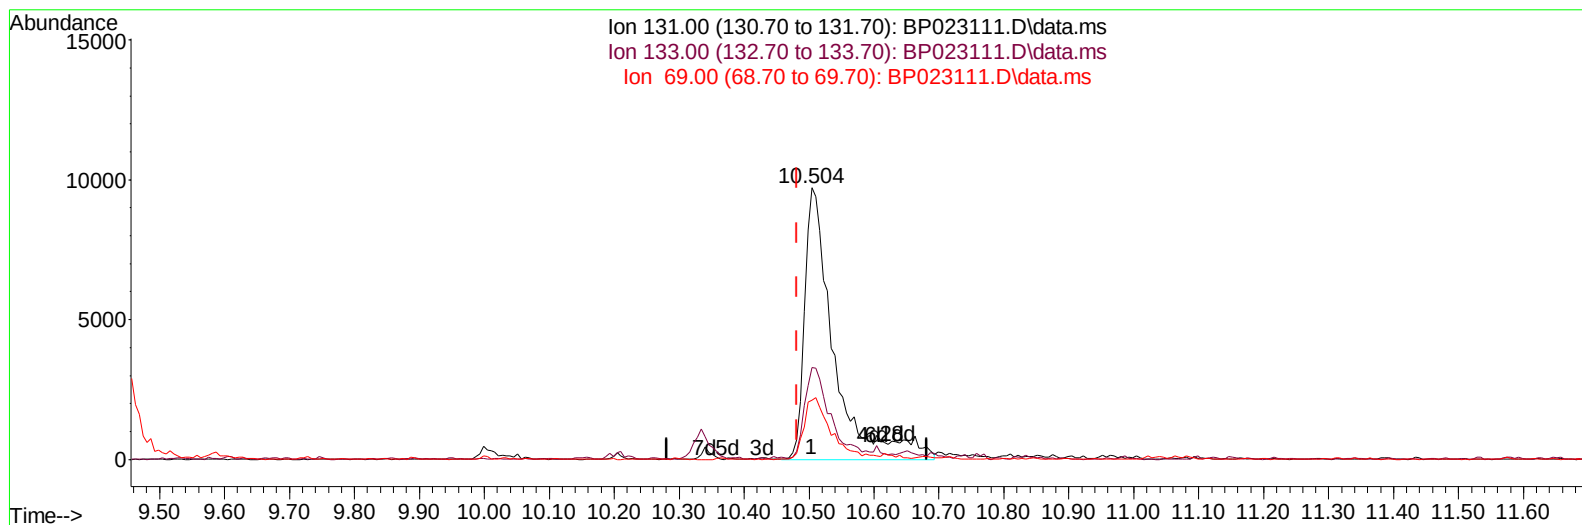

TIC: BP023111.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.504min (+ 0.023) 7.05 ng/ul m

response 30385

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	33.90	33.93
69.00	23.10	21.90
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023111.D
Acq On : 14 Nov 2024 18:26
Operator : RC/JU
Sample : P4803-07DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 14 23:46:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

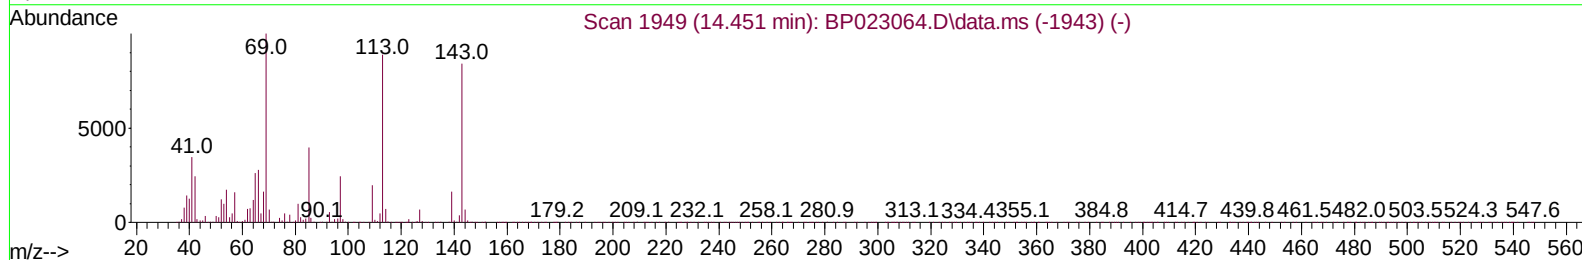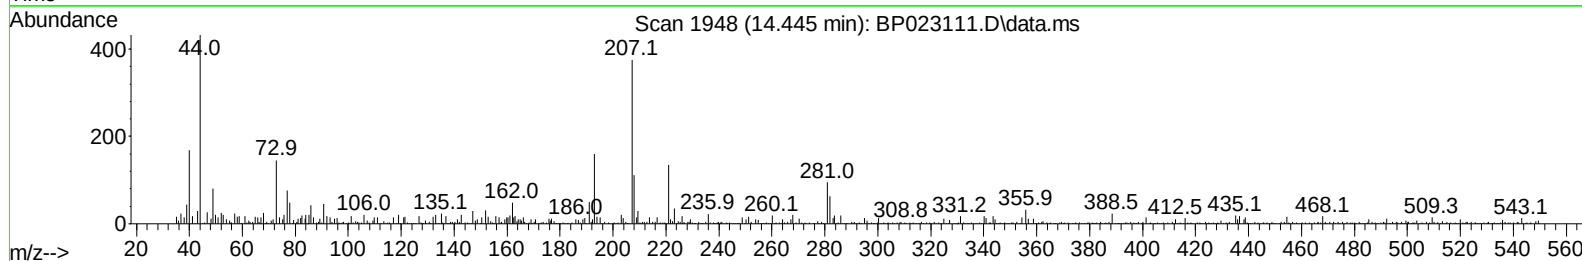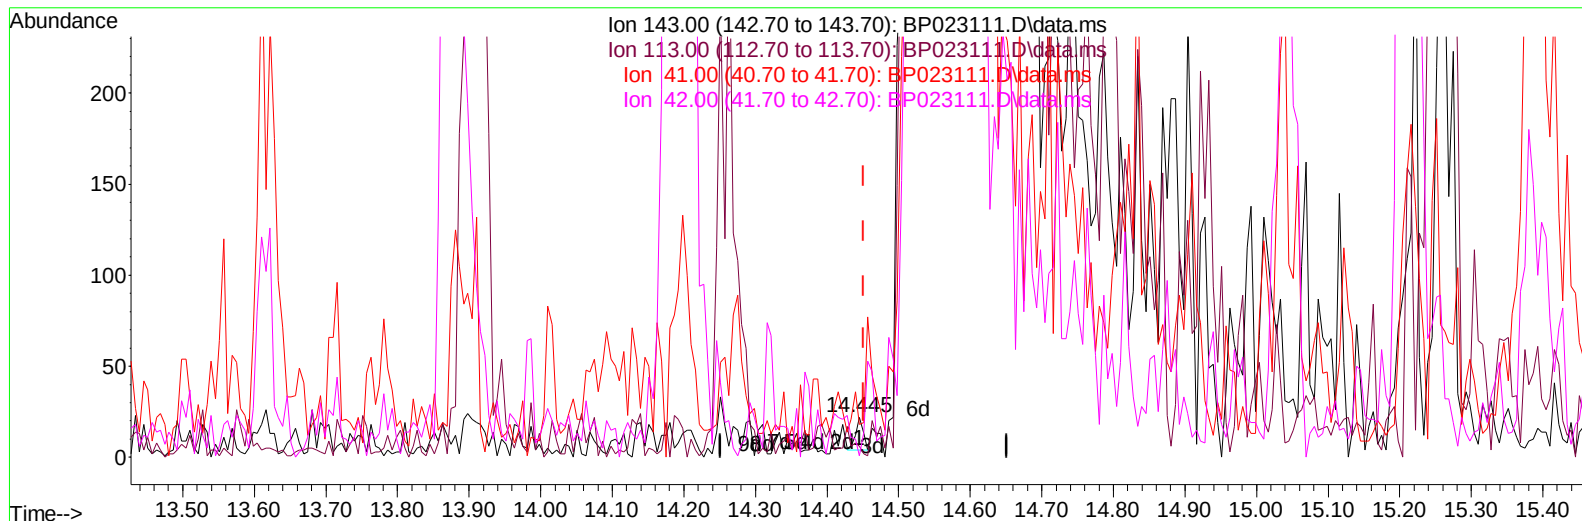

TIC: BP023111.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.445min (-0.006) 0.01 ng/u1

response 13

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	27.27#
41.00	39.20	81.82#
42.00	25.90	4.55#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023111.D
 Acq On : 14 Nov 2024 18:26
 Operator : RC/JU
 Sample : P4803-07DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:35:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

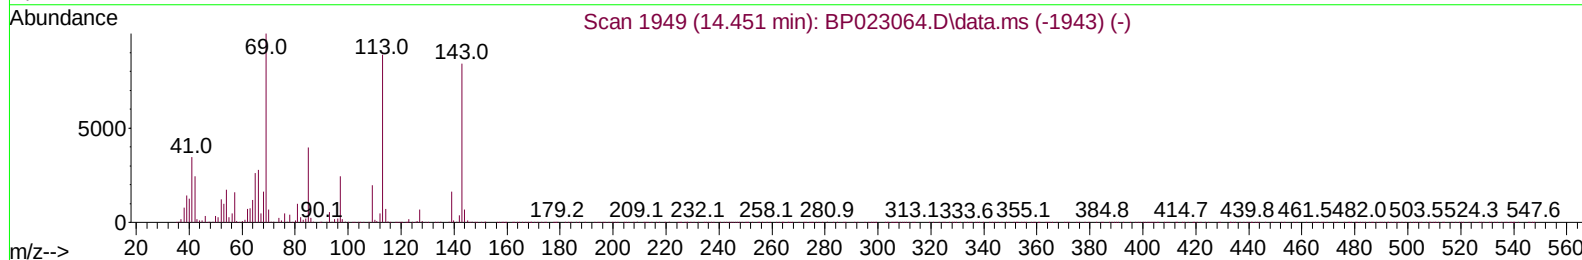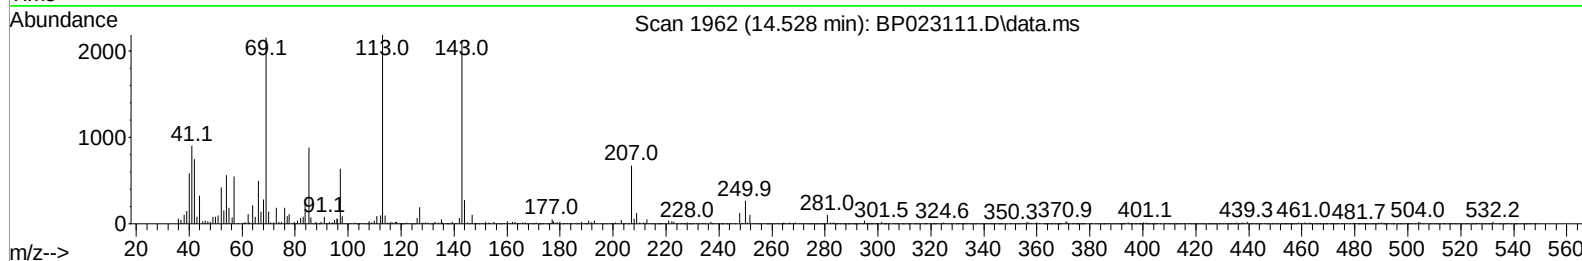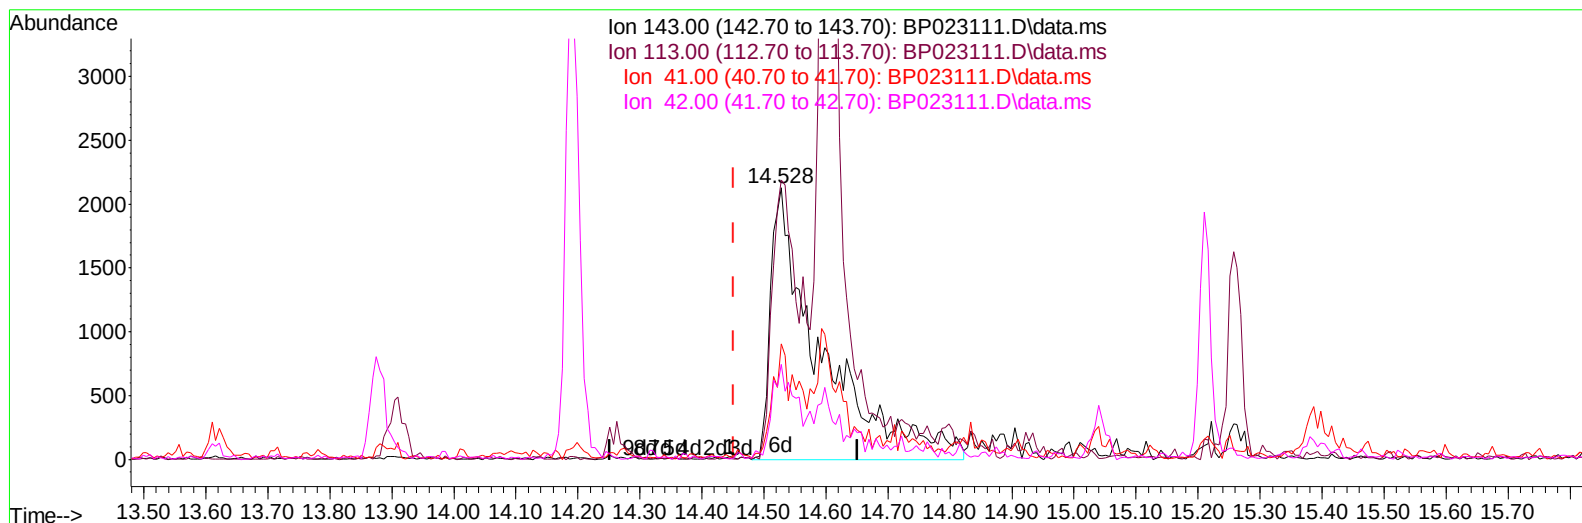

TIC: BP023111.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.528min (+ 0.076) 6.55 ng/ul m

response 11992

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	102.82
41.00	39.20	42.60
42.00	25.90	35.12#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023111.D
Acq On : 14 Nov 2024 18:26
Operator : RC/JU
Sample : P4803-07DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:38:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

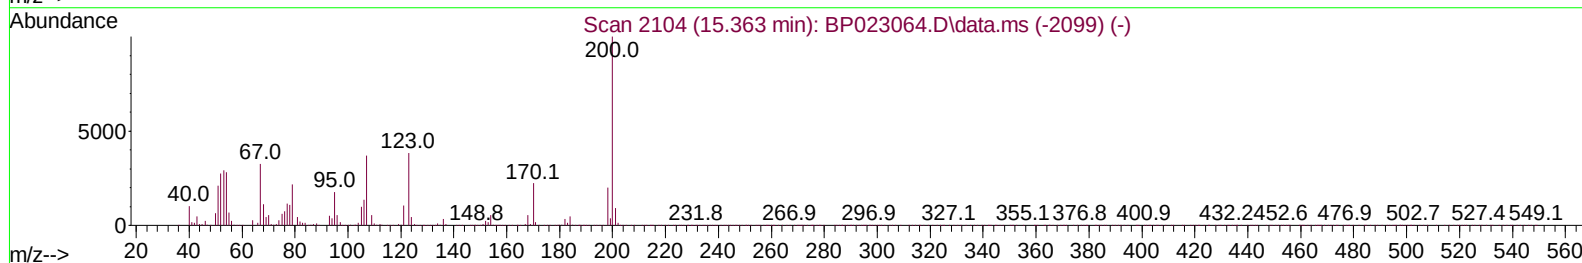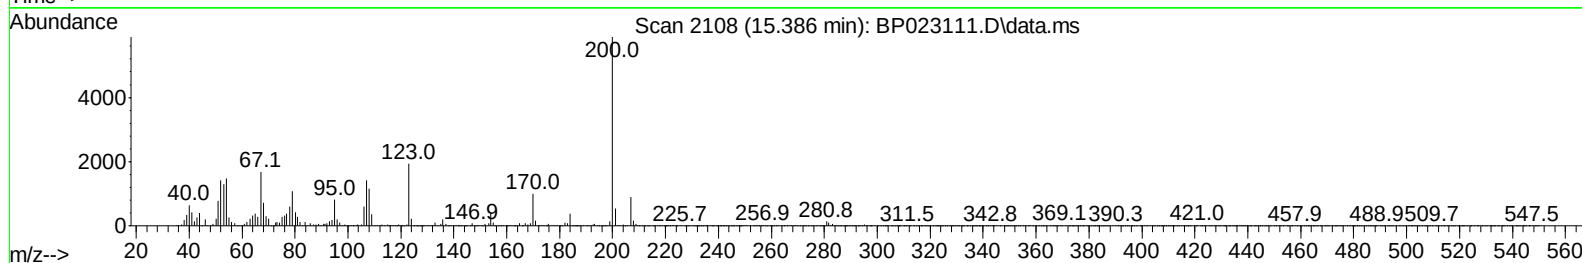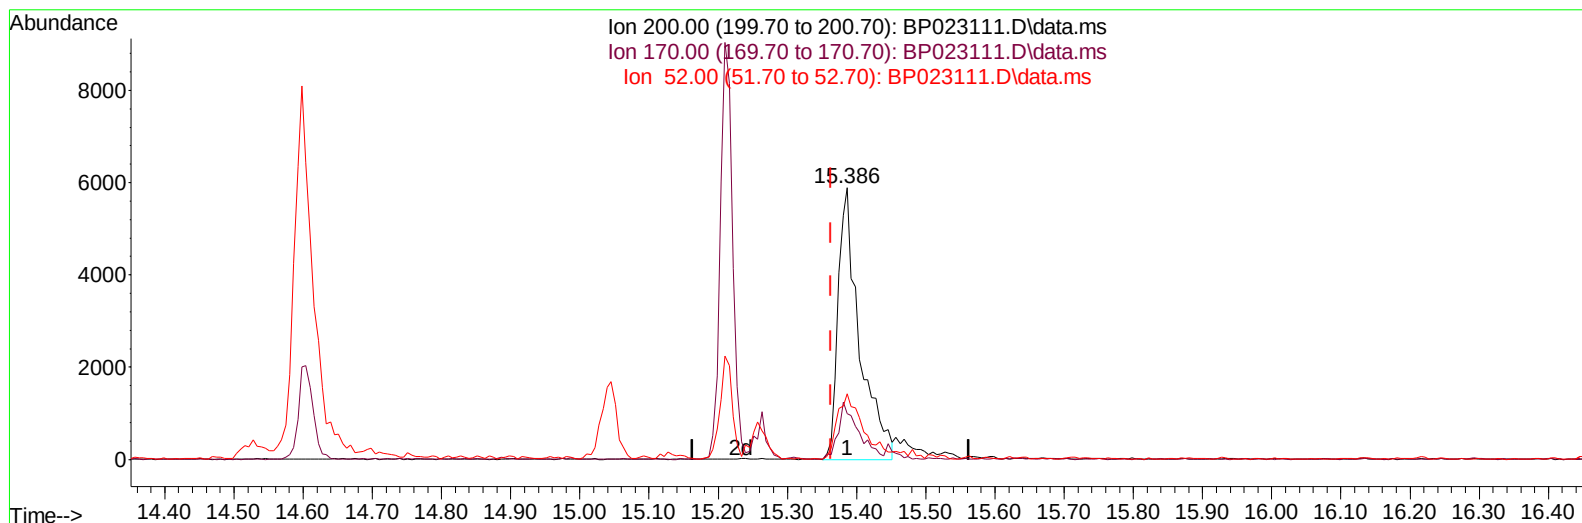

TIC: BP023111.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.386min (+ 0.023) 4.76 ng/ul

response 12647

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	22.70	16.85#
52.00	35.30	24.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023111.D
 Acq On : 14 Nov 2024 18:26
 Operator : RC/JU
 Sample : P4803-07DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:38:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

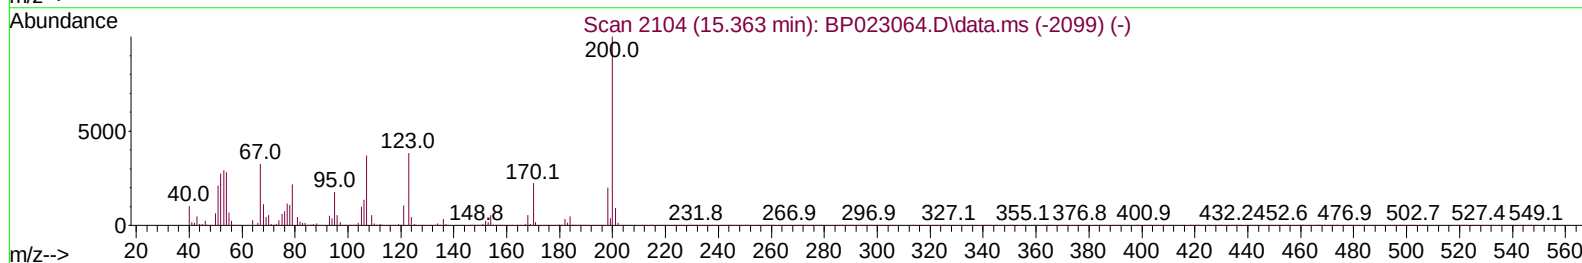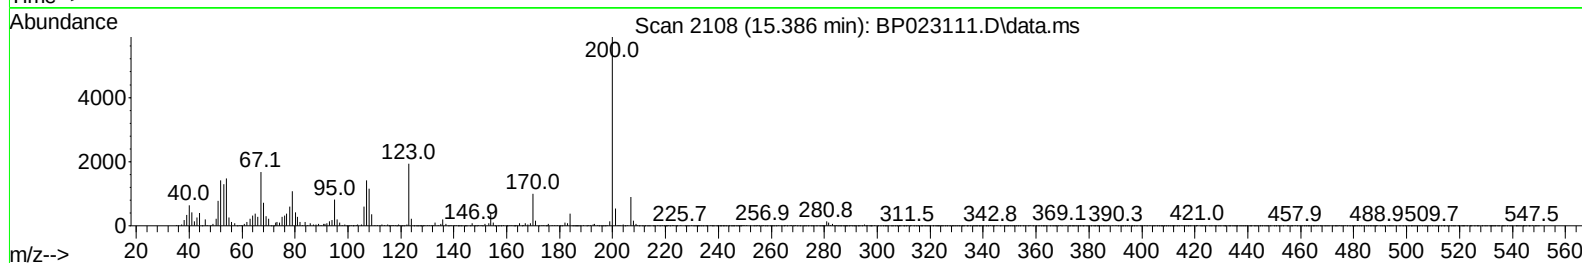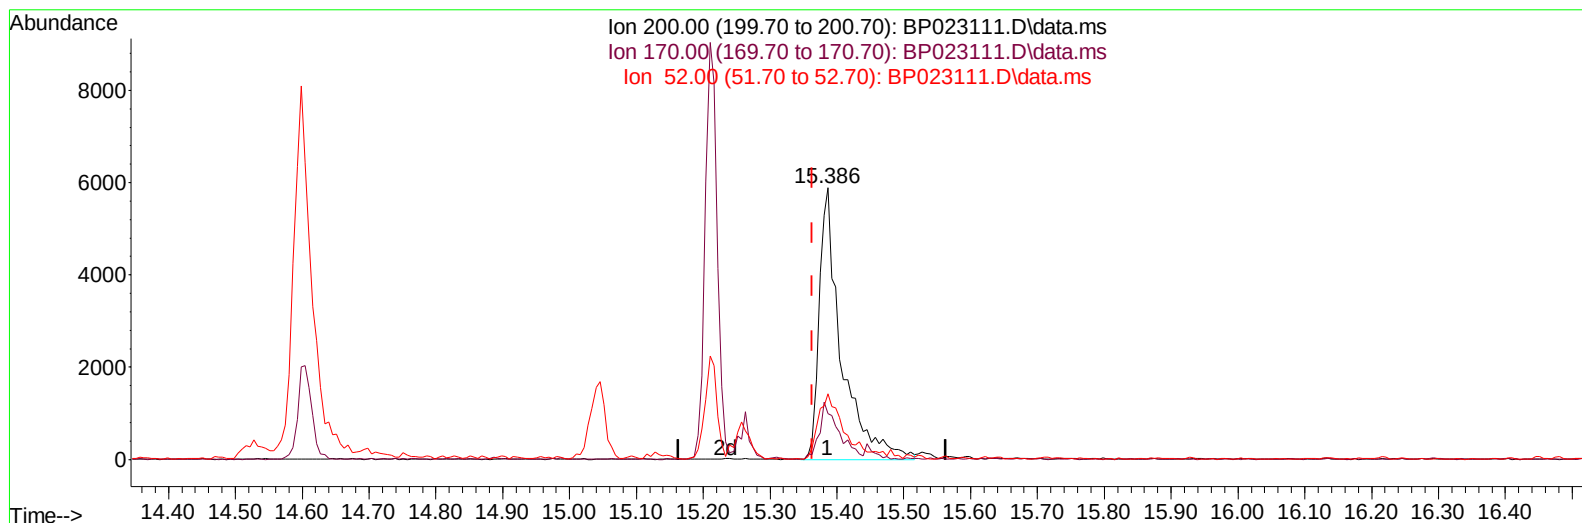

TIC: BP023111.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.386min (+ 0.023) 5.13 ng/ul m

response 13642

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	22.70	16.85#
52.00	35.30	24.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023111.D
Acq On : 14 Nov 2024 18:26
Operator : RC/JU
Sample : P4803-07DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:38:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

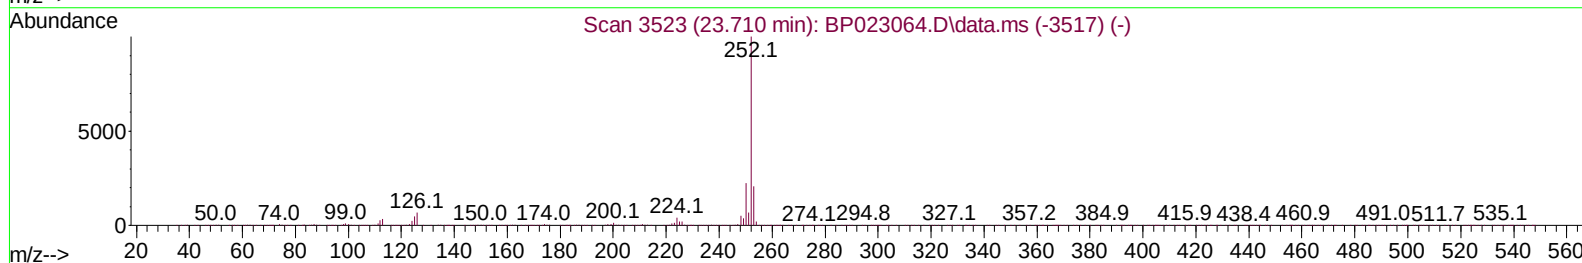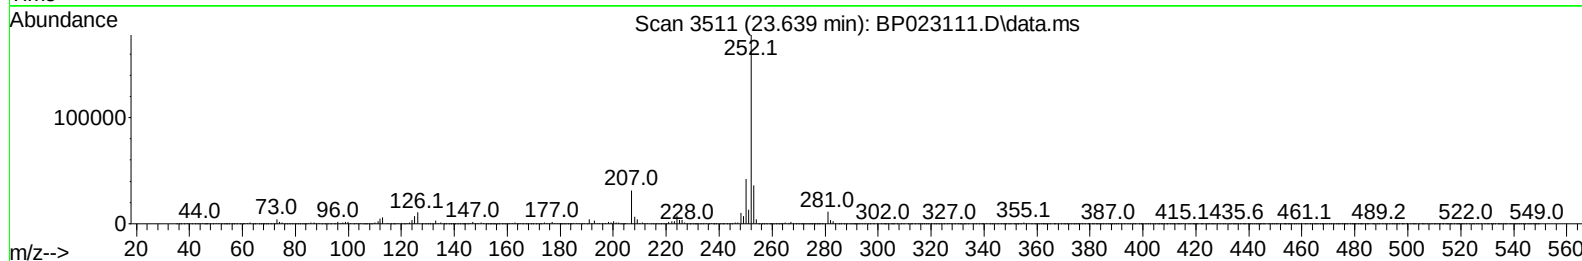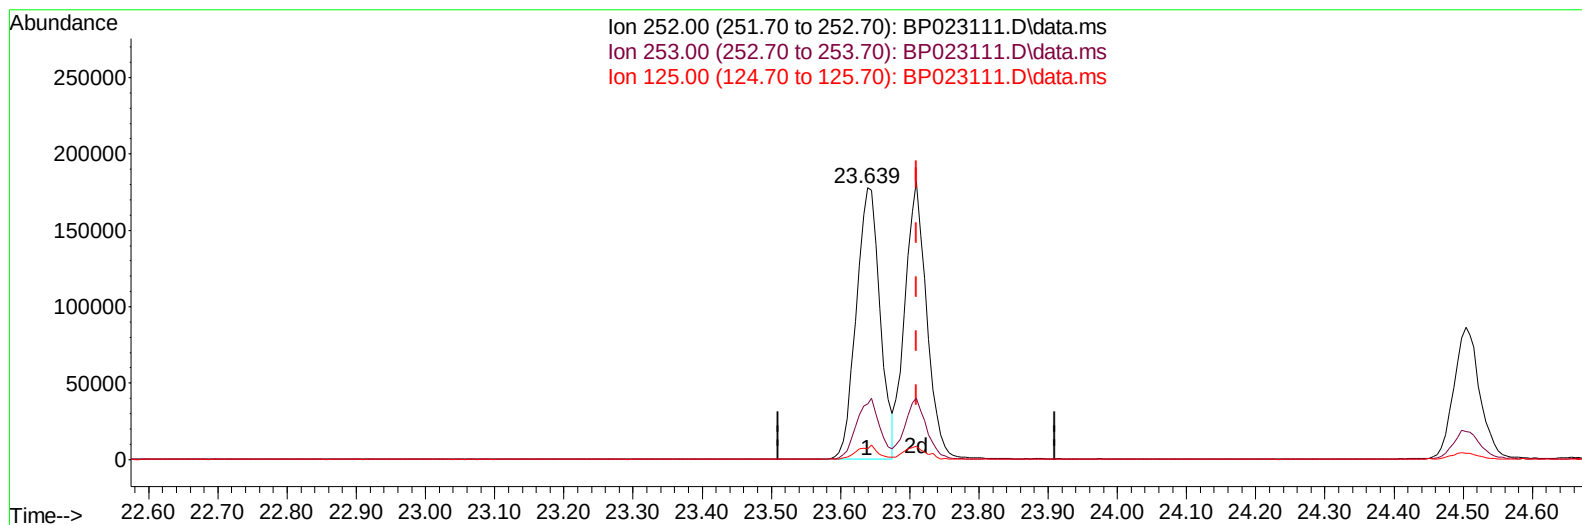

TIC: BP023111.D\data.ms

(91) Benzo(k)fluoranthene

23.639min (-0.071) 12.44 ng/u1

response 424558

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.30	20.49
125.00	3.70	3.97
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023111.D
Acq On : 14 Nov 2024 18:26
Operator : RC/JU
Sample : P4803-07DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:38:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

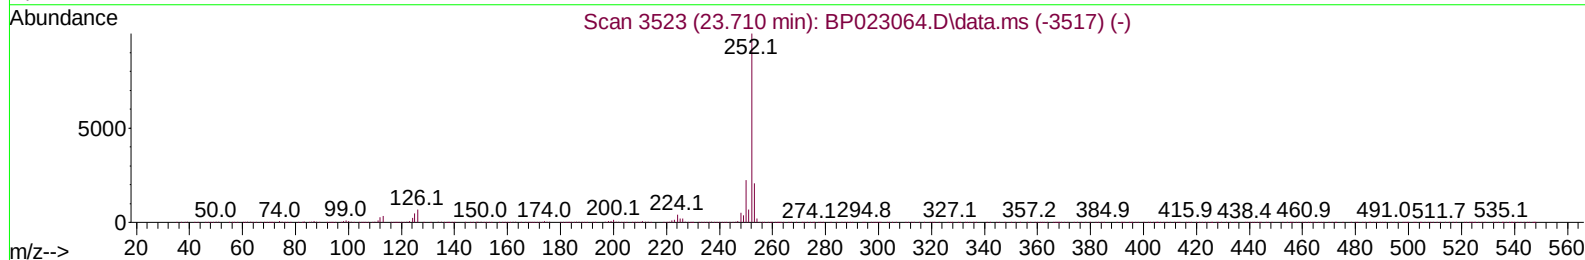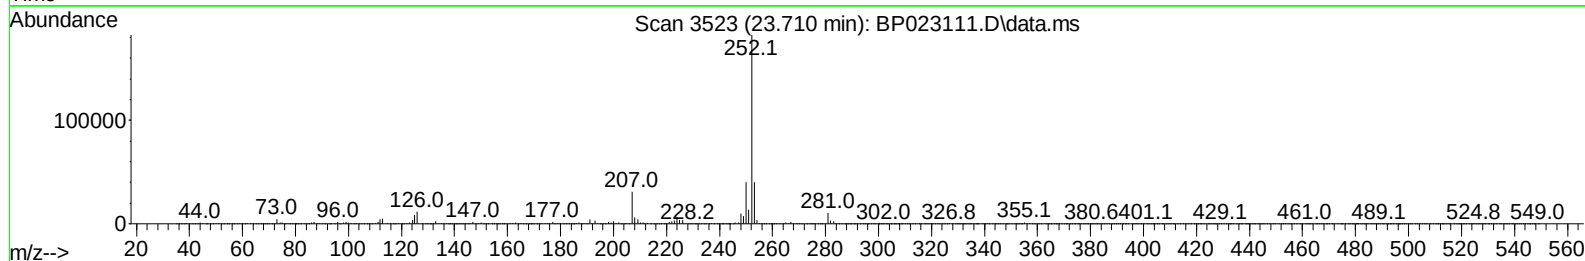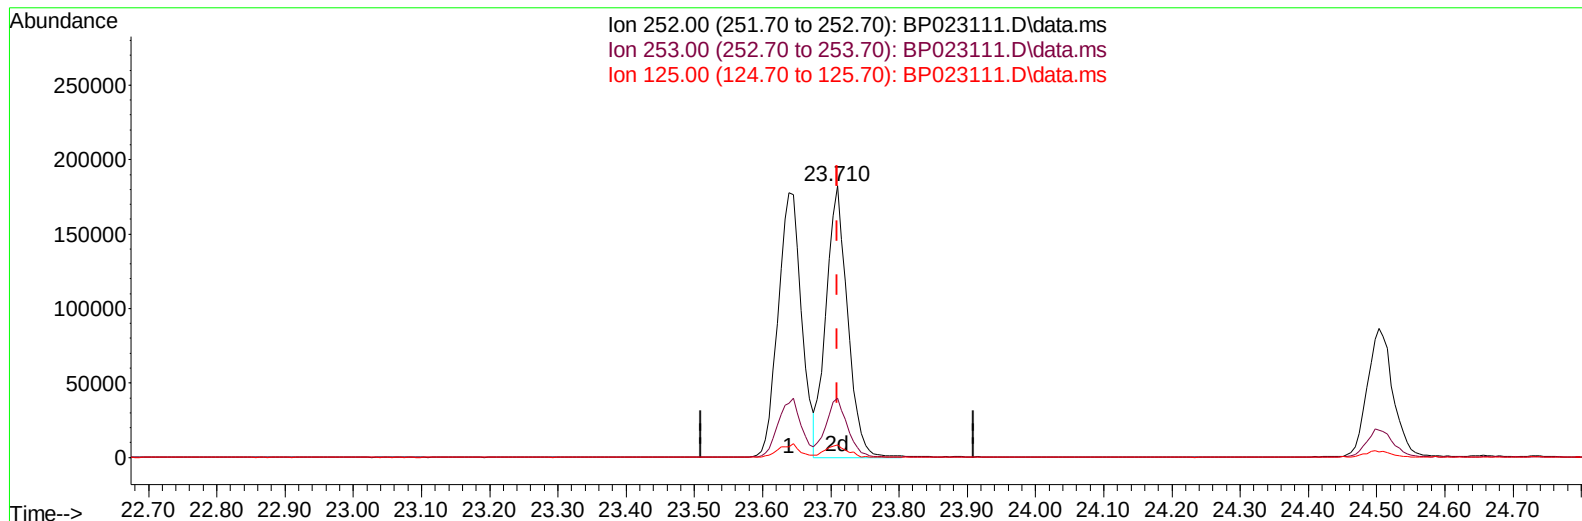

TIC: BP023111.D\data.ms

(91) Benzo(k)fluoranthene

23.710min (-0.000) 11.66 ng/ul m

response 398108

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.30	21.94
125.00	3.70	4.73#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023111.D
Acq On : 14 Nov 2024 18:26
Operator : RC/JU
Sample : P4803-07DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:38:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

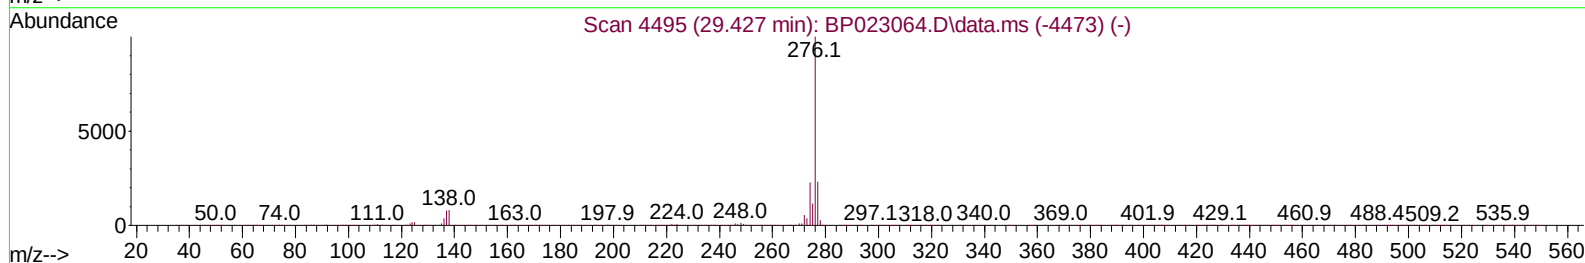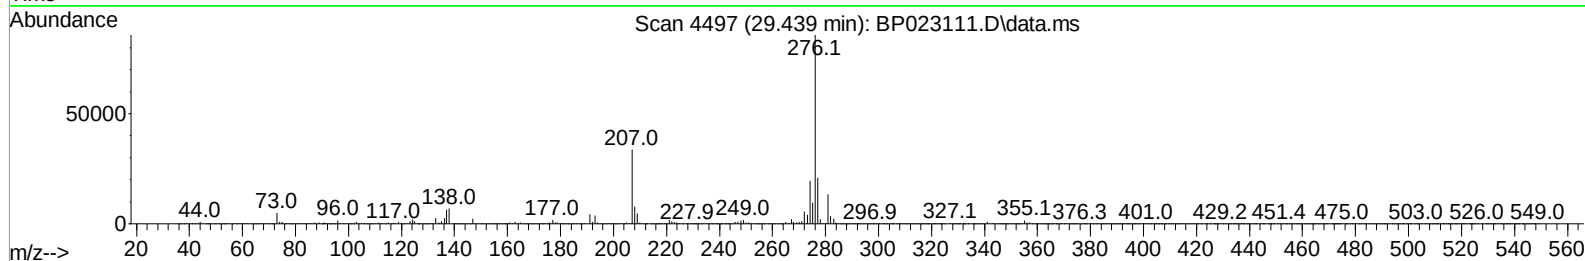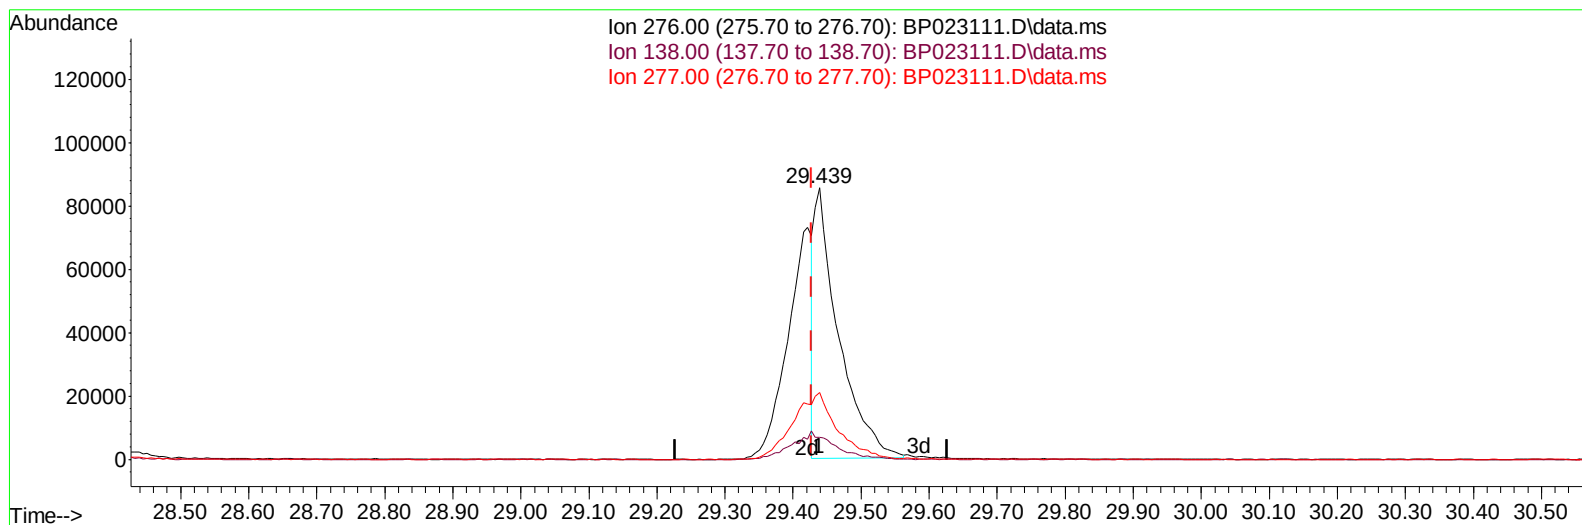

TIC: BP023111.D\data.ms

(96) Benzo(g,h,i)perylene

29.439min (+ 0.012) 6.36 ng/u1

response 211059

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	8.90	8.05
277.00	24.30	24.57
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023111.D
 Acq On : 14 Nov 2024 18:26
 Operator : RC/JU
 Sample : P4803-07DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:38:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

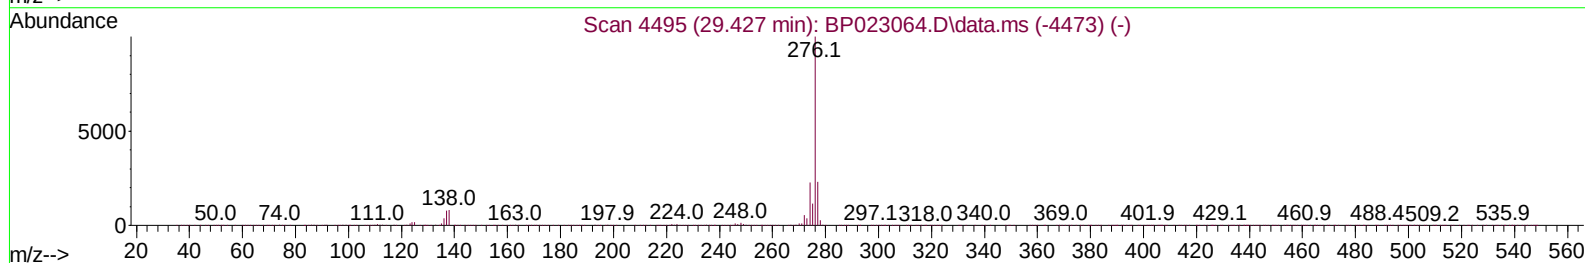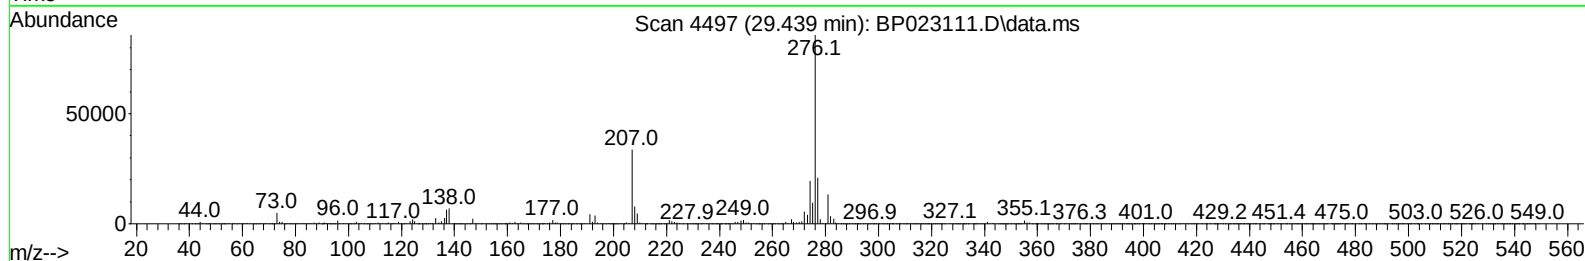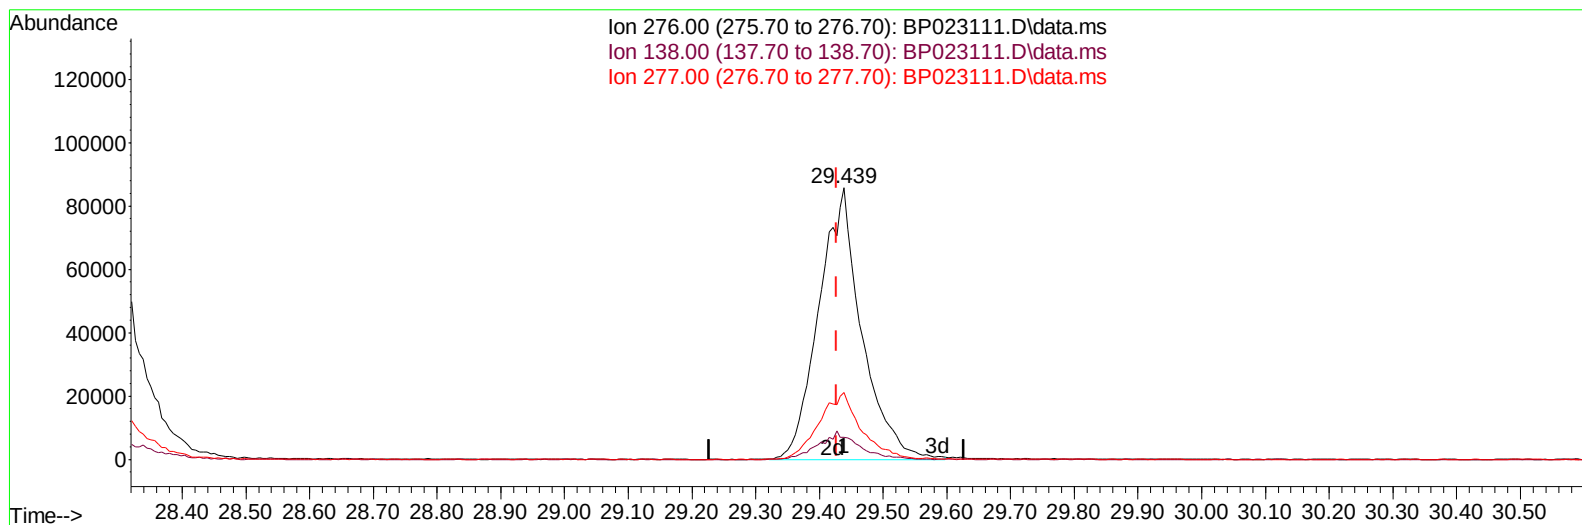

TIC: BP023111.D\data.ms

(96) Benzo(g,h,i)perylene

29.439min (+ 0.012) 12.04 ng/ul m

response 399361

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	8.90	8.05
277.00	24.30	24.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023111.D
 Acq On : 14 Nov 2024 18:26
 Operator : RC/JU
 Sample : P4803-07DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0AQ2DL

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:41:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.581	152	55127	20.000	ng/ul	0.00
20) Naphthalene-d8	10.334	136	207947	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.192	164	168924	20.000	ng/ul	-0.01
64) Phenanthrene-d10	16.998	188	443622	20.000	ng/ul	-0.02
79) Chrysene-d12	21.445	240	506113	20.000	ng/ul	0.00
88) Perylene-d12	24.668	264	622931	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	1949m	1.699	ng/uL	0.00
4) Pyridine-d5	3.564	84	18400	5.400	ng/ul	0.02
7) Phenol-d5	6.799	99	27089m	6.646	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	6.934	67	17002	7.100	ng/ul	0.00
11) 2-Chlorophenol-d4	7.134	132	20497	6.867	ng/ul	0.00
15) 4-Methylphenol-d8	8.310	113	20013	5.967	ng/ul	0.02
21) Nitrobenzene-d5	8.734	128	10535	7.277	ng/ul	0.01
24) 2-Nitrophenol-d4	9.451	143	12387m	7.177	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.004	165	25978m	7.188	ng/ul	0.04
31) 4-Chloroaniline-d4	10.504	131	30385m	7.047	ng/ul	0.02
46) Dimethylphthalate-d6	13.616	166	103049	8.464	ng/ul	0.00
49) Acenaphthylene-d8	13.881	160	100341	7.899	ng/ul	-0.02
54) 4-Nitrophenol-d4	14.528	143	11992m	6.554	ng/ul	0.08
60) Fluorene-d10	15.210	176	93009	8.713	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.386	200	13642m	5.133	ng/ul	0.02
73) Anthracene-d10	17.110	188	159817	8.508	ng/ul	0.00
81) Pyrene-d10	19.498	212	217151	9.315	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.433	264	259113	8.732	ng/ul	-0.01
Target Compounds						
					Qvalue	
10) Bis(2-Chloroethyl)ether	7.022	93	24102	7.536	ng/ul	97
14) 2,2'-oxybis(1-Chloropr...	8.099	45	55450	15.316	ng/ul#	93
17) N-Nitroso-di-n-propyla...	8.375	70	59684	21.209	ng/ul	99
19) Hexachloroethane	8.628	117	25914	17.290	ng/ul	91
22) Nitrobenzene	8.775	77	51727	12.453	ng/ul	99
23) Isophorone	9.281	82	197544	26.596	ng/ul	98
27) Bis(2-Chloroethoxy)met...	9.763	93	24635	6.028	ng/ul	96
30) Naphthalene	10.387	128	38886	3.849	ng/ul	99
33) Hexachlorobutadiene	10.657	225	54602	16.856	ng/ul	97
36) 2-Methylnaphthalene	11.998	142	102077	13.384	ng/ul	94
40) Hexachlorocyclopentadiene	12.340	237	32926	10.992	ng/ul	95
44) 2-Chloronaphthalene	13.069	162	232238	26.247	ng/ul	98
50) Acenaphthylene	13.910	152	129667	10.098	ng/ul	98
52) Acenaphthene	14.257	153	31914	3.423	ng/ul	96
56) Dibenzofuran	14.604	168	254341	17.658	ng/ul	97
57) 2,4-Dinitrotoluene	14.598	165	126302	33.930	ng/ul	91
59) Diethylphthalate	15.045	149	411244	34.631	ng/ul	99
61) Fluorene	15.257	166	30596	2.595	ng/ul	96
62) 4-Chlorophenyl-phenyle...	15.257	204	73415	10.576	ng/ul	99
69) Hexachlorobenzene	16.292	284	47874	7.570	ng/ul	98
72) Phenanthrene	17.045	178	203154	9.699	ng/ul	100
74) Anthracene	17.151	178	261820	12.433	ng/ul	99
78) Di-n-butylphthalate	18.016	149	805597	39.512	ng/ul	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023111.D
 Acq On : 14 Nov 2024 18:26
 Operator : RC/JU
 Sample : P4803-07DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A0AQ2DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 15 00:41:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
80) Fluoranthene	19.151	202	364261	13.563	ng/ul	100
83) Butylbenzylphthalate	20.469	149	110334	11.615	ng/ul	95
85) Benzo(a)anthracene	21.421	228	188228	6.091	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.351	149	130614	9.676	ng/ul	96
90) Benzo(b)fluoranthene	23.639	252	424558	12.245	ng/ul	97
91) Benzo(k)fluoranthene	23.710	252	398108m	11.664	ng/ul	
93) Benzo(a)pyrene	24.504	252	224256	7.155	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	28.303	276	342236	7.837	ng/ul	97
95) Dibenzo(a,h)anthracene	28.362	278	240246	6.776	ng/ul	98
96) Benzo(g,h,i)perylene	29.439	276	399361m	12.041	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

