




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023113.D
 Acq On : 14 Nov 2024 20:27
 Operator : RC/JU
 Sample : P4802-11
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCPD3

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:46:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

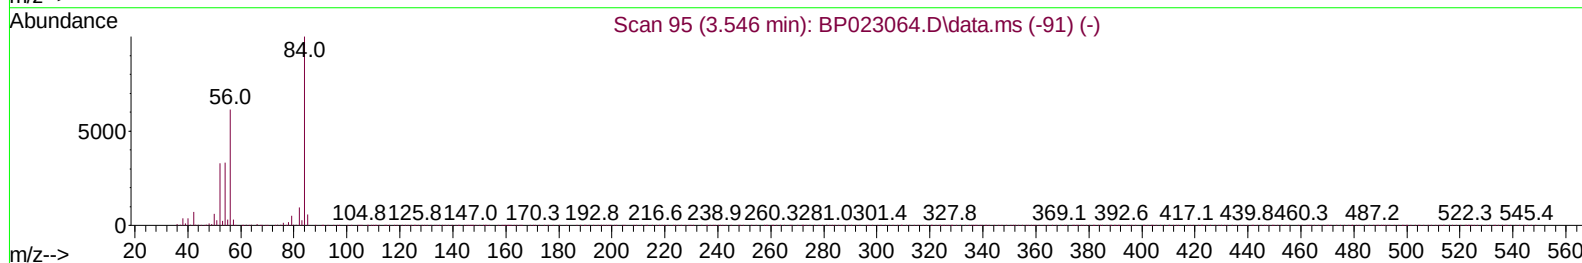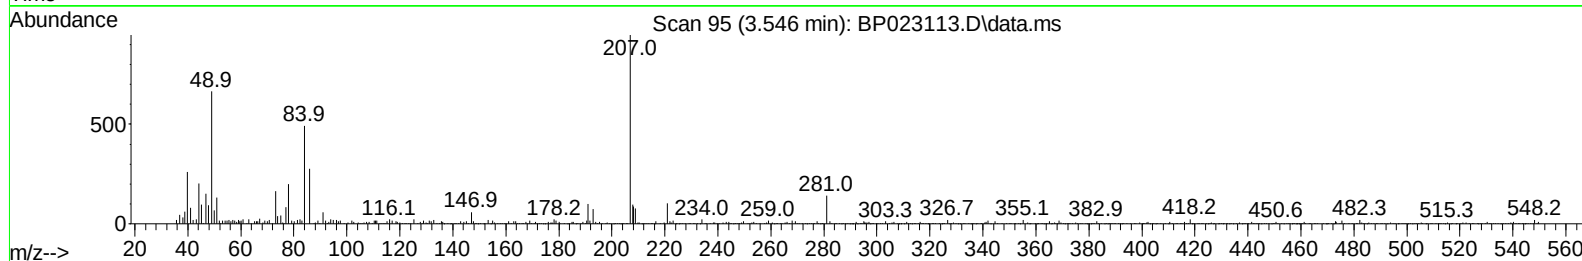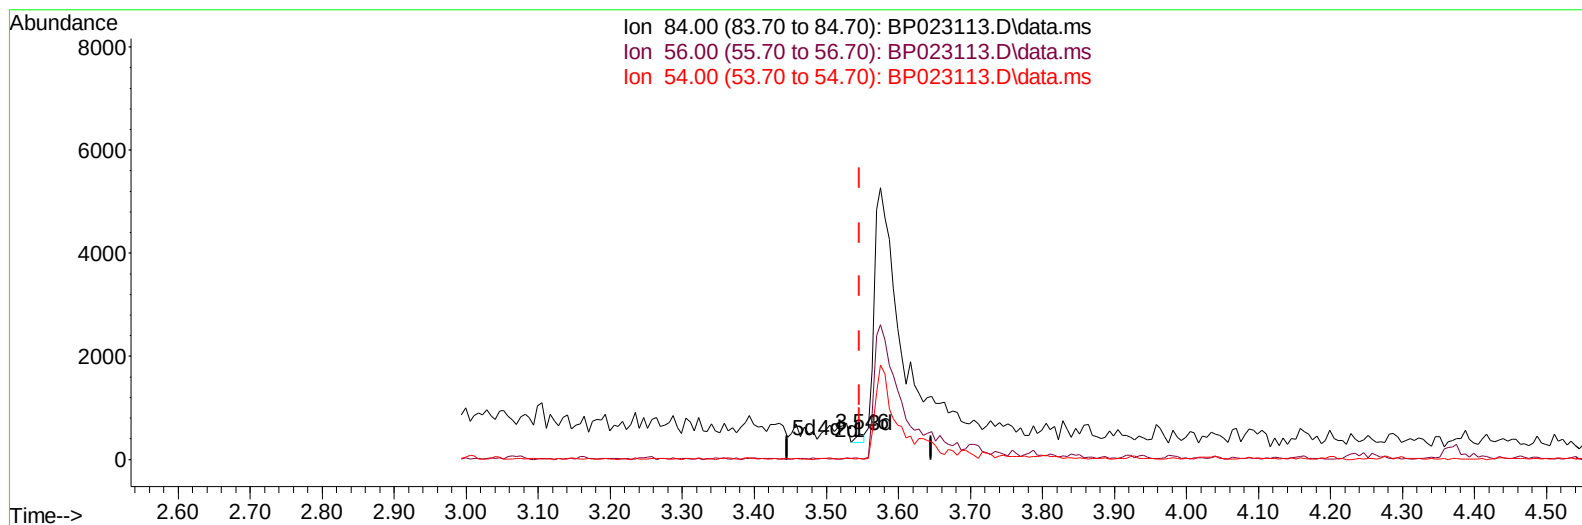

TIC: BP023113.D\data.ms

(4) Pyridine-d5 (S)

3.546min (+ 0.000) 0.03 ng/u1

response 135

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	62.10	2.85#
54.00	32.30	3.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023113.D
Acq On : 14 Nov 2024 20:27
Operator : RC/JU
Sample : P4802-11
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCPD3

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:46:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

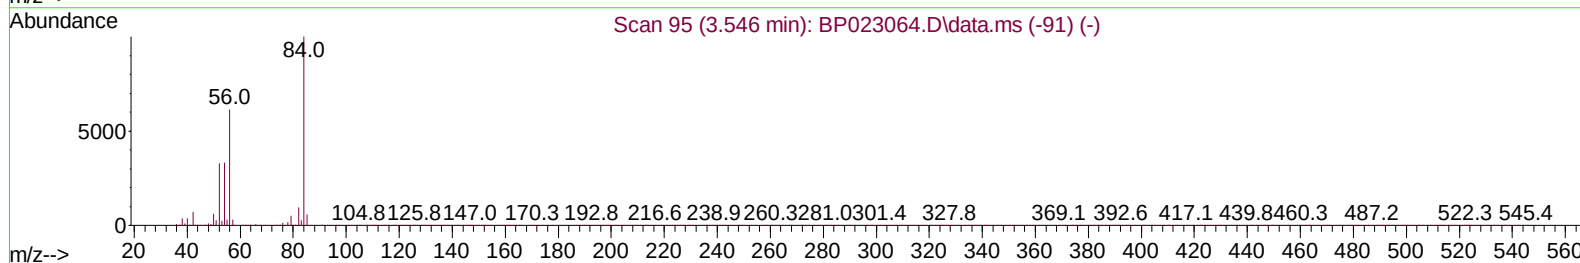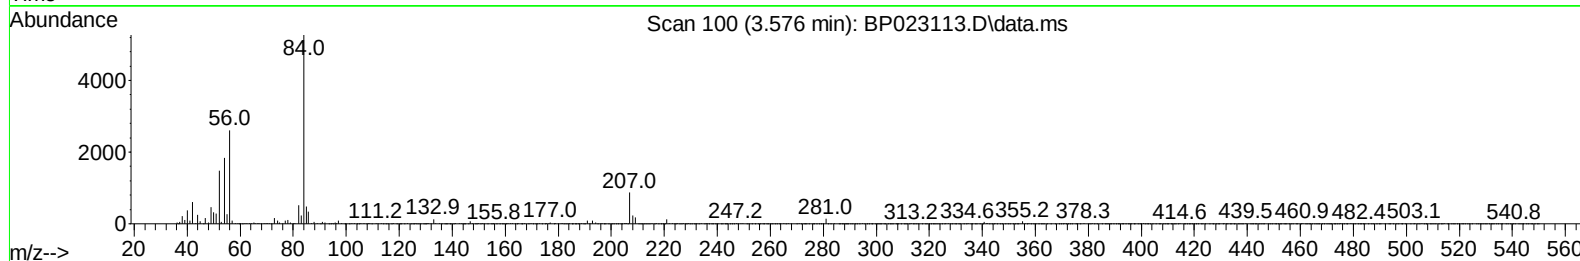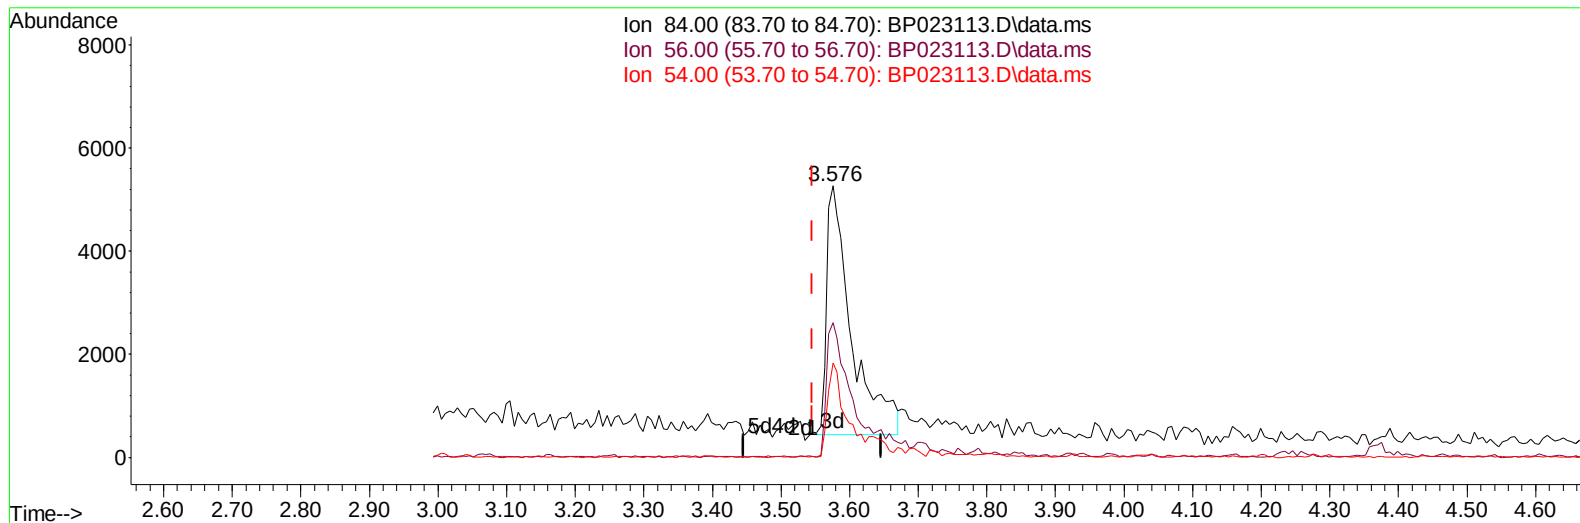

TIC: BP023113.D\data.ms

(4) Pyridine-d5 (S)

3.576min (+ 0.030) 2.52 ng/ul m

response 12121

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	62.10	49.53#
54.00	32.30	34.90
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023113.D
Acq On : 14 Nov 2024 20:27
Operator : RC/JU
Sample : P4802-11
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCPD3

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:46:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

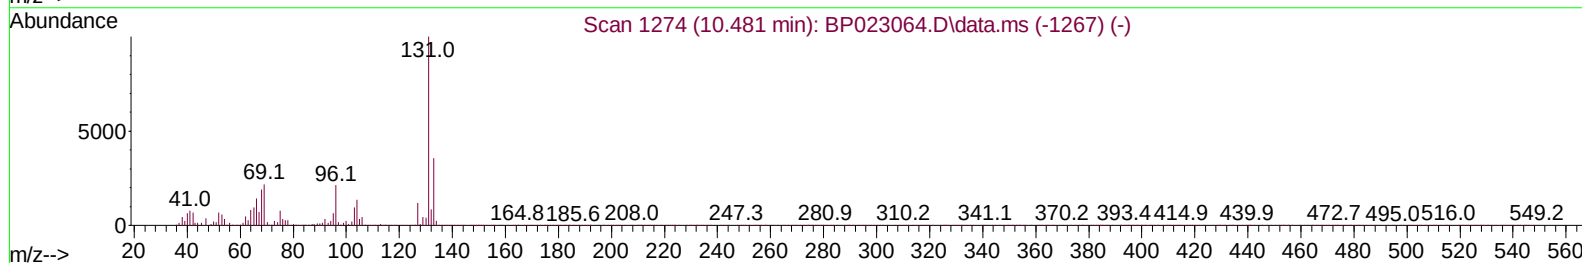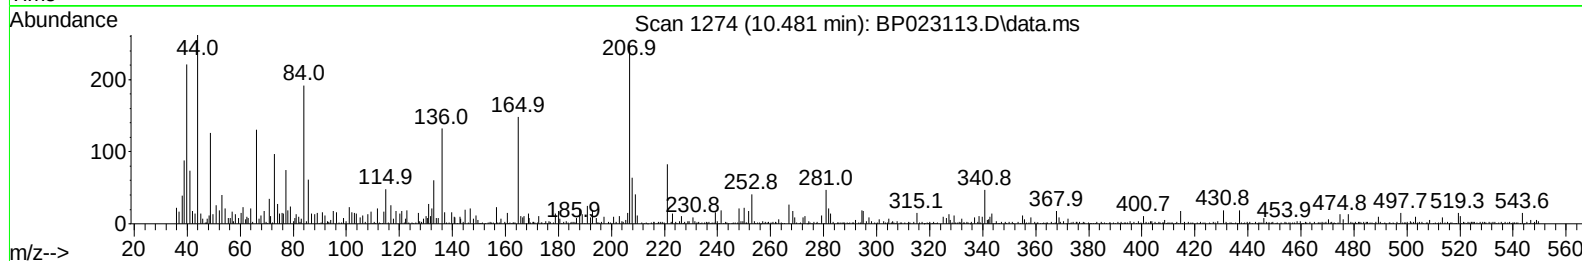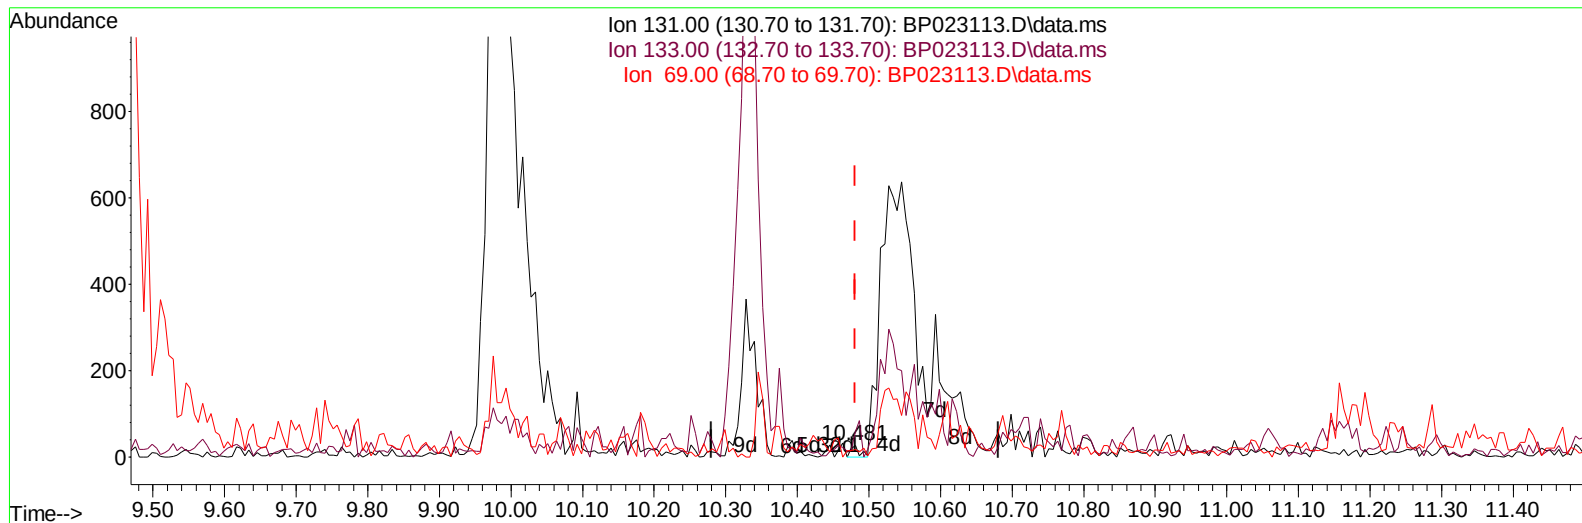

TIC: BP023113.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.481min (+ 0.000) 0.00 ng/uI

response 22

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	33.90	214.29#
69.00	23.10	64.29#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023113.D
Acq On : 14 Nov 2024 20:27
Operator : RC/JU
Sample : P4802-11
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCPD3

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:46:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

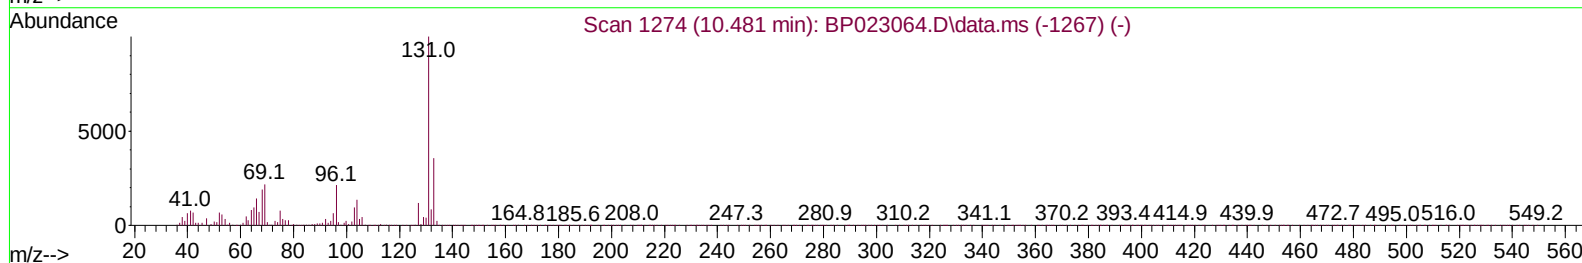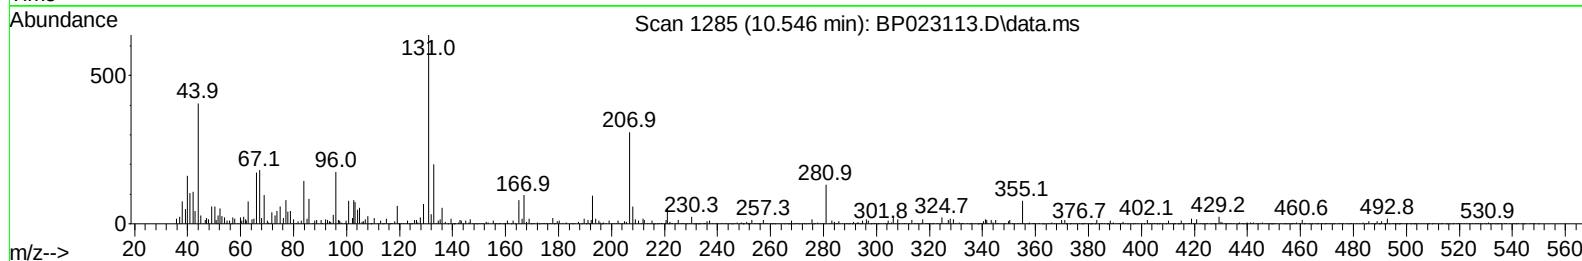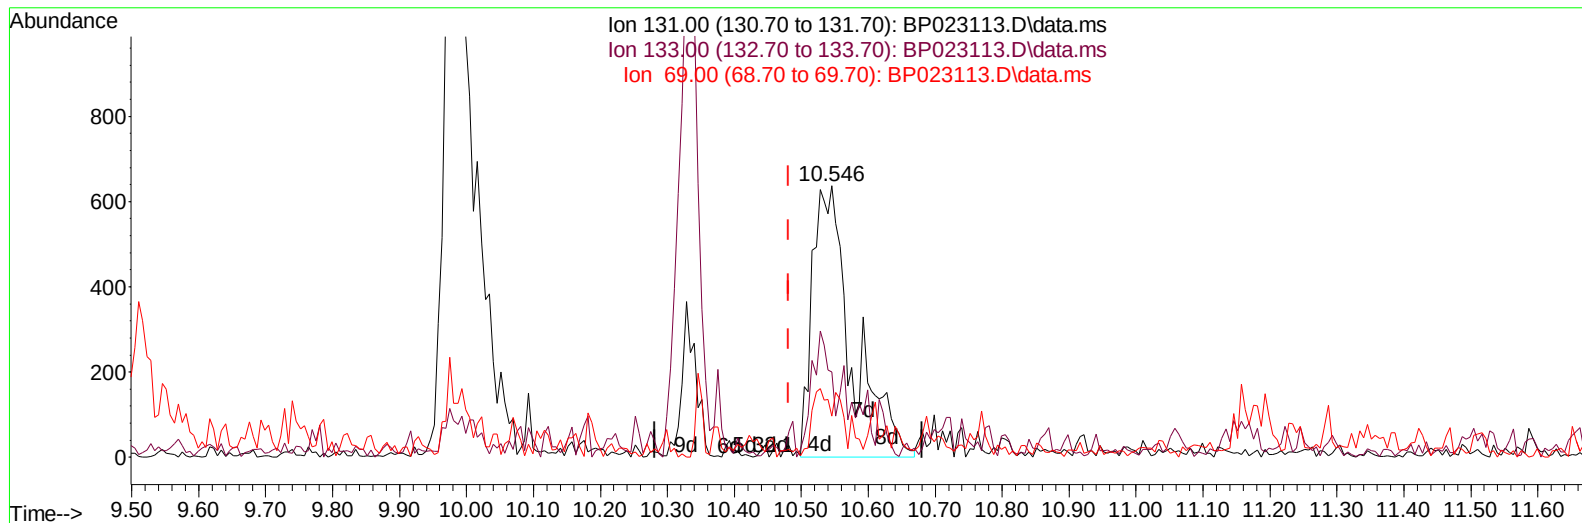

TIC: BP023113.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.546min (+ 0.065) 0.43 ng/ul m

response 2574

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	33.90	31.40
69.00	23.10	15.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023113.D
 Acq On : 14 Nov 2024 20:27
 Operator : RC/JU
 Sample : P4802-11
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCPD3

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:46:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

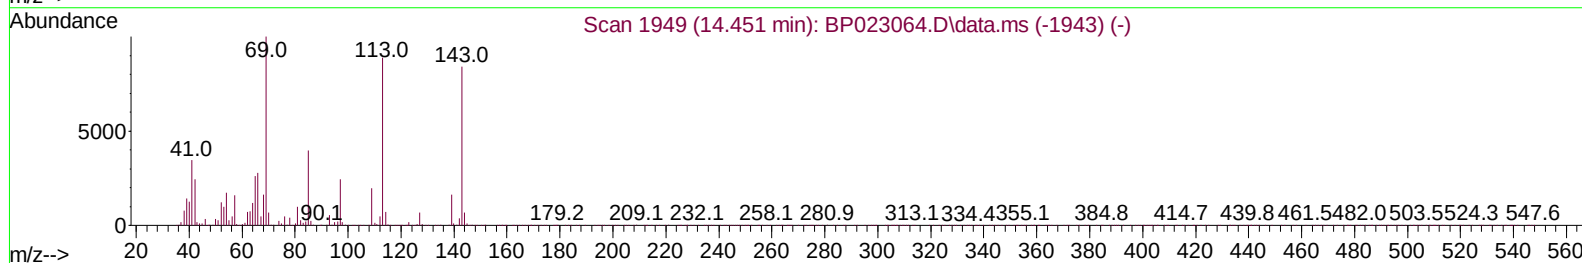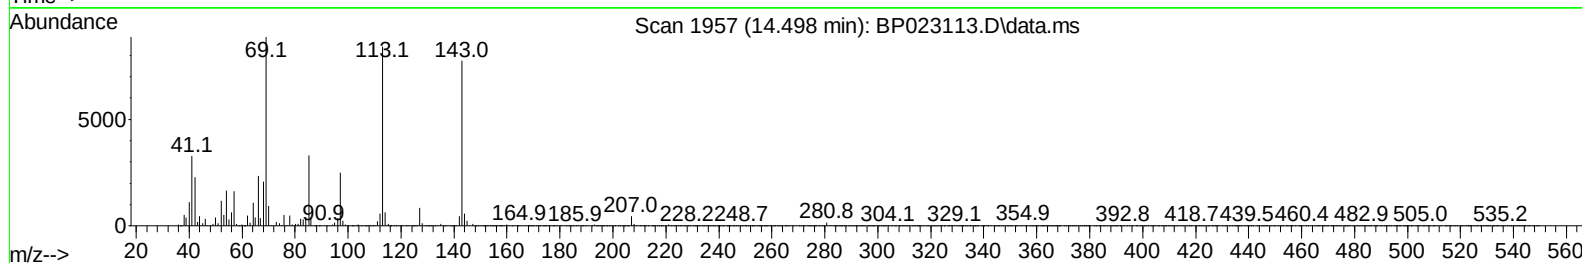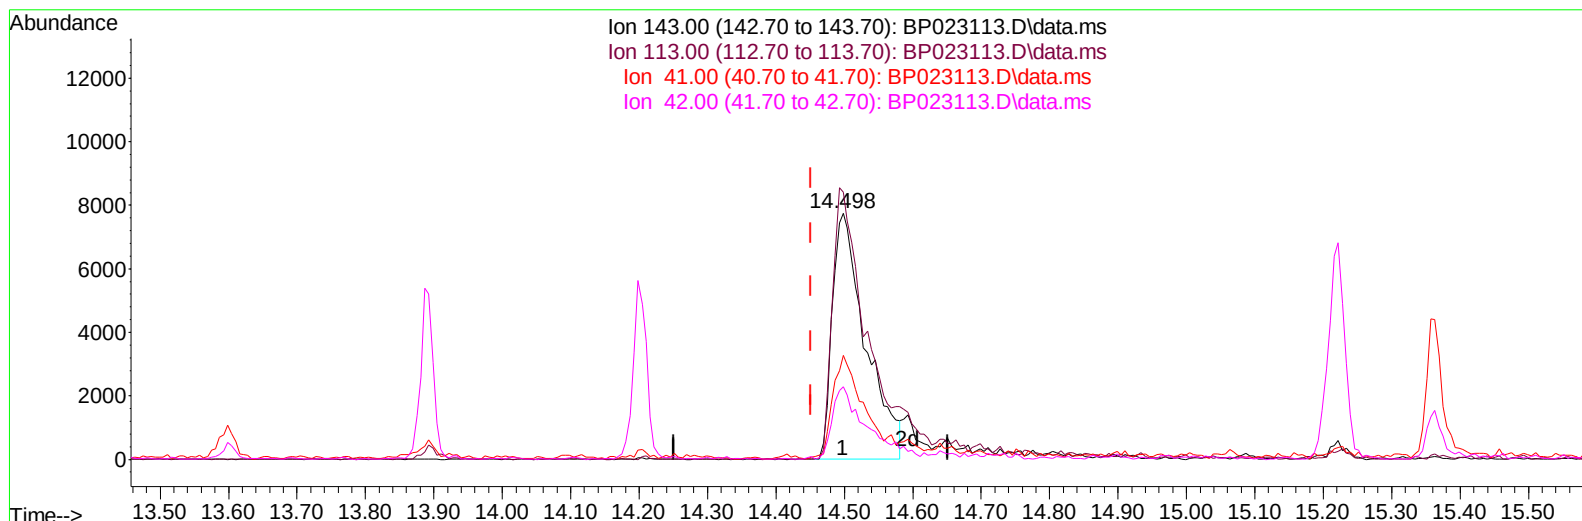

TIC: BP023113.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.498min (+ 0.047) 10.49 ng/ul

response 26087

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	108.51
41.00	39.20	42.30
42.00	25.90	29.52




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023113.D
Acq On : 14 Nov 2024 20:27
Operator : RC/JU
Sample : P4802-11
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCPD3

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:46:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

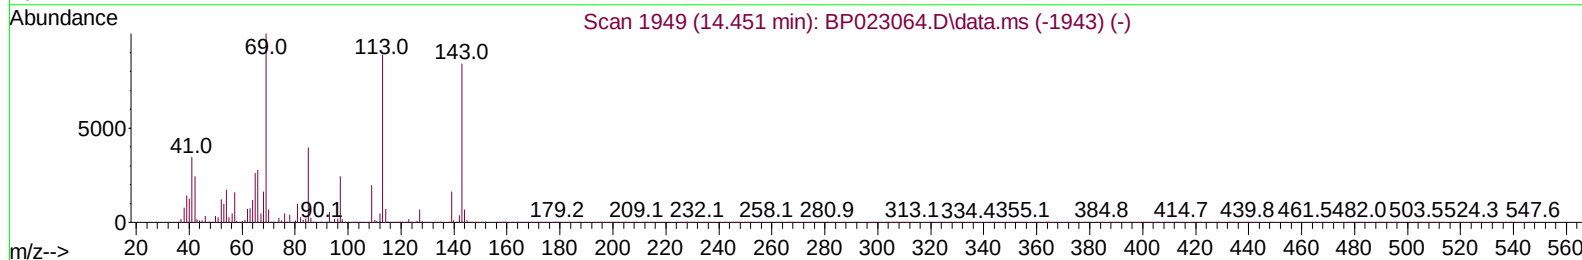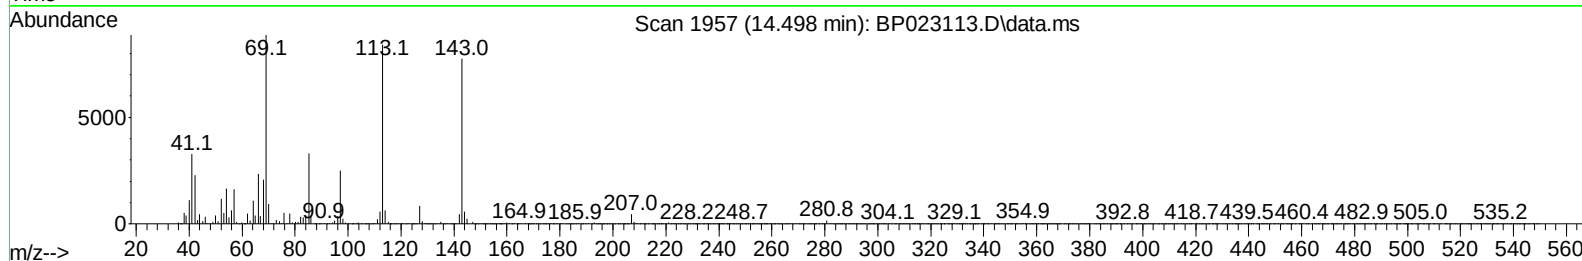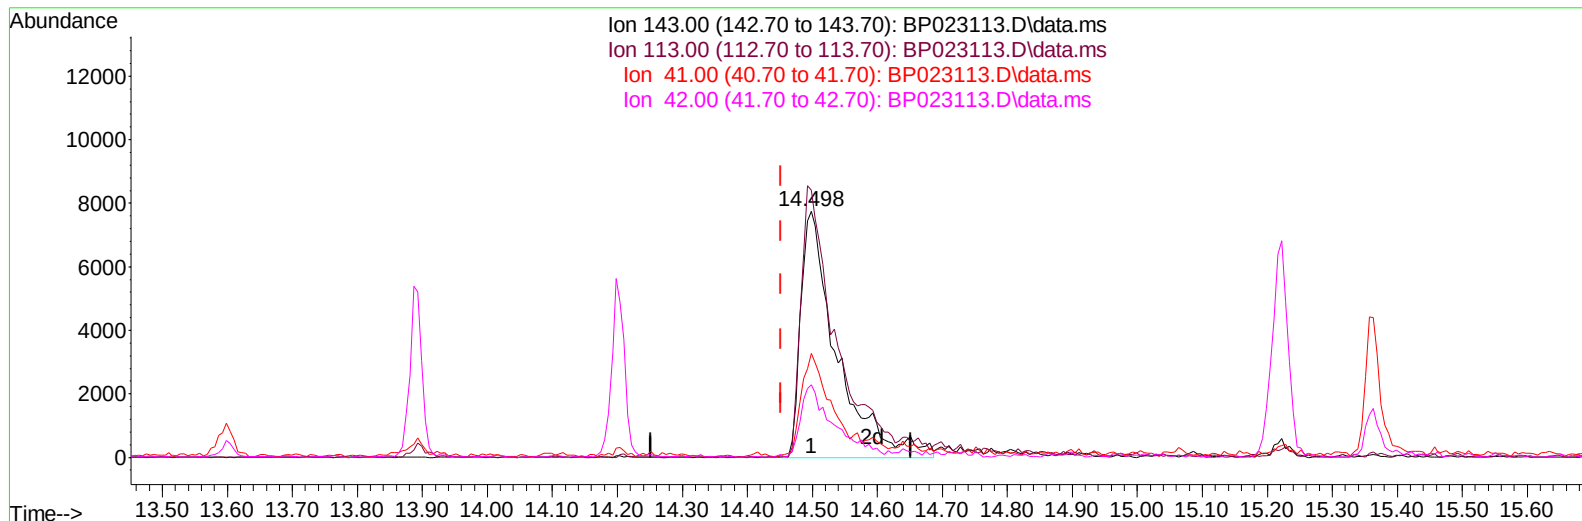

TIC: BP023113.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.498min (+ 0.047) 11.96 ng/ul m

response 29741

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	108.51
41.00	39.20	42.30
42.00	25.90	29.52

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023113.D
 Acq On : 14 Nov 2024 20:27
 Operator : RC/JU
 Sample : P4802-11
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCPD3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 15 00:48:18 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.581	152	77841	20.000	ng/ul	0.00
20) Naphthalene-d8	10.328	136	287422	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.204	164	229544	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.016	188	563654	20.000	ng/ul	0.00
79) Chrysene-d12	21.439	240	697475	20.000	ng/ul	0.00
88) Perylene-d12	24.657	264	847436	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	8044	4.967	ng/uL	0.00
4) Pyridine-d5	3.576	84	12121m	2.519	ng/ul	0.03
7) Phenol-d5	6.793	99	58791	10.216	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	6.928	67	93905	27.773	ng/ul	0.00
11) 2-Chlorophenol-d4	7.128	132	109267	25.924	ng/ul	0.00
15) 4-Methylphenol-d8	8.293	113	98364	20.770	ng/ul	0.00
21) Nitrobenzene-d5	8.722	128	59937	29.954	ng/ul	0.00
24) 2-Nitrophenol-d4	9.434	143	73066	30.629	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.981	165	145356	29.096	ng/ul	0.01
31) 4-Chloroaniline-d4	10.546	131	2574m	0.432	ng/ul	0.06
46) Dimethylphthalate-d6	13.599	166	552981	33.425	ng/ul	-0.01
49) Acenaphthylene-d8	13.893	160	502956	29.136	ng/ul	0.00
54) 4-Nitrophenol-d4	14.498	143	29741m	11.962	ng/ul	0.05
60) Fluorene-d10	15.222	176	484614	33.411	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.363	200	107018	31.694	ng/ul	0.00
73) Anthracene-d10	17.104	188	855176	35.833	ng/ul	-0.01
81) Pyrene-d10	19.486	212	1200302	37.362	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.439	264	1520106	37.657	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.176	88	2937	1.570	ng/uL#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023113.D
Acq On : 14 Nov 2024 20:27
Operator : RC/JU
Sample : P4802-11
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCPD3

Manual IntegrationsAPPROVED

Quant Time: Nov 15 00:48:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

