




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023121.D
Acq On : 15 Nov 2024 02:33
Operator : RC/JU
Sample : P4801-12
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCPB3

Manual IntegrationsAPPROVED

Quant Time: Nov 15 03:02:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

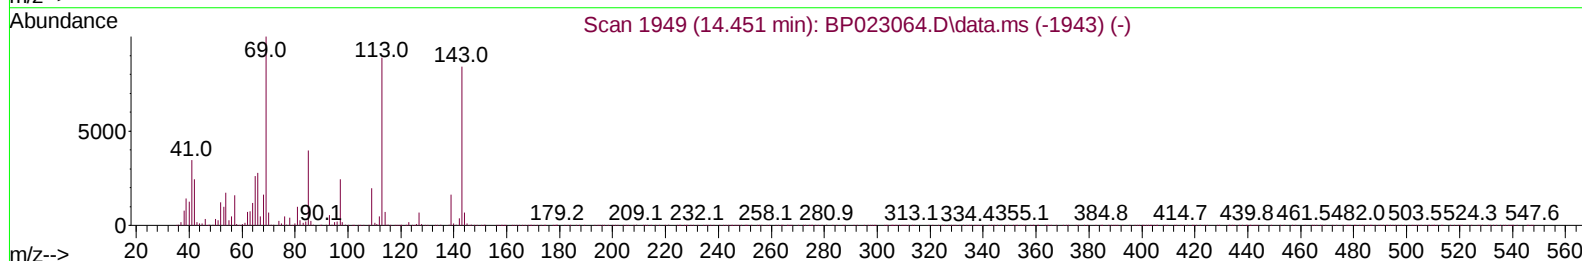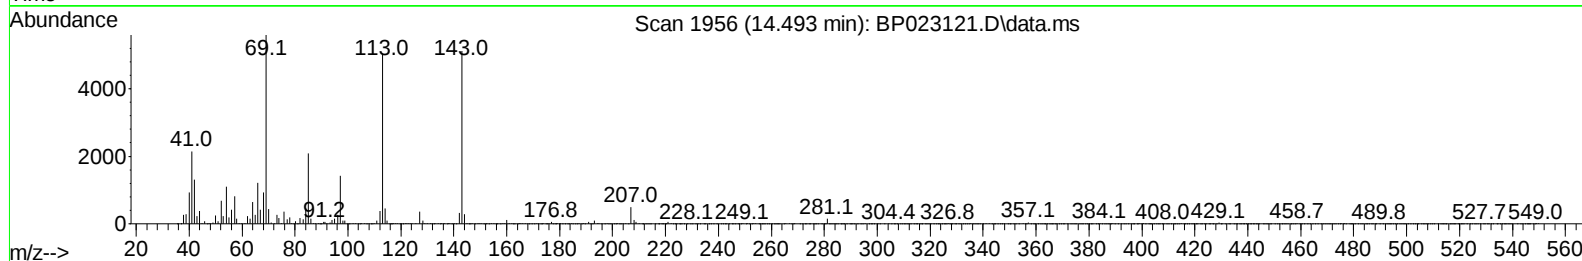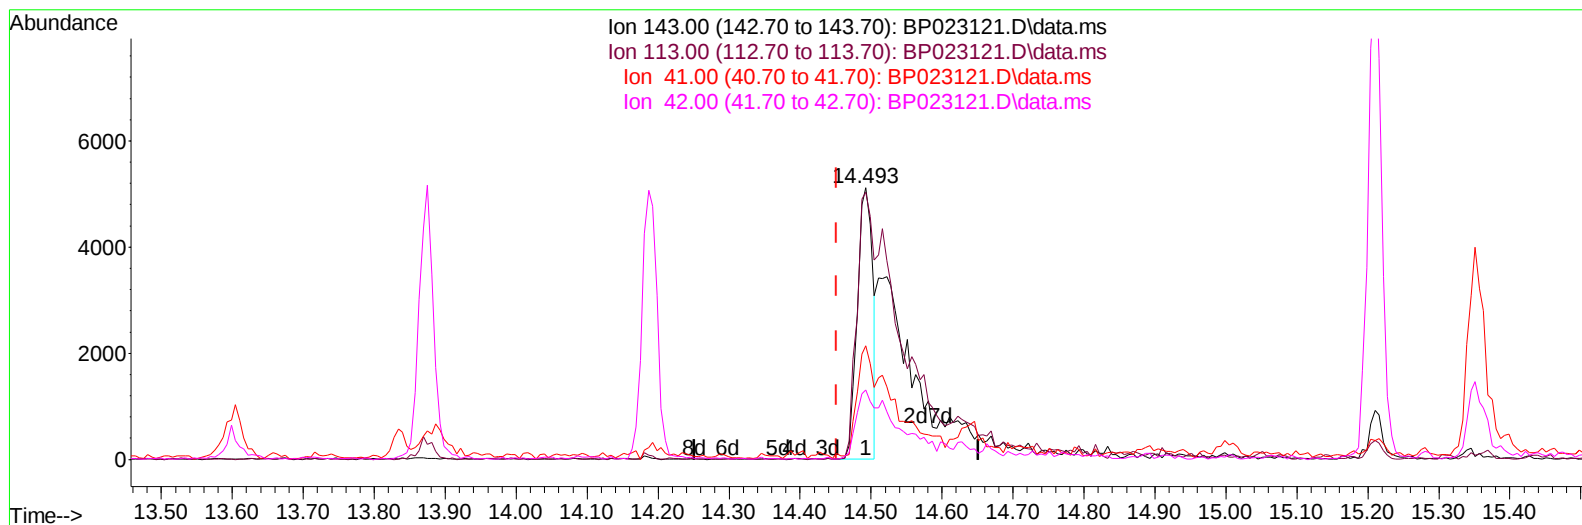

TIC: BP023121.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.493min (+ 0.041) 3.27 ng/u1

response 7706

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	98.48
41.00	39.20	41.88
42.00	25.90	25.67




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023121.D
Acq On : 15 Nov 2024 02:33
Operator : RC/JU
Sample : P4801-12
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCPB3

Manual IntegrationsAPPROVED

Quant Time: Nov 15 03:02:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

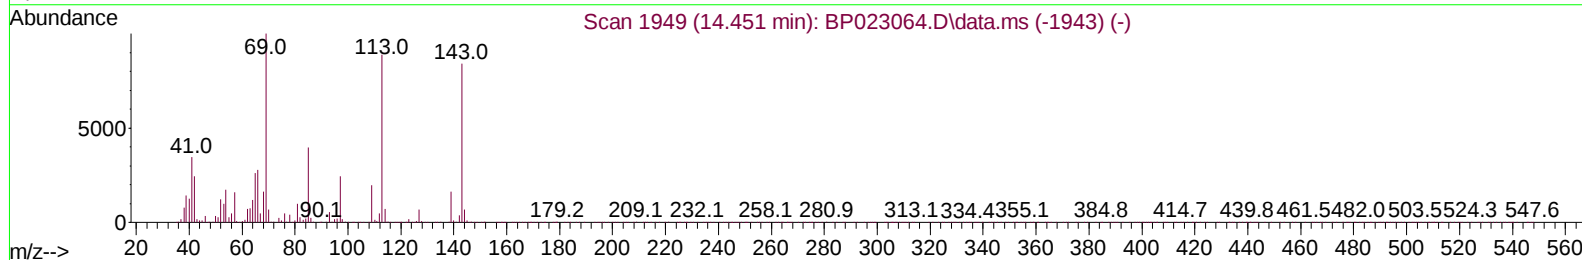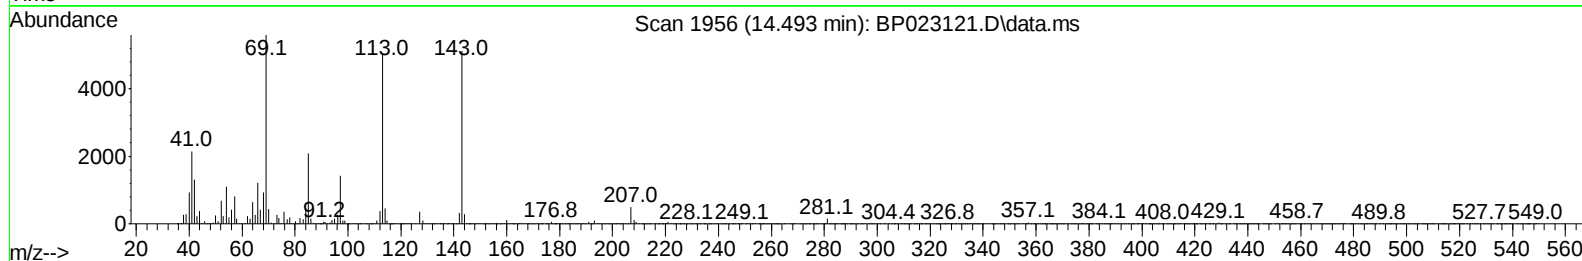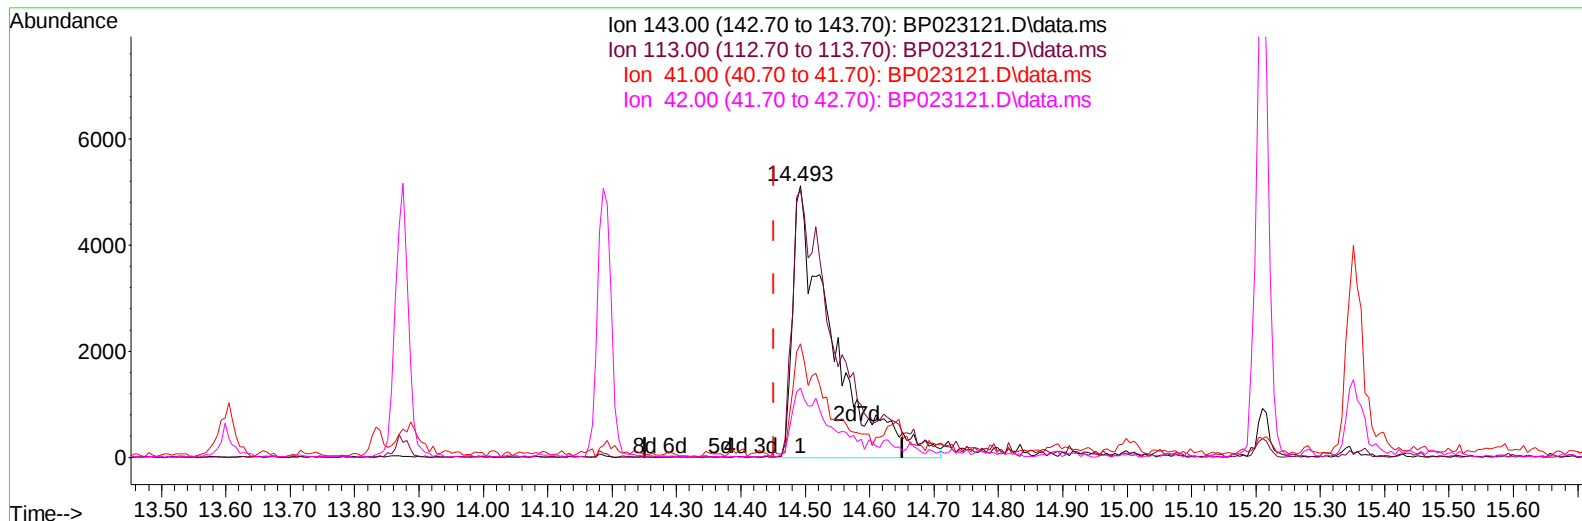

TIC: BP023121.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.493min (+ 0.041) 9.17 ng/ul m

response 21638

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	98.48
41.00	39.20	41.88
42.00	25.90	25.67

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023121.D
 Acq On : 15 Nov 2024 02:33
 Operator : RC/JU
 Sample : P4801-12
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCPB3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 15 03:03:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.575	152	70778	20.000	ng/ul	0.00
20) Naphthalene-d8	10.322	136	268536	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.187	164	217758	20.000	ng/ul	-0.02
64) Phenanthrene-d10	17.004	188	545330	20.000	ng/ul	-0.01
79) Chrysene-d12	21.433	240	798517	20.000	ng/ul	-0.01
88) Perylene-d12	24.645	264	961674	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	6354	4.315	ng/uL	0.00
4) Pyridine-d5	3.558	84	23191	5.301	ng/ul	0.01
7) Phenol-d5	6.787	99	39525	7.553	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.922	67	89464	29.100	ng/ul	0.00
11) 2-Chlorophenol-d4	7.122	132	101184	26.402	ng/ul	0.00
15) 4-Methylphenol-d8	8.287	113	75502	17.534	ng/ul	0.00
21) Nitrobenzene-d5	8.722	128	56655	30.305	ng/ul	0.00
24) 2-Nitrophenol-d4	9.428	143	68392	30.686	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.969	165	131935	28.267	ng/ul	0.00
31) 4-Chloroaniline-d4	10.481	131	94076	16.895	ng/ul	0.00
46) Dimethylphthalate-d6	13.598	166	548927	34.976	ng/ul	-0.01
49) Acenaphthylene-d8	13.875	160	545081	33.285	ng/ul	-0.02
54) 4-Nitrophenol-d4	14.493	143	21638m	9.174	ng/ul	0.04
60) Fluorene-d10	15.210	176	492266	35.775	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.351	200	100017	30.616	ng/ul	-0.01
73) Anthracene-d10	17.098	188	849296	36.782	ng/ul	-0.02
81) Pyrene-d10	19.498	212	1253657	34.085	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.433	264	1768047	38.597	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023121.D
Acq On : 15 Nov 2024 02:33
Operator : RC/JU
Sample : P4801-12
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCPB3

Manual IntegrationsAPPROVED

Quant Time: Nov 15 03:03:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

