




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023127.D
Acq On : 15 Nov 2024 06:38
Operator : RC/JU
Sample : P4740-06
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE7

Manual IntegrationsAPPROVED

Quant Time: Nov 15 07:45:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

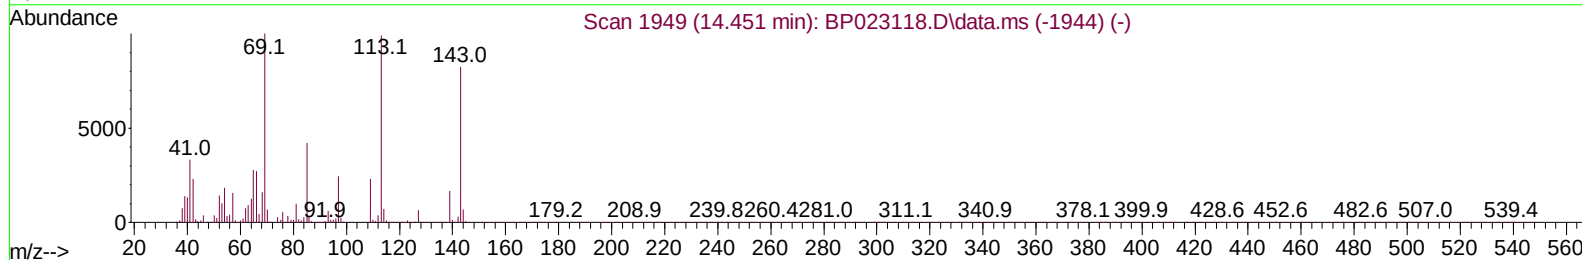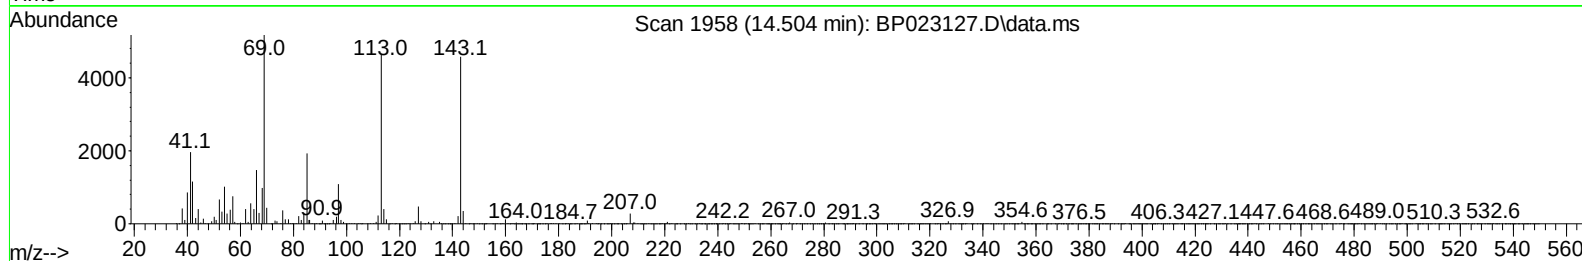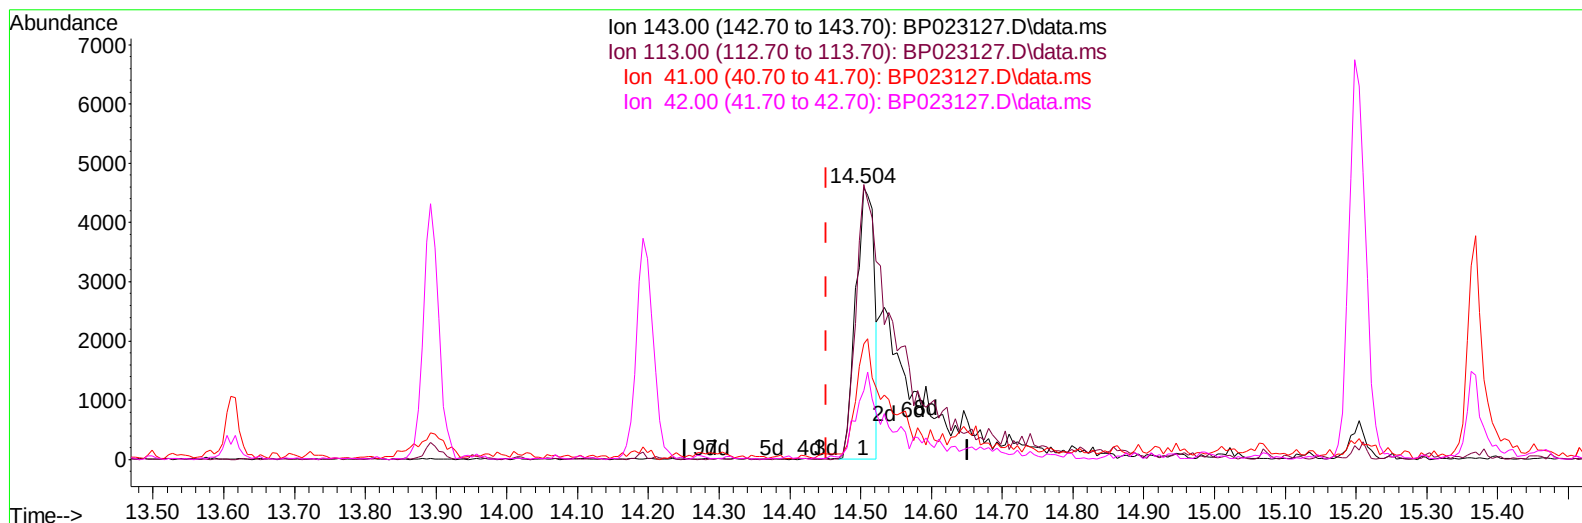

TIC: BP023127.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.504min (+ 0.053) 4.21 ng/ul

response 8346

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	101.35
41.00	39.20	42.69
42.00	25.90	25.39




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023127.D
Acq On : 15 Nov 2024 06:38
Operator : RC/JU
Sample : P4740-06
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE7

Manual IntegrationsAPPROVED

Quant Time: Nov 15 07:45:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

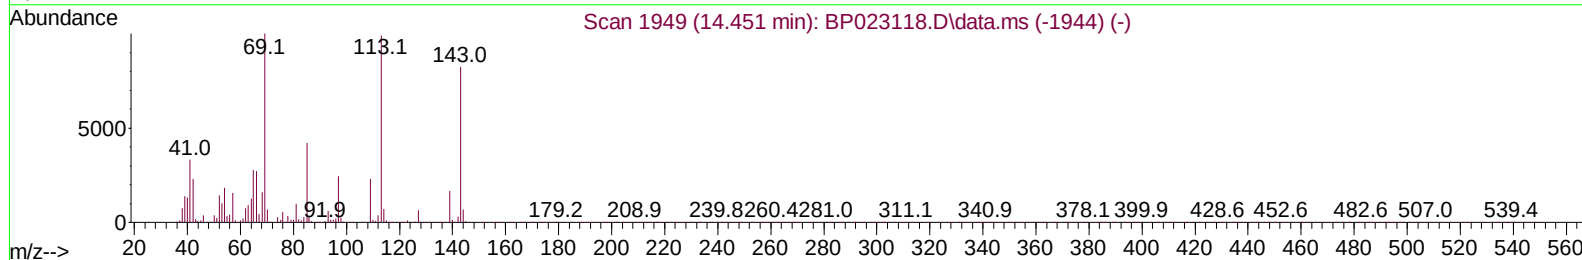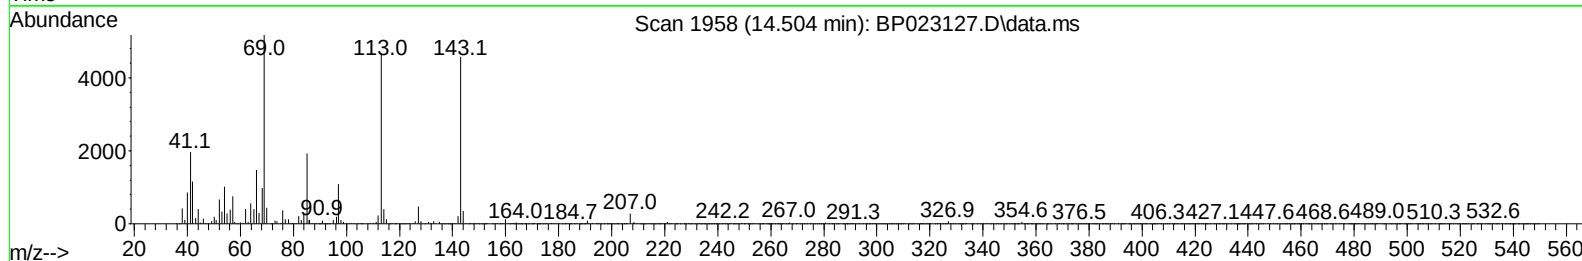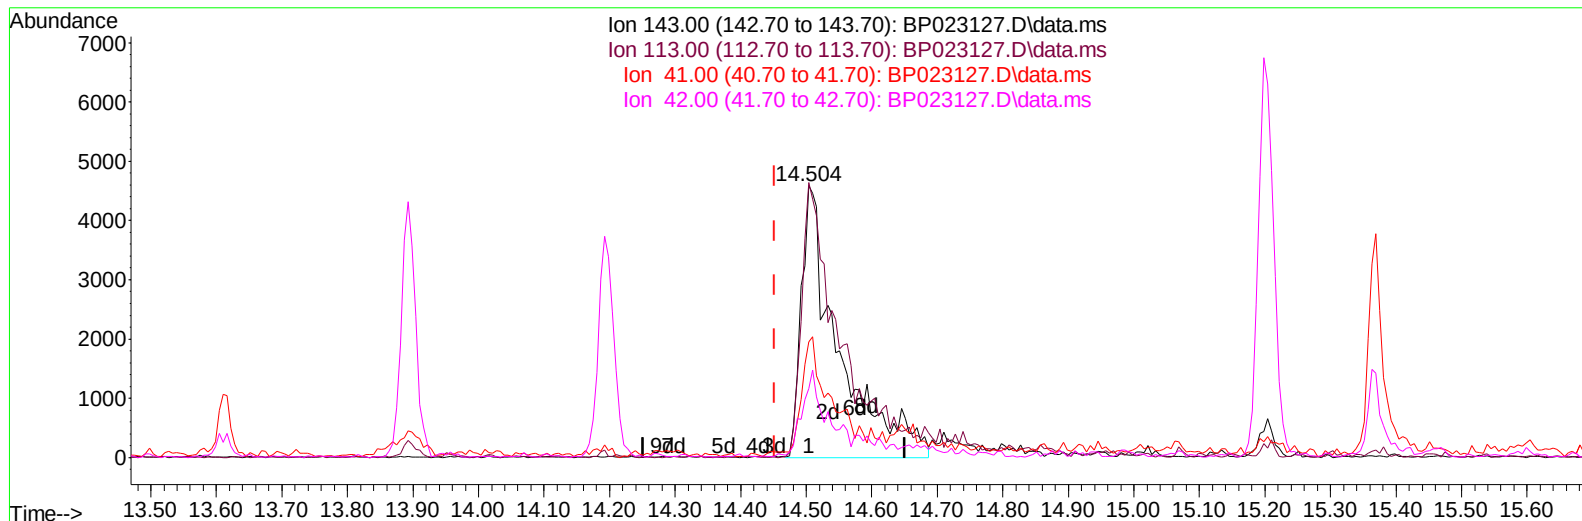

TIC: BP023127.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.504min (+ 0.053) 9.18 ng/ul m

response 18196

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	101.35
41.00	39.20	42.69
42.00	25.90	25.39

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023127.D
 Acq On : 15 Nov 2024 06:38
 Operator : RC/JU
 Sample : P4740-06
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CE7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 15 07:45:50 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.581	152	59770	20.000	ng/ul	0.00
20) Naphthalene-d8	10.328	136	223849	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.198	164	183094	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.992	188	472776	20.000	ng/ul	-0.02
79) Chrysene-d12	21.451	240	547132	20.000	ng/ul	0.00
88) Perylene-d12	24.674	264	677797	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	6993	5.624	ng/uL	0.00
4) Pyridine-d5	3.558	84	39444	10.677	ng/ul	0.01
7) Phenol-d5	6.793	99	42027	9.511	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	6.928	67	85887	33.081	ng/ul	0.00
11) 2-Chlorophenol-d4	7.134	132	95063	29.374	ng/ul	0.00
15) 4-Methylphenol-d8	8.299	113	78170	21.496	ng/ul	0.00
21) Nitrobenzene-d5	8.728	128	53254	34.173	ng/ul	0.00
24) 2-Nitrophenol-d4	9.440	143	62796	33.800	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.981	165	126444	32.499	ng/ul	0.01
31) 4-Chloroaniline-d4	10.487	131	134617	29.002	ng/ul	0.00
46) Dimethylphthalate-d6	13.616	166	511531	38.764	ng/ul	0.00
49) Acenaphthylene-d8	13.892	160	490991	35.659	ng/ul	0.00
54) 4-Nitrophenol-d4	14.504	143	18196m	9.175	ng/ul	0.05
60) Fluorene-d10	15.204	176	432399	37.373	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.369	200	88586	31.279	ng/ul	0.00
73) Anthracene-d10	17.110	188	769952	38.463	ng/ul	0.00
81) Pyrene-d10	19.498	212	1038382	41.204	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.445	264	1299530	40.250	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023127.D
Acq On : 15 Nov 2024 06:38
Operator : RC/JU
Sample : P4740-06
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 15 07:45:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

