




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023128.D
Acq On : 15 Nov 2024 07:18
Operator : RC/JU
Sample : P4784-03
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27N1

Manual IntegrationsAPPROVED

Quant Time: Nov 15 07:49:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

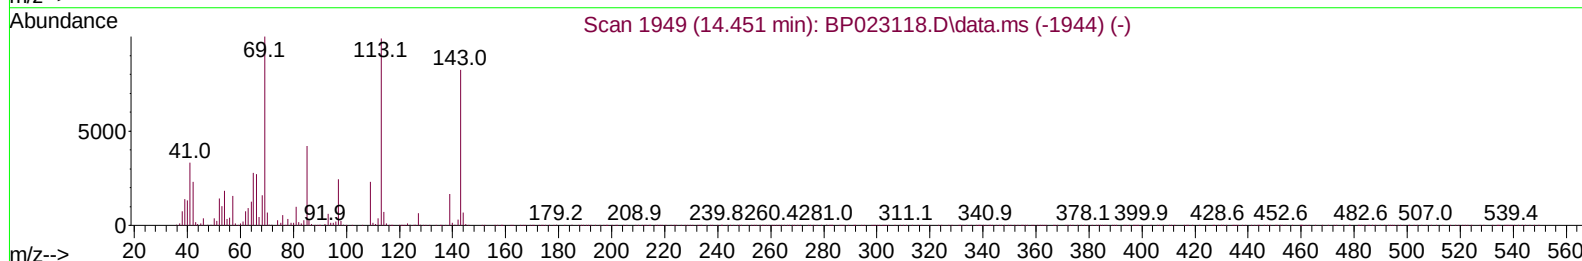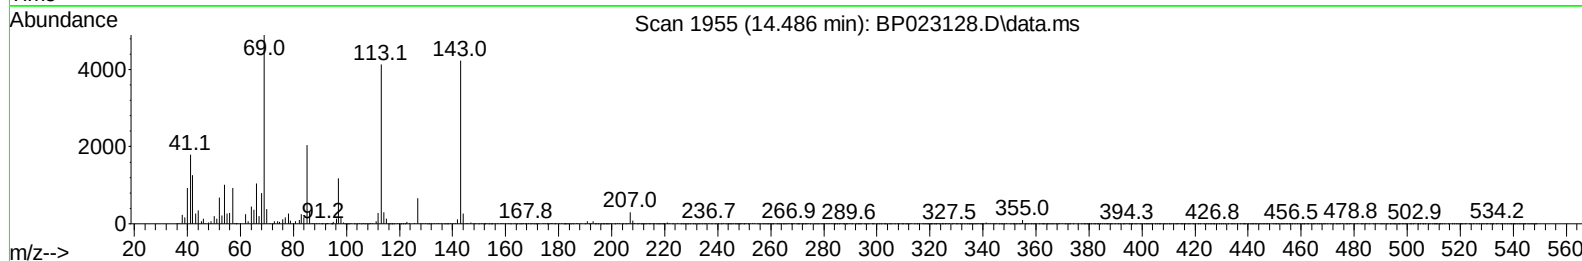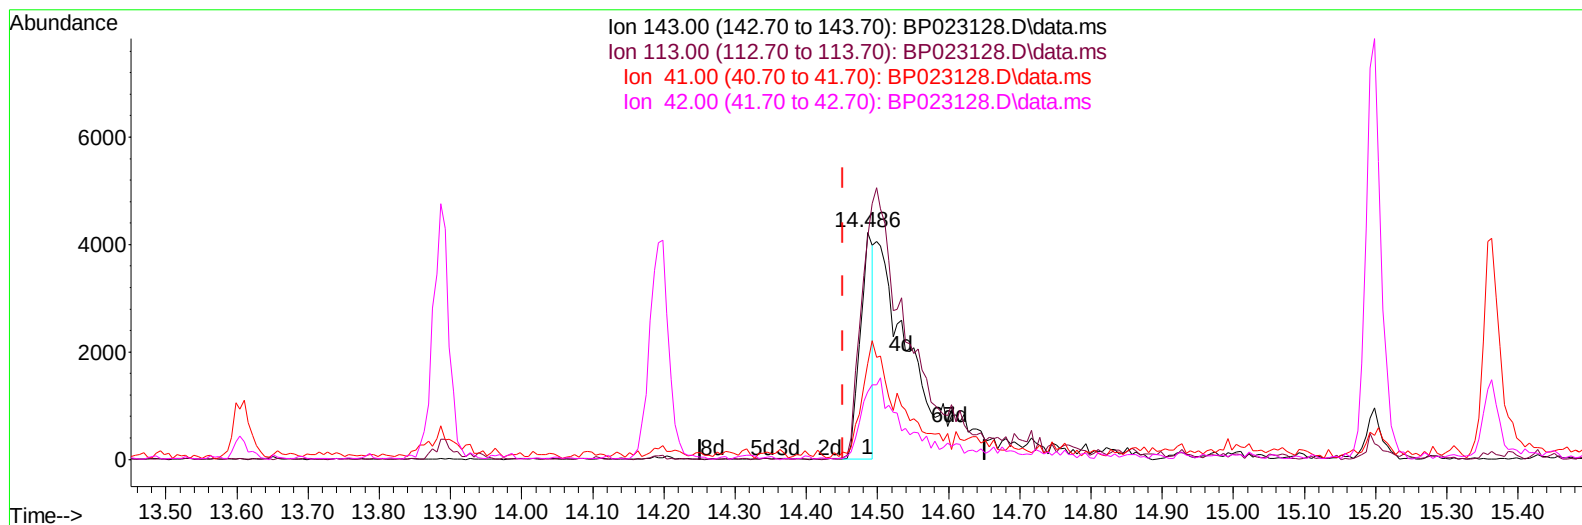

TIC: BP023128.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.486min (+ 0.035) 2.28 ng/ul

response 5283

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	97.52
41.00	39.20	42.28
42.00	25.90	29.84




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023128.D
Acq On : 15 Nov 2024 07:18
Operator : RC/JU
Sample : P4784-03
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27N1

Manual IntegrationsAPPROVED

Quant Time: Nov 15 07:49:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

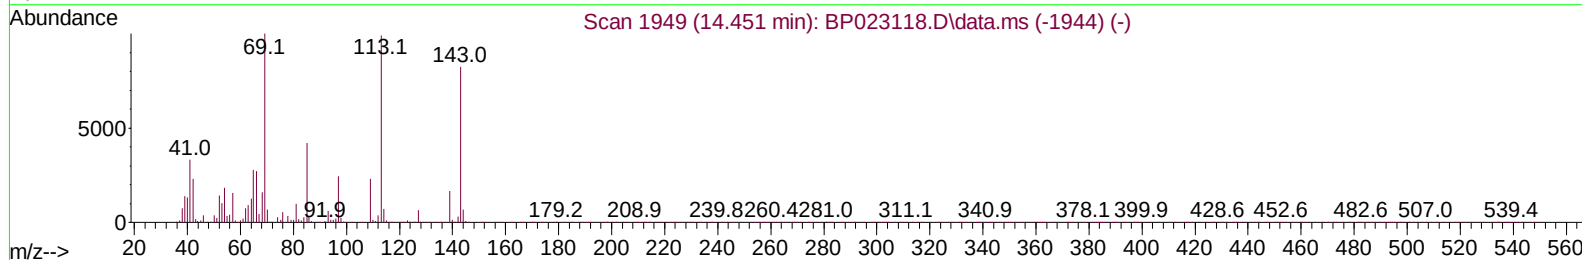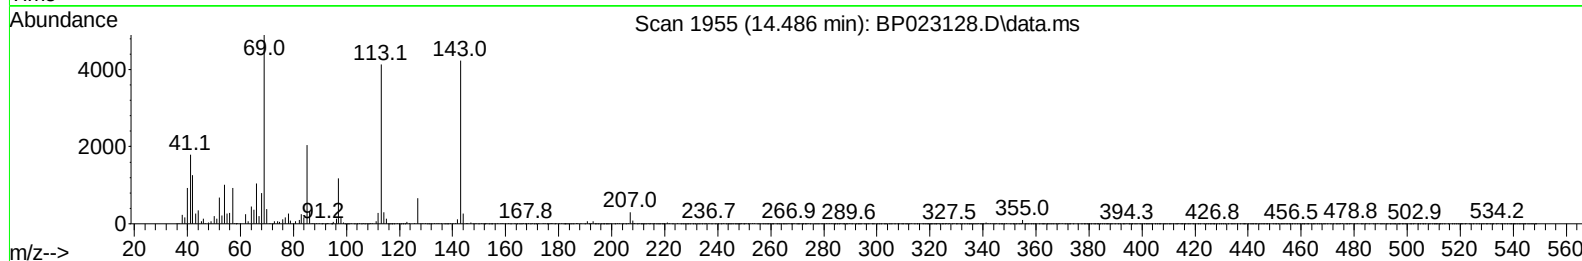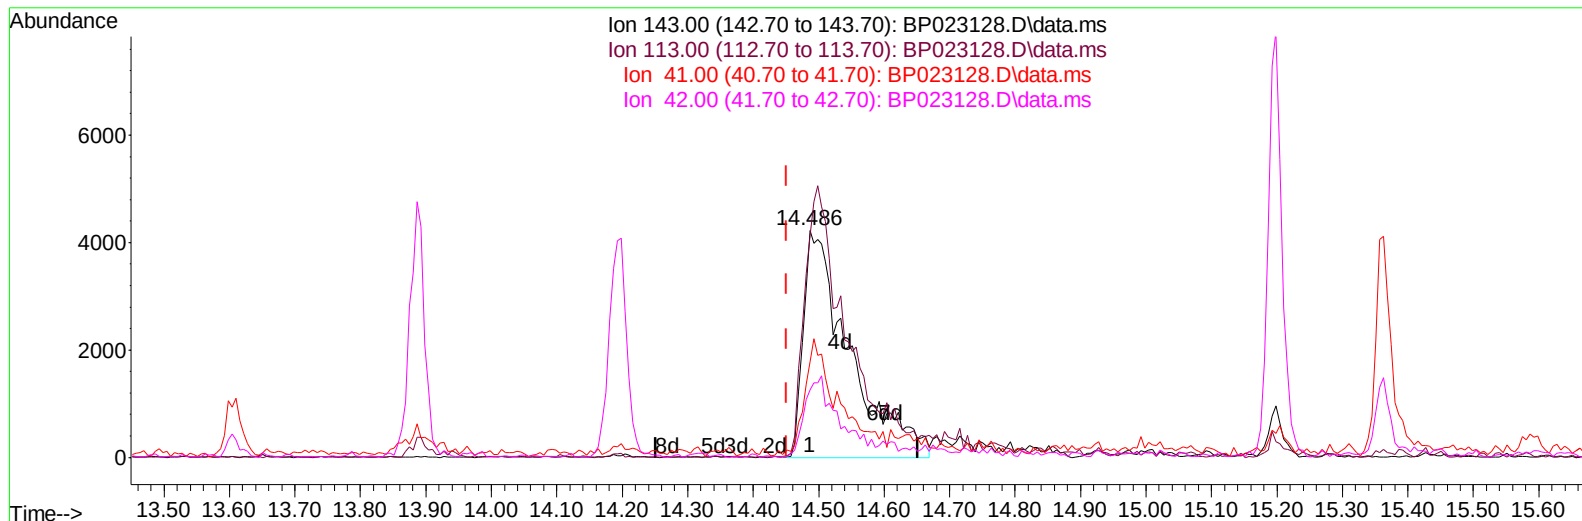

TIC: BP023128.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.486min (+ 0.035) 8.90 ng/ul m

response 20646

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	97.52
41.00	39.20	42.28
42.00	25.90	29.84

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023128.D
 Acq On : 15 Nov 2024 07:18
 Operator : RC/JU
 Sample : P4784-03
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E27N1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 15 07:50:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.581	152	68124	20.000	ng/ul	0.00
20) Naphthalene-d8	10.322	136	261450	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.198	164	214133	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.992	188	553191	20.000	ng/ul	-0.02
79) Chrysene-d12	21.439	240	672795	20.000	ng/ul	0.00
88) Perylene-d12	24.662	264	815697	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	7403	5.223	ng/uL	0.00
4) Pyridine-d5	3.552	84	45179	10.729	ng/ul	0.00
7) Phenol-d5	6.787	99	55097	10.939	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.928	67	94178	31.827	ng/ul	0.00
11) 2-Chlorophenol-d4	7.122	132	107332	29.098	ng/ul	0.00
15) 4-Methylphenol-d8	8.293	113	99067	23.902	ng/ul	0.00
21) Nitrobenzene-d5	8.722	128	60398	33.183	ng/ul	0.00
24) 2-Nitrophenol-d4	9.434	143	71975	33.169	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.969	165	140926	31.012	ng/ul	0.00
31) 4-Chloroaniline-d4	10.475	131	158501	29.237	ng/ul	0.00
46) Dimethylphthalate-d6	13.610	166	550991	35.702	ng/ul	0.00
49) Acenaphthylene-d8	13.886	160	525943	32.660	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.486	143	20646m	8.902	ng/ul	0.04
60) Fluorene-d10	15.198	176	480183	35.488	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.363	200	107265	32.368	ng/ul	0.00
73) Anthracene-d10	17.104	188	886565	37.851	ng/ul	-0.01
81) Pyrene-d10	19.492	212	1197755	38.650	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.433	264	1512840	38.936	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023128.D
Acq On : 15 Nov 2024 07:18
Operator : RC/JU
Sample : P4784-03
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27N1

Manual IntegrationsAPPROVED

Quant Time: Nov 15 07:50:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/18/2024

