




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023130.D
Acq On : 15 Nov 2024 08:39
Operator : RC/JU
Sample : P4784-05
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27N3

Manual IntegrationsAPPROVED

Quant Time: Nov 15 22:16:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/16/2024
Supervised By :mohammad ahmed 11/18/2024

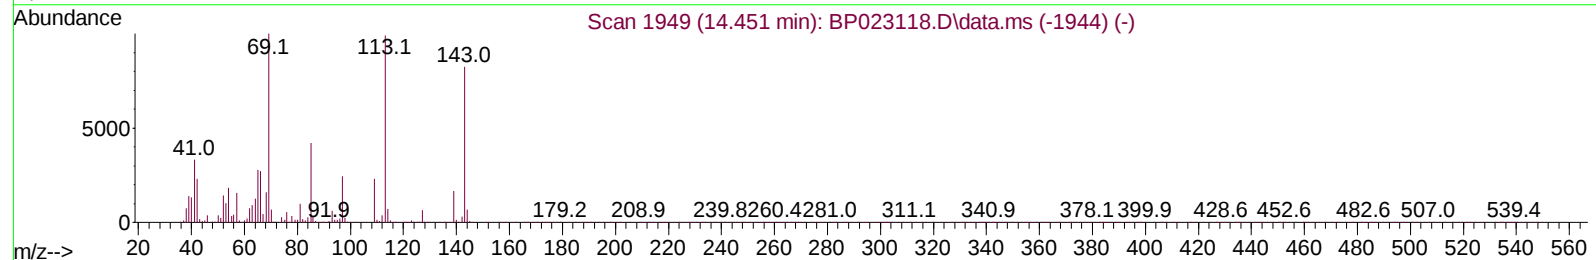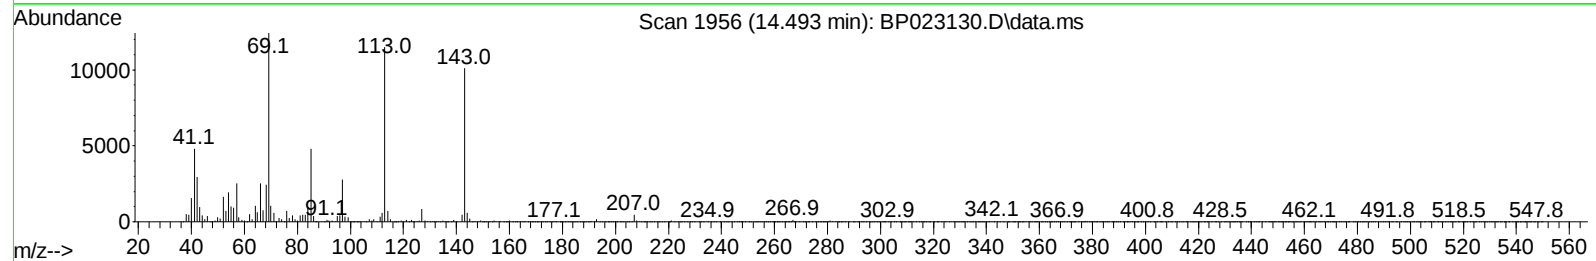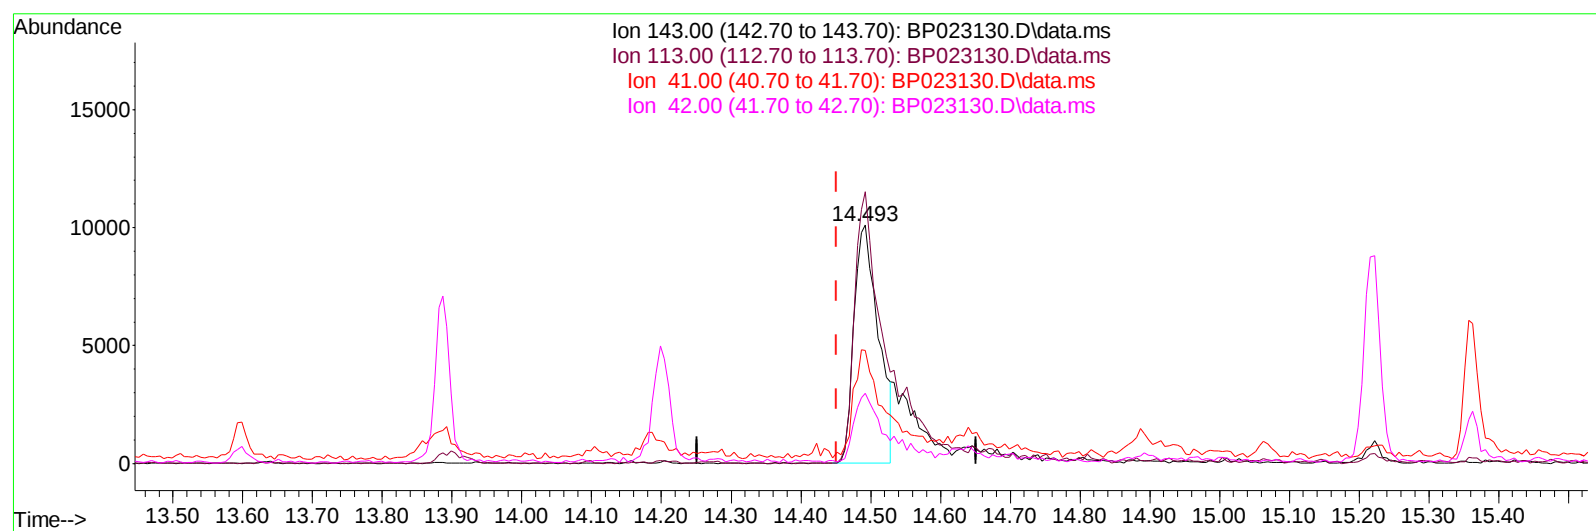

TIC: BP023130.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.493min (+ 0.041) 9.19 ng/u1

response 24574

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	113.96
41.00	39.20	47.51#
42.00	25.90	29.39




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023130.D
Acq On : 15 Nov 2024 08:39
Operator : RC/JU
Sample : P4784-05
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27N3

Manual IntegrationsAPPROVED

Quant Time: Nov 15 22:16:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/16/2024
Supervised By :mohammad ahmed 11/18/2024

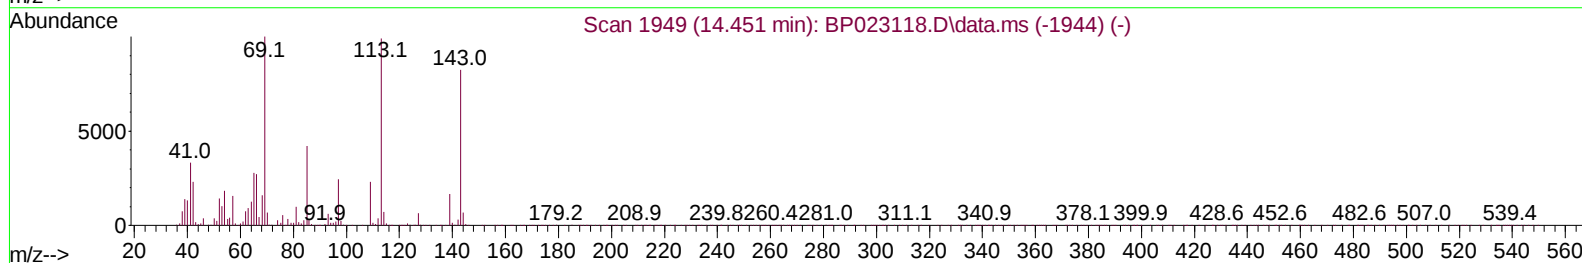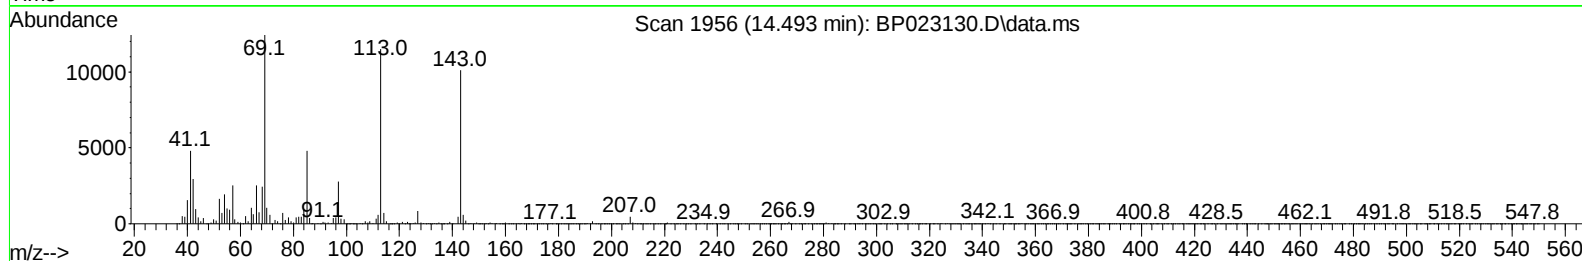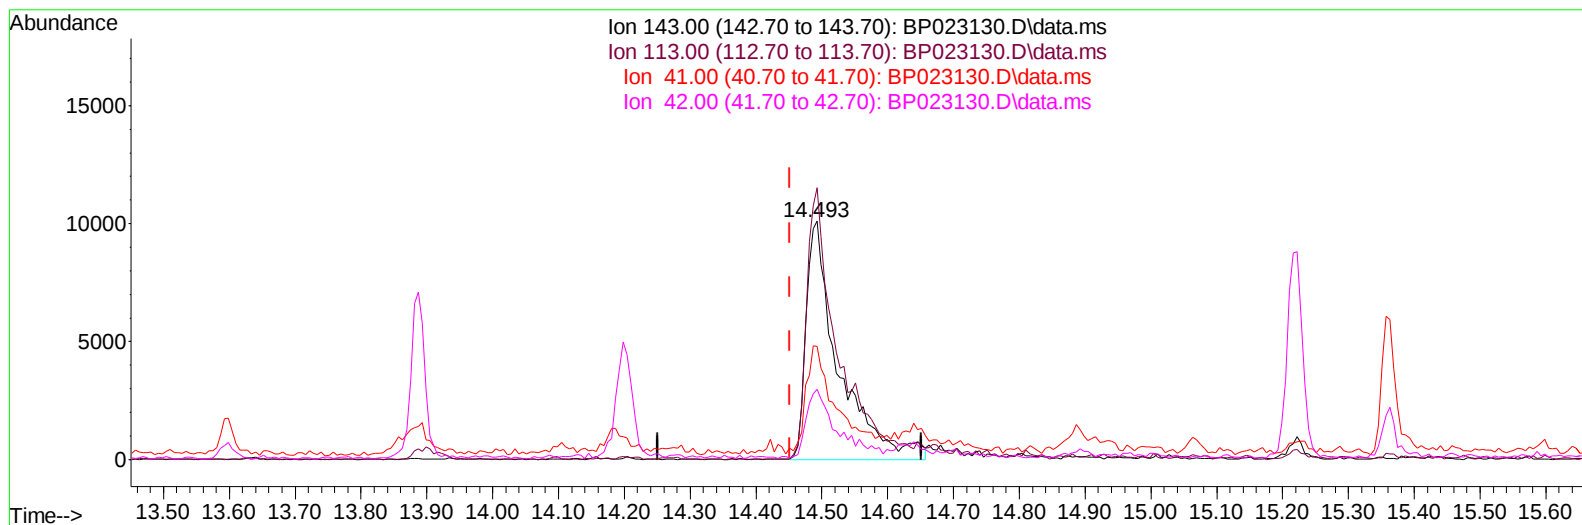

TIC: BP023130.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.493min (+ 0.041) 13.00 ng/ul m

response 34763

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	113.96
41.00	39.20	47.51#
42.00	25.90	29.39

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023130.D
 Acq On : 15 Nov 2024 08:39
 Operator : RC/JU
 Sample : P4784-05
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E27N3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/16/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 15 22:20:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.581	152	81255	20.000	ng/ul	0.00
20) Naphthalene-d8	10.328	136	310381	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.198	164	246872	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.010	188	621953	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.451	240	792718	20.000	ng/ul	0.00
88) Perylene-d12	24.663	264	918208	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	10997	6.505	ng/uL	0.00
4) Pyridine-d5	3.552	84	69478	13.834	ng/ul	0.00
7) Phenol-d5	6.787	99	80607	13.418	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.928	67	133543	37.837	ng/ul	0.00
11) 2-Chlorophenol-d4	7.128	132	162482	36.930	ng/ul	0.00
15) 4-Methylphenol-d8	8.287	113	133699	27.045	ng/ul	0.00
21) Nitrobenzene-d5	8.722	128	85875	39.742	ng/ul	0.00
24) 2-Nitrophenol-d4	9.434	143	102887	39.940	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.975	165	211579	39.220	ng/ul	0.00
31) 4-Chloroaniline-d4	10.481	131	145753	22.647	ng/ul	0.00
46) Dimethylphthalate-d6	13.598	166	736808	41.410	ng/ul	-0.01
49) Acenaphthylene-d8	13.887	160	751815	40.495	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.493	143	34763m	13.001	ng/ul	0.04
60) Fluorene-d10	15.222	176	637786	40.884	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.363	200	132226	35.489	ng/ul	0.00
73) Anthracene-d10	17.110	188	1095162	41.587	ng/ul	0.00
81) Pyrene-d10	19.486	212	1460220	39.992	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.445	264	1825850	41.745	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023130.D
Acq On : 15 Nov 2024 08:39
Operator : RC/JU
Sample : P4784-05
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27N3

Manual IntegrationsAPPROVED

Quant Time: Nov 15 22:20:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/16/2024
Supervised By :mohammad ahmed 11/18/2024

