




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023131.D
Acq On : 15 Nov 2024 09:19
Operator : RC/JU
Sample : P4740-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE5

Manual IntegrationsAPPROVED

Quant Time: Nov 15 22:23:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/16/2024
Supervised By :mohammad ahmed 11/18/2024

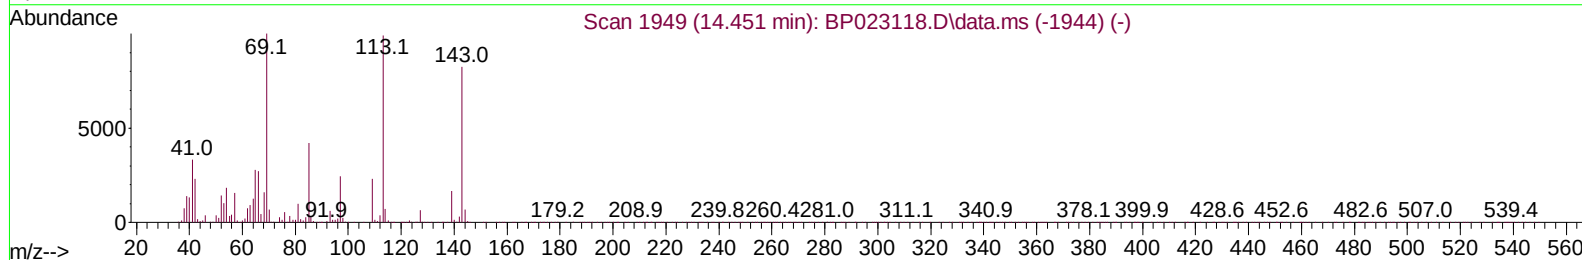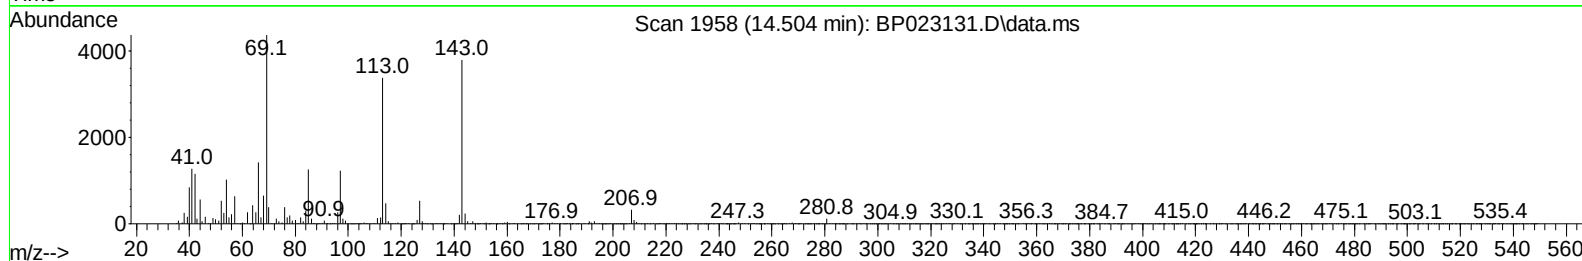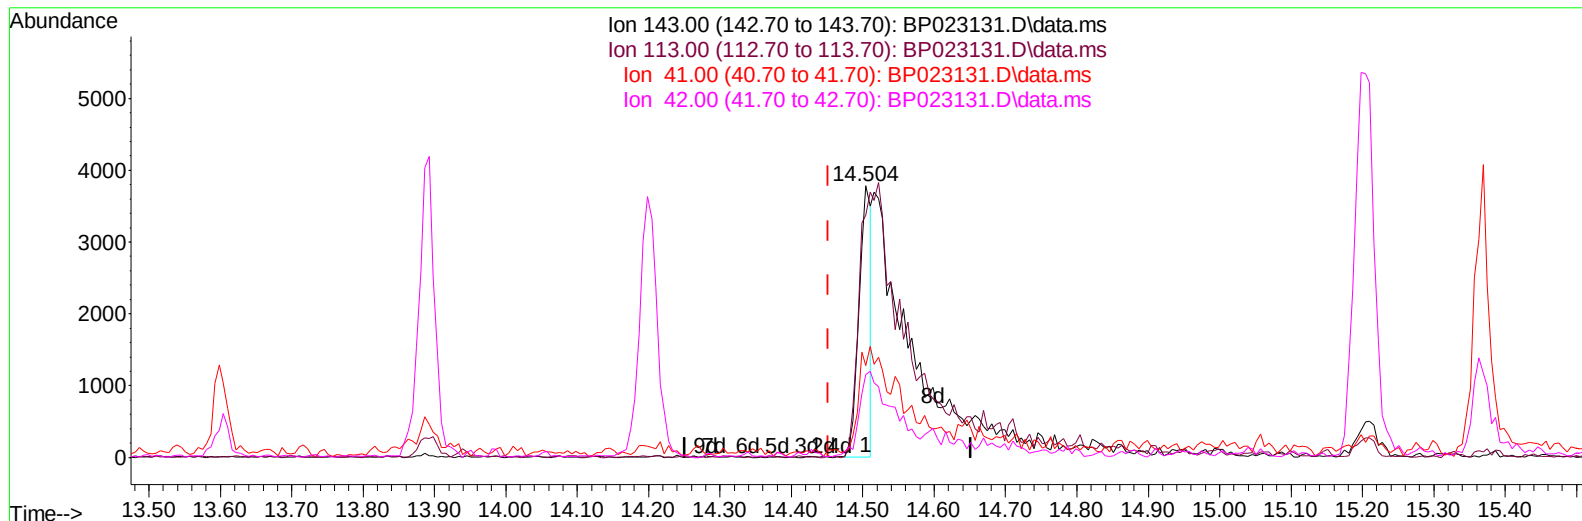

TIC: BP023131.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.504min (+ 0.053) 1.98 ng/u1

response 4409

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	89.37
41.00	39.20	33.75
42.00	25.90	30.47




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023131.D
Acq On : 15 Nov 2024 09:19
Operator : RC/JU
Sample : P4740-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE5

Manual IntegrationsAPPROVED

Quant Time: Nov 15 22:23:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/16/2024
Supervised By :mohammad ahmed 11/18/2024

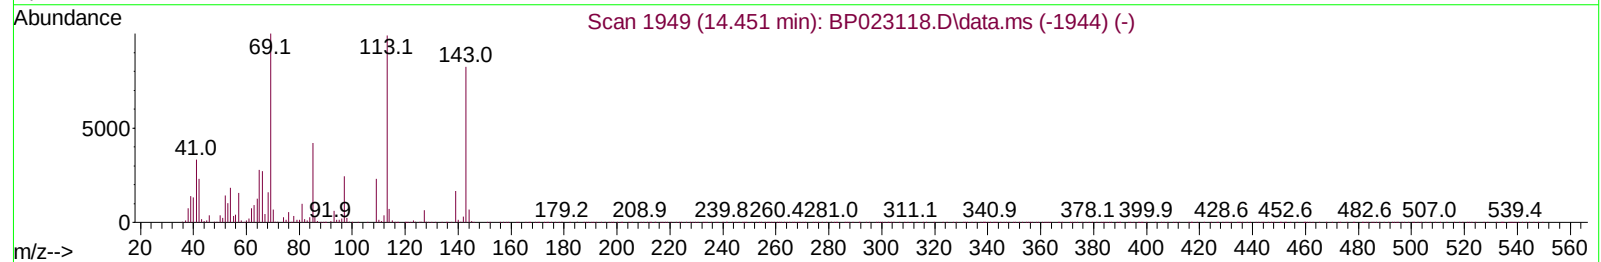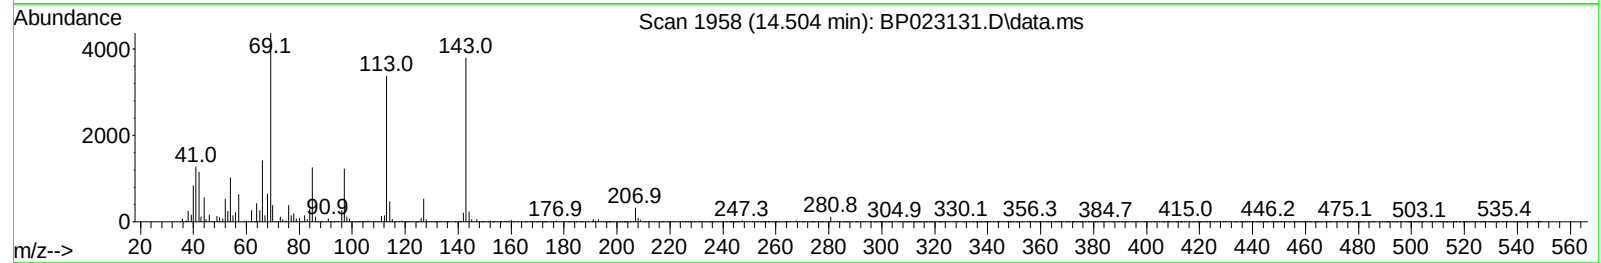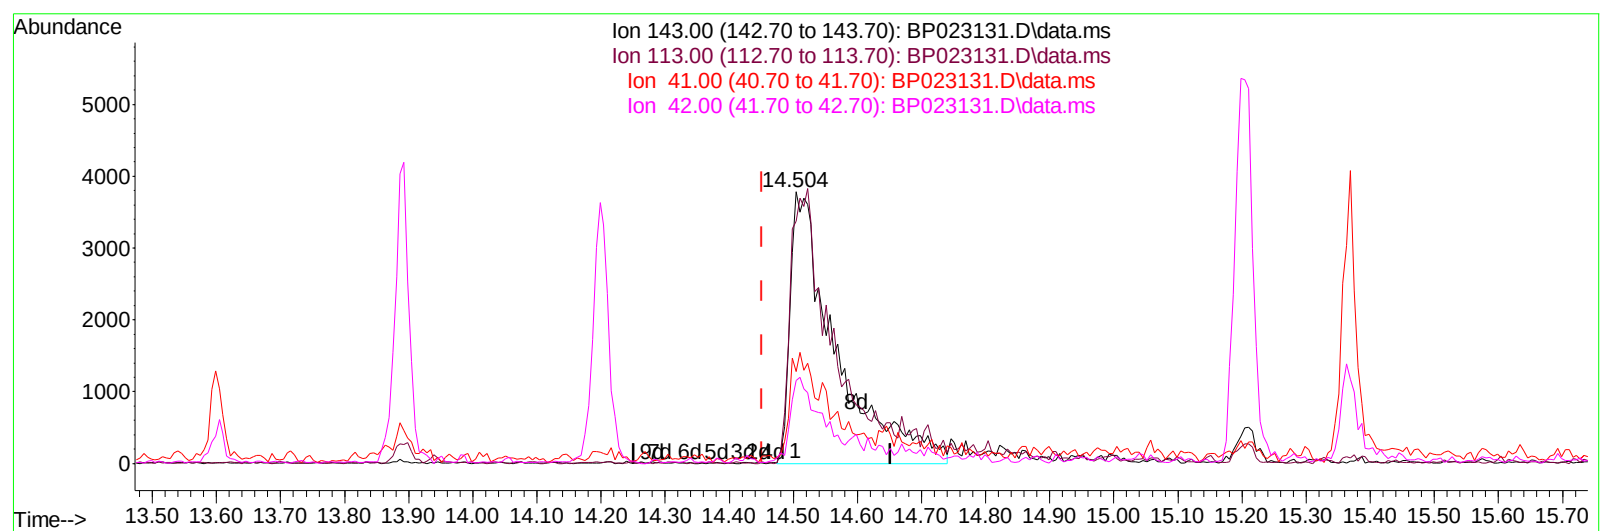

TIC: BP023131.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.504min (+ 0.053) 8.43 ng/ul m

response 18735

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	107.90	89.37
41.00	39.20	33.75
42.00	25.90	30.47

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023131.D
 Acq On : 15 Nov 2024 09:19
 Operator : RC/JU
 Sample : P4740-01
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CE5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/16/2024
 Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 15 22:24:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 04:49:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.581	152	68029	20.000	ng/ul	0.00
20) Naphthalene-d8	10.328	136	254182	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.198	164	205096	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.004	188	527367	20.000	ng/ul	-0.01
79) Chrysene-d12	21.445	240	615197	20.000	ng/ul	0.00
88) Perylene-d12	24.674	264	726931	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	6549	4.627	ng/uL	0.00
4) Pyridine-d5	3.570	84	9674	2.301	ng/ul	0.02
7) Phenol-d5	6.793	99	40384	8.029	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	6.928	67	92133	31.179	ng/ul	0.00
11) 2-Chlorophenol-d4	7.128	132	102946	27.948	ng/ul	0.00
15) 4-Methylphenol-d8	8.299	113	78550	18.979	ng/ul	0.00
21) Nitrobenzene-d5	8.728	128	58731	33.190	ng/ul	0.00
24) 2-Nitrophenol-d4	9.434	143	71164	33.733	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.975	165	131616	29.791	ng/ul	0.00
31) 4-Chloroaniline-d4	10.481	131	115776	21.966	ng/ul	0.00
46) Dimethylphthalate-d6	13.604	166	516808	34.962	ng/ul	0.00
49) Acenaphthylene-d8	13.893	160	516736	33.502	ng/ul	0.00
54) 4-Nitrophenol-d4	14.504	143	18735m	8.434	ng/ul	0.05
60) Fluorene-d10	15.204	176	453817	35.017	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.369	200	96785	30.636	ng/ul	0.00
73) Anthracene-d10	17.110	188	822818	36.849	ng/ul	0.00
81) Pyrene-d10	19.492	212	1070394	37.775	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.445	264	1277379	36.890	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023131.D
Acq On : 15 Nov 2024 09:19
Operator : RC/JU
Sample : P4740-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/16/2024
Supervised By :mohammad ahmed 11/18/2024

Quant Time: Nov 15 22:24:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 04:49:01 2024
Response via : Initial Calibration

