

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023107.D
 Acq On : 14 Nov 2024 14:23
 Operator : RC/JU
 Sample : PB164783BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK783

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023107.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	22	25	40	rVB	24116	36318	1.02%	0.124%
2	3.546	92	95	115	rBV	261226	446501	12.59%	1.520%
3	3.858	143	148	153	rVB3	6161	9157	0.26%	0.031%
4	6.781	638	645	664	rBV	296062	596291	16.81%	2.031%
5	6.928	664	670	683	rVB	283033	431572	12.16%	1.470%
6	7.122	697	703	717	rBV	327336	592496	16.70%	2.018%
7	7.581	774	781	796	rVB	305858	527796	14.88%	1.797%
8	8.293	896	902	923	rBV	439435	748734	21.10%	2.550%
9	8.722	967	975	992	rBV	372116	616179	17.37%	2.098%
10	8.863	992	999	1006	rBV2	22553	47551	1.34%	0.162%
11	9.434	1086	1096	1114	rBV	317400	549286	15.48%	1.870%
12	9.975	1180	1188	1211	rBV	409615	835807	23.56%	2.846%
13	10.328	1240	1248	1263	rBV	399432	712366	20.08%	2.426%
14	10.481	1265	1274	1296	rBV	364184	750711	21.16%	2.556%
15	11.946	1515	1523	1531	rBV5	5250	14369	0.41%	0.049%
16	13.604	1797	1805	1818	rBV	1000126	1377735	38.83%	4.692%
17	13.887	1845	1853	1862	rBV2	1005738	1493553	42.10%	5.086%
18	14.198	1899	1906	1920	rVB	825721	1097368	30.93%	3.737%
19	14.463	1946	1951	1970	rBV2	216545	628390	17.71%	2.140%
20	15.045	2047	2050	2056	rVB5	2700	4539	0.13%	0.015%
21	15.210	2072	2078	2089	rBV	1463456	2028906	57.19%	6.909%
22	15.363	2096	2104	2118	rBV2	330310	683500	19.27%	2.327%
23	15.463	2119	2121	2126	rVV6	9362	14741	0.42%	0.050%
24	15.592	2139	2143	2146	rVB6	3184	3971	0.11%	0.014%
25	15.787	2173	2176	2181	rBV7	2044	3744	0.11%	0.013%
26	16.786	2341	2346	2350	rBV4	2962	4289	0.12%	0.015%
27	17.010	2377	2384	2393	rBV	1145620	1554369	43.81%	5.293%
28	17.104	2393	2400	2415	rVV2	1721998	2432854	68.58%	8.284%
29	17.704	2499	2502	2508	rVB8	2771	3866	0.11%	0.013%
30	17.945	2540	2543	2548	rBV7	5438	8406	0.24%	0.029%
31	19.033	2723	2728	2734	rBV4	23721	36054	1.02%	0.123%
32	19.116	2739	2742	2747	rBV	16475	24017	0.68%	0.082%
33	19.292	2769	2772	2776	rBV6	5110	8220	0.23%	0.028%
34	19.492	2799	2806	2816	rBV	2201194	3167586	89.29%	10.786%
35	21.445	3132	3138	3151	rBV	1403244	2103796	59.30%	7.164%
36	24.439	3637	3647	3660	rVB	1521053	3547683	100.00%	12.081%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023107.D
Acq On : 14 Nov 2024 14:23
Operator : RC/JU
Sample : PB164783BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK783

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	24.663	3676	3685	3706	rVB	785047	2223697	62.68%	7.572%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 29366418

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023107.D
Acq On : 14 Nov 2024 14:23
Operator : RC/JU
Sample : PB164783BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK783

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

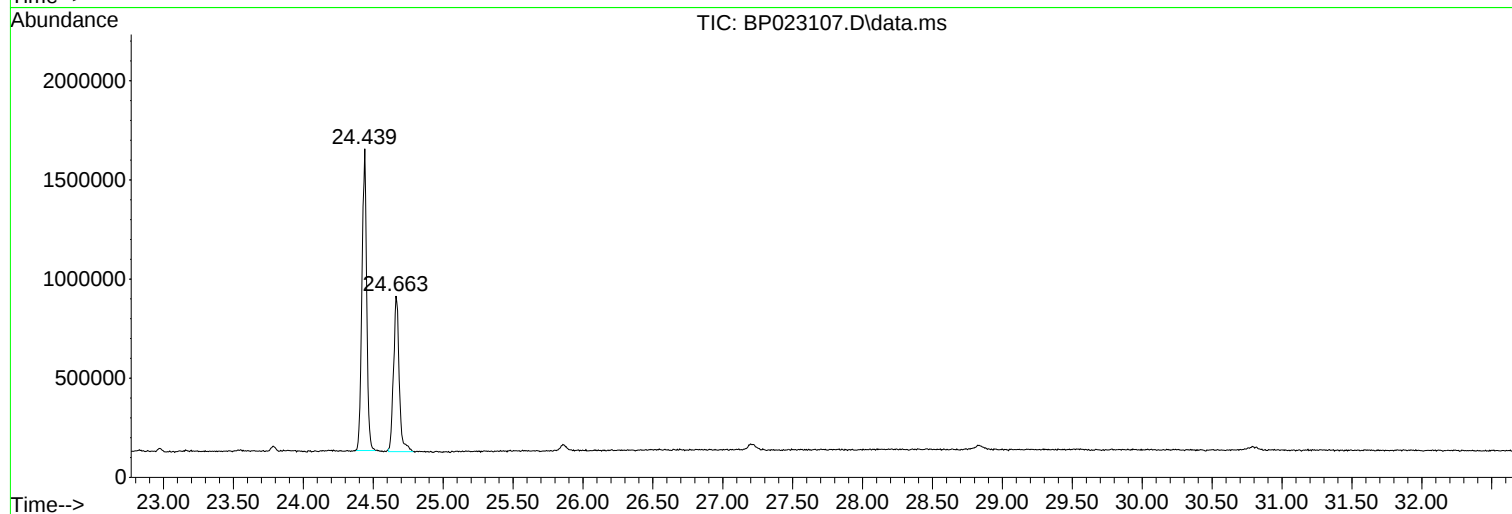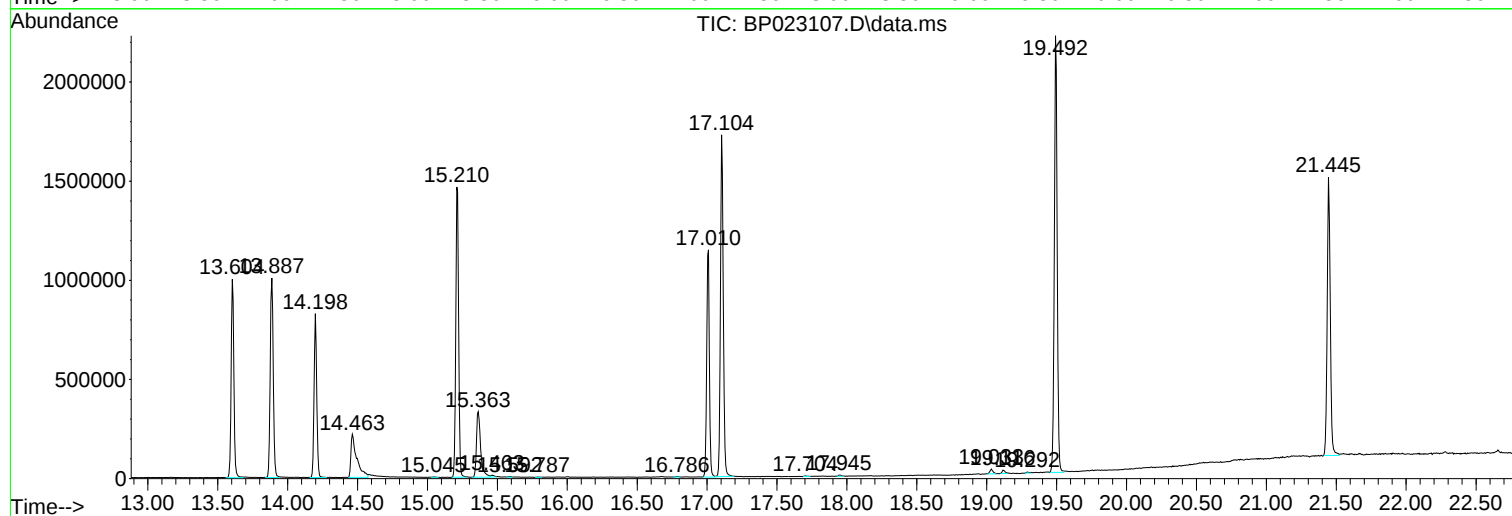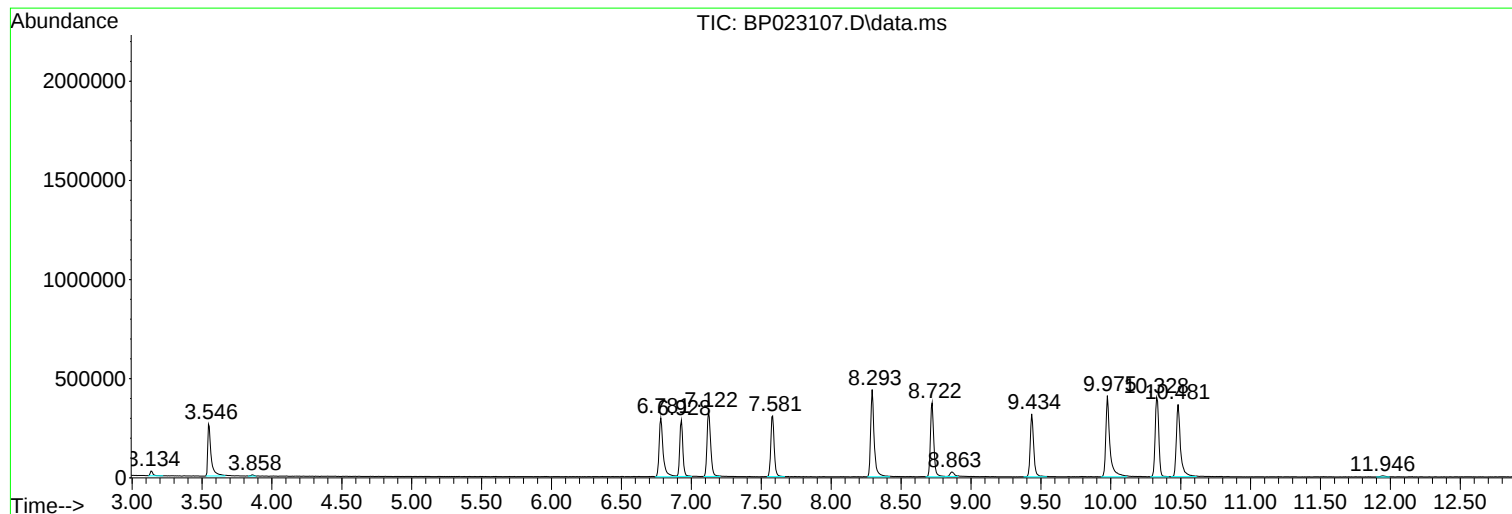

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023107.D
Acq On : 14 Nov 2024 14:23
Operator : RC/JU
Sample : PB164783BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK783

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023107.D
Acq On : 14 Nov 2024 14:23
Operator : RC/JU
Sample : PB164783BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK783

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc