

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023113.D
 Acq On : 14 Nov 2024 20:27
 Operator : RC/JU
 Sample : P4802-11
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCPD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.105	17	20	23	rBV3	5092	7246	0.21%	0.029%
2	3.140	23	26	29	rVV	15843	20712	0.60%	0.083%
3	3.176	29	32	37	rVB2	6821	8788	0.26%	0.035%
4	3.576	96	100	108	rBV	14100	28161	0.82%	0.113%
5	3.864	145	149	155	rVB2	3837	6293	0.18%	0.025%
6	4.287	216	221	225	rBV2	5966	8443	0.25%	0.034%
7	4.370	229	235	240	rVB9	2769	4948	0.14%	0.020%
8	6.722	630	635	641	rVV2	6265	10226	0.30%	0.041%
9	6.793	641	647	662	rVV	86052	187717	5.48%	0.755%
10	6.928	665	670	687	rVB	222041	346518	10.12%	1.393%
11	7.128	698	704	719	rBV	265604	457830	13.37%	1.840%
12	7.581	775	781	790	rBV	294462	474885	13.86%	1.909%
13	7.652	790	793	801	rVB4	6073	10433	0.30%	0.042%
14	7.881	827	832	835	rBV7	1997	3795	0.11%	0.015%
15	8.293	895	902	920	rBV	282142	479462	14.00%	1.927%
16	8.722	967	975	991	rBV	279618	511894	14.94%	2.058%
17	9.105	1035	1040	1045	rBV4	5647	9541	0.28%	0.038%
18	9.434	1088	1096	1112	rBV	266339	460605	13.45%	1.851%
19	9.981	1181	1189	1216	rBV	268169	718603	20.98%	2.889%
20	10.163	1216	1220	1226	rVB9	3061	6447	0.19%	0.026%
21	10.328	1241	1248	1260	rBV	381005	647573	18.91%	2.603%
22	10.528	1277	1282	1289	rVB10	2587	5777	0.17%	0.023%
23	10.775	1318	1324	1326	rBV7	2151	3657	0.11%	0.015%
24	11.175	1385	1392	1404	rBV7	5225	19404	0.57%	0.078%
25	11.328	1411	1418	1430	rBV9	5339	20293	0.59%	0.082%
26	11.587	1457	1462	1467	rVB6	3869	6348	0.19%	0.026%
27	11.869	1506	1510	1513	rVV6	2043	3478	0.10%	0.014%
28	11.940	1517	1522	1531	rVB6	4412	9999	0.29%	0.040%
29	13.093	1711	1718	1726	rBV	25748	46468	1.36%	0.187%
30	13.599	1798	1804	1819	rBV	893049	1229821	35.90%	4.943%
31	13.893	1846	1854	1864	rBV	901187	1177276	34.37%	4.732%
32	14.198	1900	1906	1920	rVB	692614	999679	29.19%	4.018%
33	14.498	1949	1957	1969	rBV3	60444	198629	5.80%	0.798%
34	15.034	2046	2048	2057	rVB5	2864	6004	0.18%	0.024%
35	15.222	2071	2080	2090	rBV	1033513	1787921	52.20%	7.187%
36	15.363	2098	2104	2115	rBV	415980	652451	19.05%	2.623%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023113.D
 Acq On : 14 Nov 2024 20:27
 Operator : RC/JU
 Sample : P4802-11
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCPD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

37	15.451	2117	2119	2128	rVB9	7299	12287	0.36%	0.049%
38	15.598	2139	2144	2148	rVB7	3296	4695	0.14%	0.019%
39	15.945	2201	2203	2208	rVV6	2652	3510	0.10%	0.014%
40	16.134	2230	2235	2243	rVB5	4399	7680	0.22%	0.031%
41	16.275	2252	2259	2261	rBV8	2699	5355	0.16%	0.022%
42	16.481	2290	2294	2297	rBV5	3744	4346	0.13%	0.017%
43	16.681	2325	2328	2334	rVB8	2392	3865	0.11%	0.016%
44	16.763	2338	2342	2345	rBV5	3647	4817	0.14%	0.019%
45	16.887	2356	2363	2367	rBV9	3329	6934	0.20%	0.028%
46	16.934	2367	2371	2376	rBV3	23190	32411	0.95%	0.130%
47	17.016	2378	2385	2394	rVV	904382	1343553	39.23%	5.401%
48	17.104	2395	2400	2410	rVV	1635775	2132957	62.27%	8.574%
49	17.204	2415	2417	2424	rVB7	3483	4339	0.13%	0.017%
50	17.316	2432	2436	2443	rBV5	6101	10343	0.30%	0.042%
51	17.704	2497	2502	2508	rVB5	30624	41255	1.20%	0.166%
52	17.939	2537	2542	2551	rBV	84192	119376	3.49%	0.480%
53	18.022	2553	2556	2559	rVV2	7256	10457	0.31%	0.042%
54	18.057	2559	2562	2568	rVB7	5176	7770	0.23%	0.031%
55	18.298	2600	2603	2606	rBV4	4881	7291	0.21%	0.029%
56	18.387	2613	2618	2624	rVB2	33347	42127	1.23%	0.169%
57	18.475	2629	2633	2639	rBV6	10998	22673	0.66%	0.091%
58	18.539	2641	2644	2648	rVB5	9236	12265	0.36%	0.049%
59	19.034	2723	2728	2732	rBV3	21794	36657	1.07%	0.147%
60	19.122	2738	2743	2744	rBV	16047	22449	0.66%	0.090%
61	19.151	2744	2748	2756	rVB3	37153	66992	1.96%	0.269%
62	19.286	2767	2771	2778	rBV4	35972	47641	1.39%	0.192%
63	19.486	2799	2805	2816	rBV	1799231	2933332	85.64%	11.791%
64	21.439	3131	3137	3145	rBV	1227702	1846399	53.91%	7.422%
65	24.439	3637	3647	3663	rVB	1383039	3425216	100.00%	13.768%
66	24.657	3675	3684	3705	rVB	769513	2081306	60.76%	8.366%




Sum of corrected areas: 24877623

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023113.D
Acq On : 14 Nov 2024 20:27
Operator : RC/JU
Sample : P4802-11
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCPD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

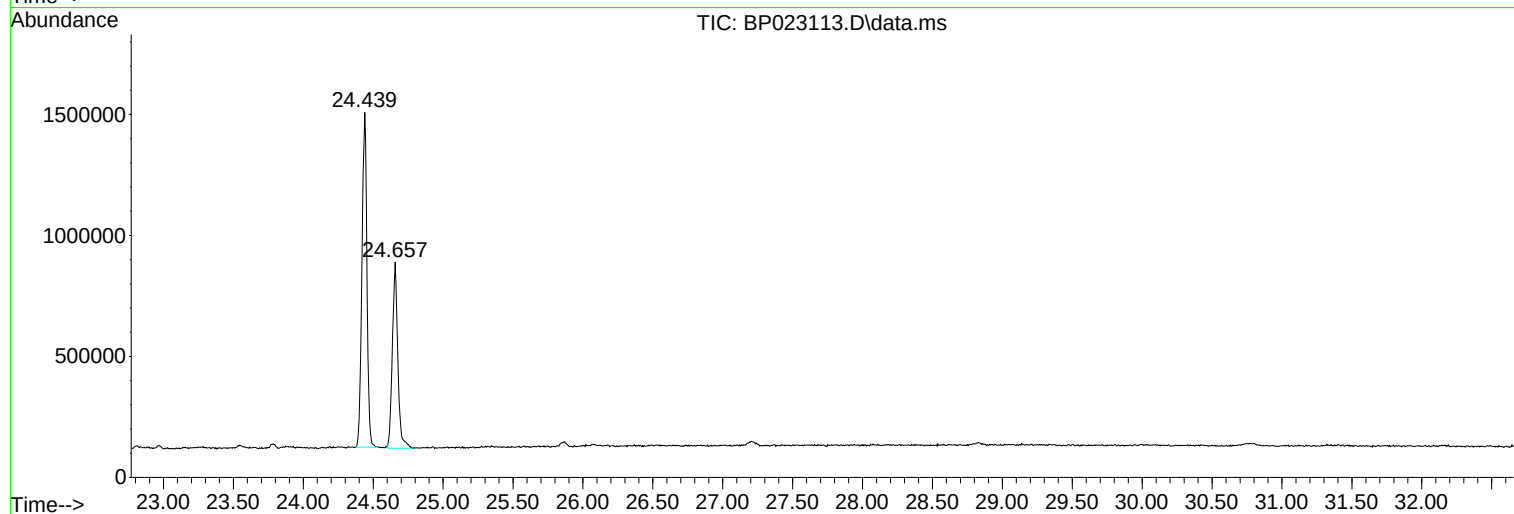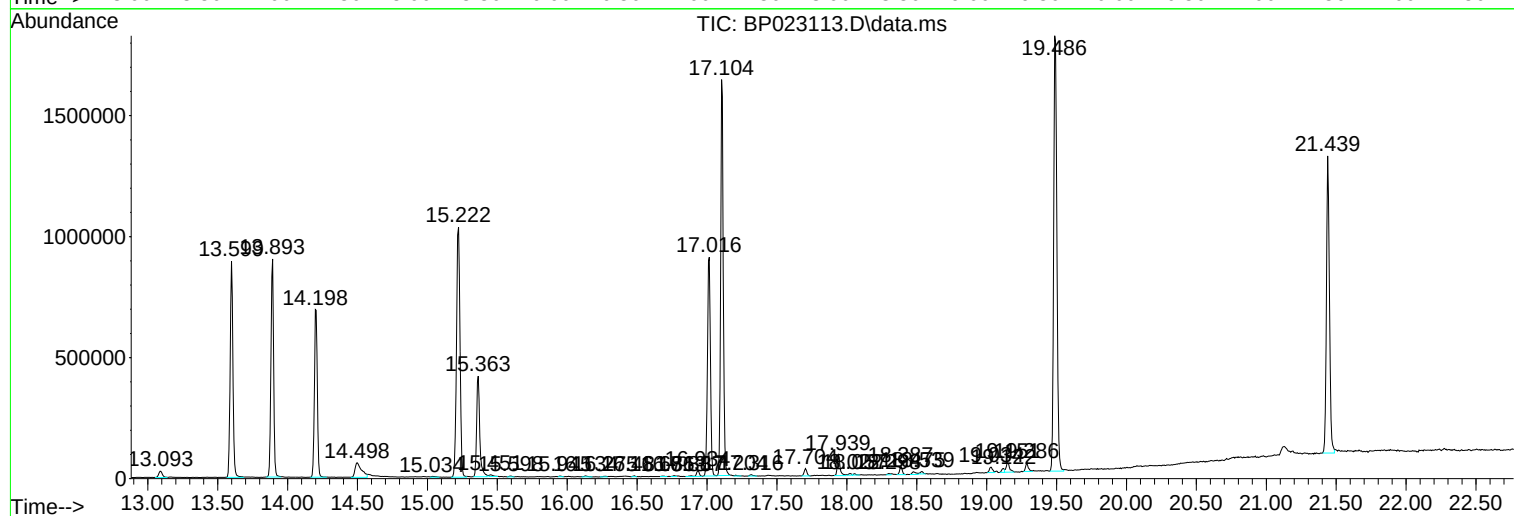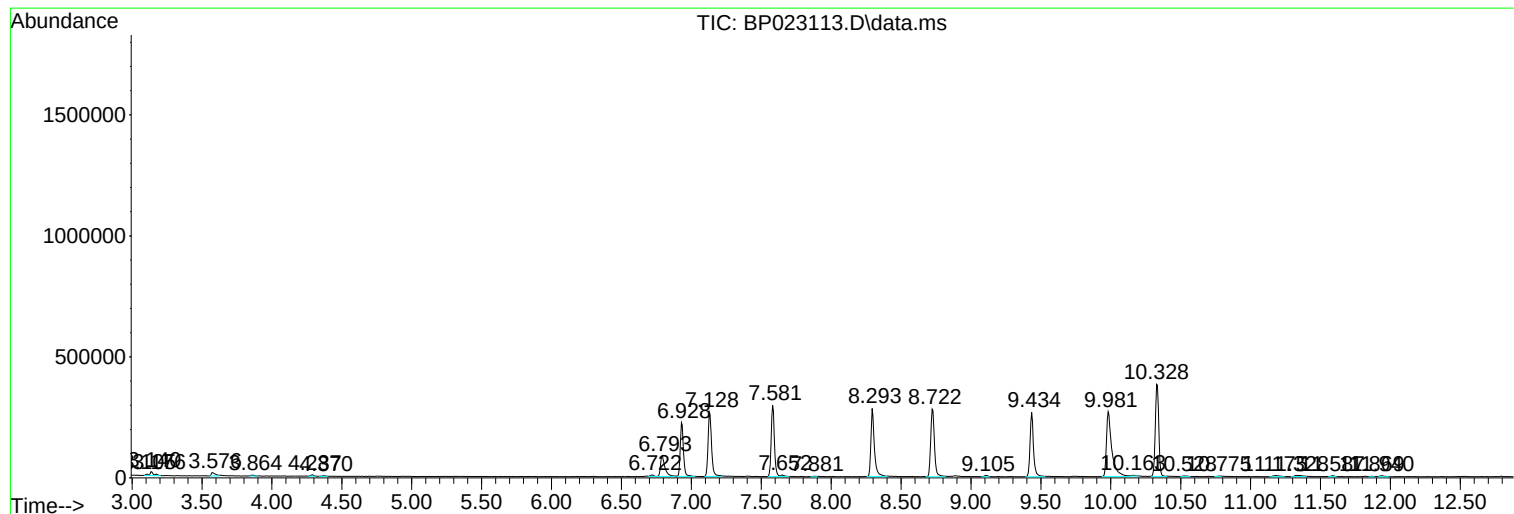

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023113.D
Acq On : 14 Nov 2024 20:27
Operator : RC/JU
Sample : P4802-11
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCPD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023113.D
Acq On : 14 Nov 2024 20:27
Operator : RC/JU
Sample : P4802-11
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCPD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc