

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023120.D
 Acq On : 15 Nov 2024 01:52
 Operator : RC/JU
 Sample : PB164958BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK958

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	33	rVB	16416	22086	0.85%	0.103%
2	3.552	92	96	116	rBV	181647	316939	12.24%	1.479%
3	3.864	144	149	153	rBV3	4197	6582	0.25%	0.031%
4	6.787	640	646	663	rBV	219961	424609	16.40%	1.981%
5	6.928	665	670	683	rVB	198931	301583	11.65%	1.407%
6	7.128	698	704	722	rBV	248792	429620	16.60%	2.005%
7	7.581	774	781	791	rBV	224126	374003	14.45%	1.745%
8	8.287	895	901	922	rBV	291571	546202	21.10%	2.549%
9	8.722	966	975	989	rBV	237662	453830	17.53%	2.118%
10	8.869	995	1000	1009	rBV2	18344	32341	1.25%	0.151%
11	9.440	1089	1097	1107	rBV	212390	401170	15.50%	1.872%
12	9.981	1181	1189	1211	rBV	288699	611708	23.63%	2.855%
13	10.328	1241	1248	1262	rVB	315803	522653	20.19%	2.439%
14	10.481	1265	1274	1301	rBV	255864	564381	21.80%	2.634%
15	11.952	1518	1524	1532	rBV7	4388	9806	0.38%	0.046%
16	13.610	1798	1806	1823	rBV	645547	1041304	40.23%	4.859%
17	13.881	1844	1852	1867	rBV	707234	1120460	43.29%	5.229%
18	14.193	1897	1905	1918	rBV	576953	818721	31.63%	3.821%
19	14.469	1946	1952	1969	rBV	153988	425946	16.46%	1.988%
20	15.210	2071	2078	2090	rBV	1151579	1535242	59.31%	7.164%
21	15.369	2098	2105	2119	rBV	289434	498900	19.27%	2.328%
22	15.469	2119	2122	2129	rVB6	7720	14459	0.56%	0.067%
23	15.581	2138	2141	2148	rVB9	2041	4497	0.17%	0.021%
24	16.669	2323	2326	2334	rVB9	2743	5178	0.20%	0.024%
25	16.792	2342	2347	2349	rBV6	2464	2694	0.10%	0.013%
26	16.998	2376	2382	2391	rBV	878568	1157431	44.72%	5.401%
27	17.098	2392	2399	2418	rVV	1091858	1829239	70.67%	8.536%
28	17.957	2539	2545	2548	rBV8	3570	6555	0.25%	0.031%
29	19.039	2723	2729	2734	rBV4	16709	28267	1.09%	0.132%
30	19.116	2738	2742	2747	rVV	15751	20330	0.79%	0.095%
31	19.492	2799	2806	2817	rBV	1555746	2356781	91.05%	10.998%
32	21.439	3131	3137	3149	rBV	915730	1452070	56.10%	6.776%
33	24.433	3637	3646	3663	rVB	1050415	2588438	100.00%	12.079%
34	24.657	3676	3684	3695	rBV	542842	1504738	58.13%	7.022%

Sum of corrected areas: 21428763




Instrument :
BNA_P
ClientSampleId :
SBLK958

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023120.D
Acq On : 15 Nov 2024 01:52
Operator : RC/JU
Sample : PB164958BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK958

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

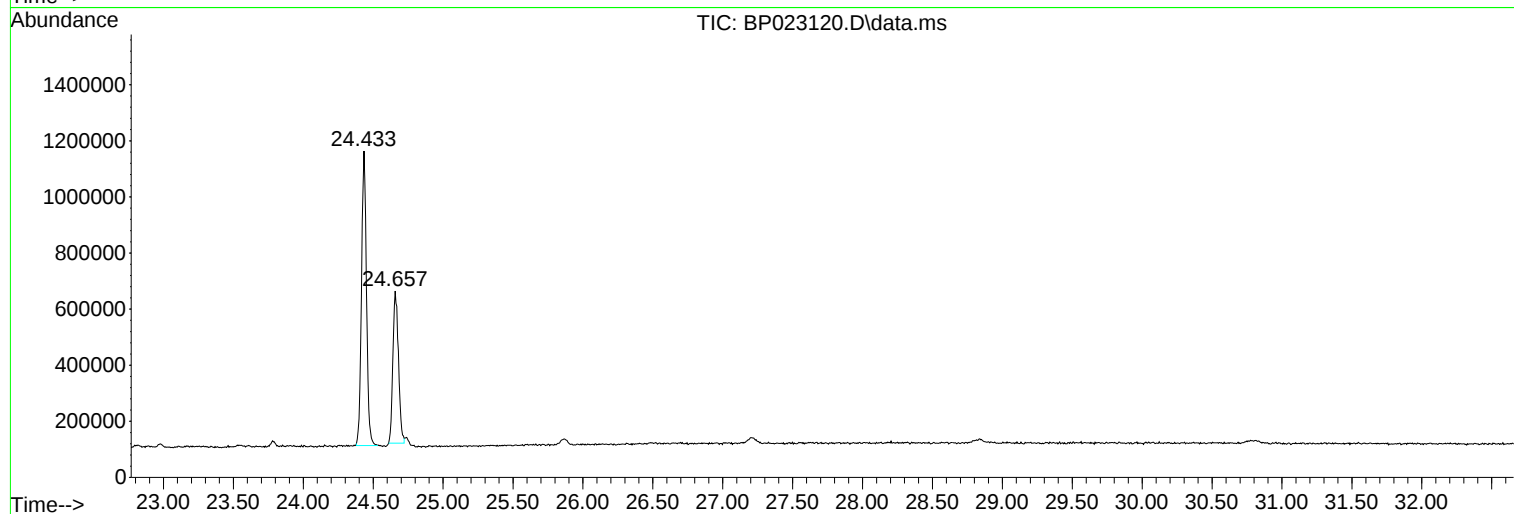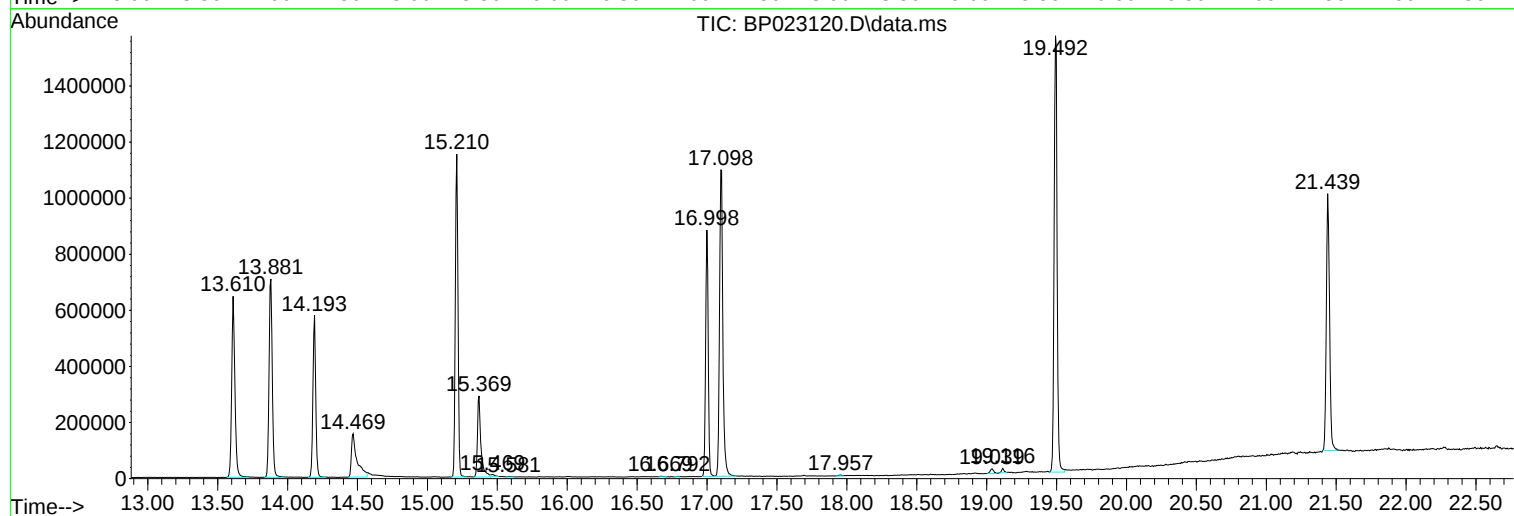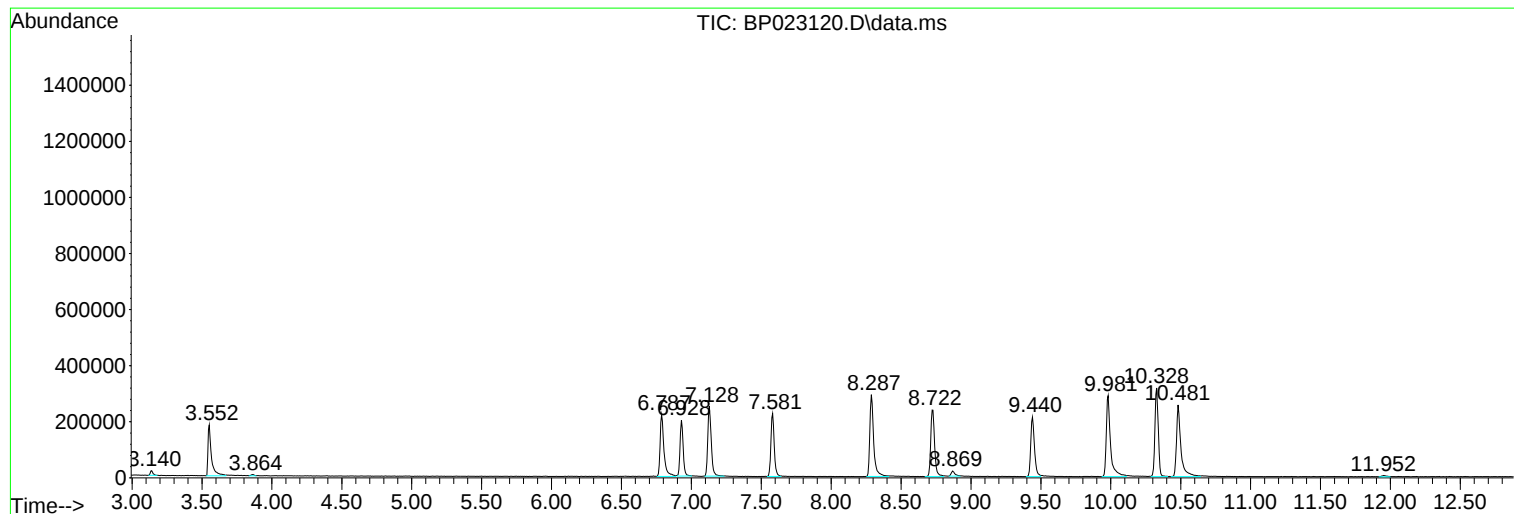

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023120.D
Acq On : 15 Nov 2024 01:52
Operator : RC/JU
Sample : PB164958BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK958

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023120.D
Acq On : 15 Nov 2024 01:52
Operator : RC/JU
Sample : PB164958BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK958

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc