

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023125.D
 Acq On : 15 Nov 2024 05:16
 Operator : RC/JU
 Sample : P4740-04
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023125.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	22	25	36	rVB	14223	20890	0.70%	0.089%
2	3.558	93	97	108	rBV	42351	78055	2.63%	0.331%
3	3.858	144	148	155	rVB3	3859	6736	0.23%	0.029%
4	4.287	215	221	225	rBV2	3318	5986	0.20%	0.025%
5	4.370	230	235	242	rVB5	5116	8612	0.29%	0.037%
6	6.722	628	635	640	rBV6	2980	5959	0.20%	0.025%
7	6.787	640	646	663	rBV	66367	145036	4.88%	0.615%
8	6.928	663	670	682	rVV	217166	351958	11.84%	1.492%
9	7.128	697	704	721	rBV	266313	461161	15.52%	1.955%
10	7.575	774	780	790	rBV	251786	425931	14.33%	1.806%
11	7.640	790	791	798	rVB6	2644	3659	0.12%	0.016%
12	8.287	894	901	924	rBV	219017	437215	14.71%	1.854%
13	8.722	968	975	996	rBV	303176	540752	18.20%	2.293%
14	9.111	1037	1041	1049	rVB6	2941	5470	0.18%	0.023%
15	9.434	1089	1096	1110	rBV	270162	485550	16.34%	2.059%
16	9.969	1180	1187	1216	rBV	323498	734673	24.72%	3.115%
17	10.322	1240	1247	1260	rVB	364692	605707	20.38%	2.568%
18	10.481	1265	1274	1298	rBV	240442	539522	18.15%	2.288%
19	11.205	1388	1397	1402	rBV10	4227	11217	0.38%	0.048%
20	11.940	1516	1522	1523	rBV2	3421	5406	0.18%	0.023%
21	12.040	1534	1539	1541	rBV2	5512	8625	0.29%	0.037%
22	13.087	1708	1717	1726	rBV	44495	69966	2.35%	0.297%
23	13.599	1796	1804	1817	rBV	719067	1206913	40.61%	5.117%
24	13.881	1843	1852	1866	rBV	952910	1269430	42.71%	5.382%
25	14.198	1899	1906	1917	rVB	675088	935732	31.49%	3.967%
26	14.498	1949	1957	1960	rBV3	30120	55856	1.88%	0.237%
27	14.646	1979	1982	1985	rVV5	3242	3833	0.13%	0.016%
28	14.687	1987	1989	1994	rVB6	3729	4678	0.16%	0.020%
29	15.216	2070	2079	2086	rBV	1436056	1786199	60.10%	7.573%
30	15.281	2087	2090	2097	rVB2	16421	25094	0.84%	0.106%
31	15.363	2097	2104	2117	rBV	310002	585993	19.72%	2.485%
32	15.593	2139	2143	2146	rVB6	2564	3344	0.11%	0.014%
33	15.798	2173	2178	2183	rBV8	1952	3901	0.13%	0.017%
34	16.134	2228	2235	2240	rBV7	2946	5532	0.19%	0.023%
35	16.269	2251	2258	2259	rBV6	2338	3295	0.11%	0.014%
36	16.416	2277	2283	2289	rVB6	5158	10952	0.37%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023125.D
Acq On : 15 Nov 2024 05:16
Operator : RC/JU
Sample : P4740-04
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	16.475	2289	2293	2295	rBV4	3303	4908	0.17%	0.021%
38	16.516	2295	2300	2315	rVV	18622	51263	1.72%	0.217%
39	16.675	2323	2327	2331	rVB6	2880	4556	0.15%	0.019%
40	16.934	2366	2371	2376	rBV	27375	34539	1.16%	0.146%
41	17.004	2377	2383	2393	rBV	1000094	1266932	42.63%	5.372%
42	17.104	2393	2400	2413	rBV	1309068	2097093	70.56%	8.891%
43	17.310	2431	2435	2440	rBV6	5028	8703	0.29%	0.037%
44	17.704	2499	2502	2508	rVB7	4802	8239	0.28%	0.035%
45	17.828	2516	2523	2525	rBV8	4916	9522	0.32%	0.040%
46	17.939	2537	2542	2550	rBV2	68993	110821	3.73%	0.470%
47	18.010	2552	2554	2558	rVB3	2673	3533	0.12%	0.015%
48	18.387	2615	2618	2624	rVB7	7590	10106	0.34%	0.043%
49	18.934	2708	2711	2716	rVB6	13362	15833	0.53%	0.067%
50	19.039	2725	2729	2734	rBV4	15118	24608	0.83%	0.104%
51	19.128	2740	2744	2747	rBV	16388	24730	0.83%	0.105%
52	19.157	2747	2749	2752	rVB4	9349	10574	0.36%	0.045%
53	19.281	2766	2770	2776	rBV2	45053	54373	1.83%	0.231%
54	19.498	2801	2807	2816	rBV	1897167	2625885	88.36%	11.133%
55	21.445	3132	3138	3149	rBV	1022436	1608665	54.13%	6.821%
56	24.439	3638	3647	3664	rVB	1201362	2971905	100.00%	12.601%
57	24.663	3676	3685	3704	rVB	572918	1779841	59.89%	7.546%




Sum of corrected areas: 23585467

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023125.D
Acq On : 15 Nov 2024 05:16
Operator : RC/JU
Sample : P4740-04
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

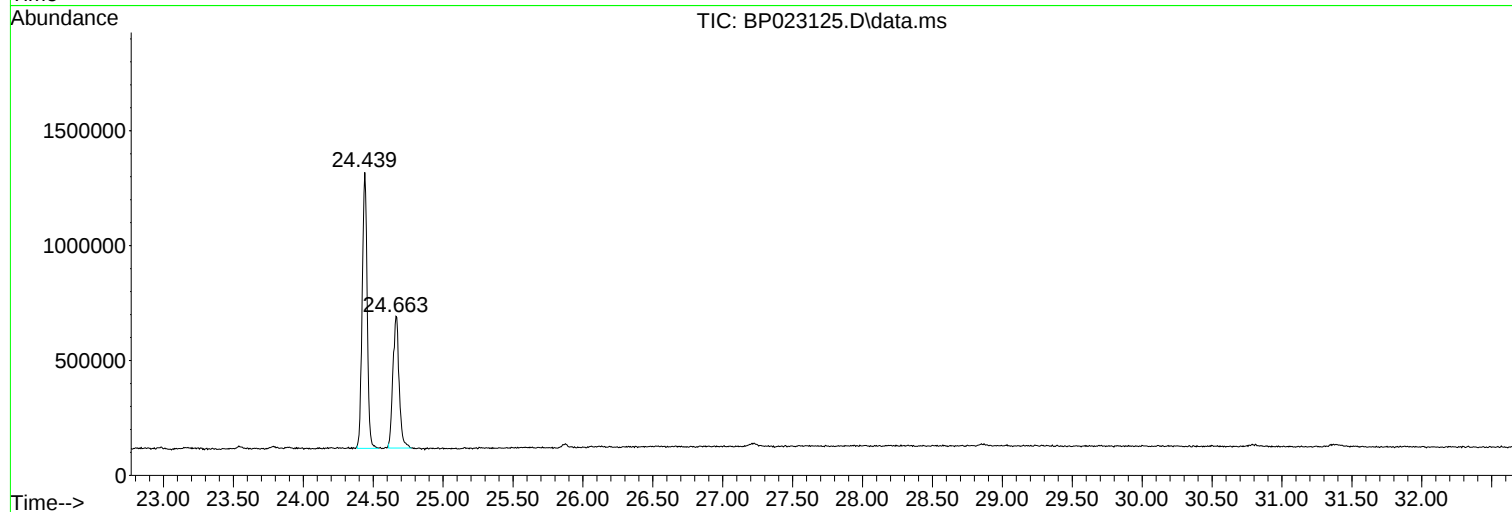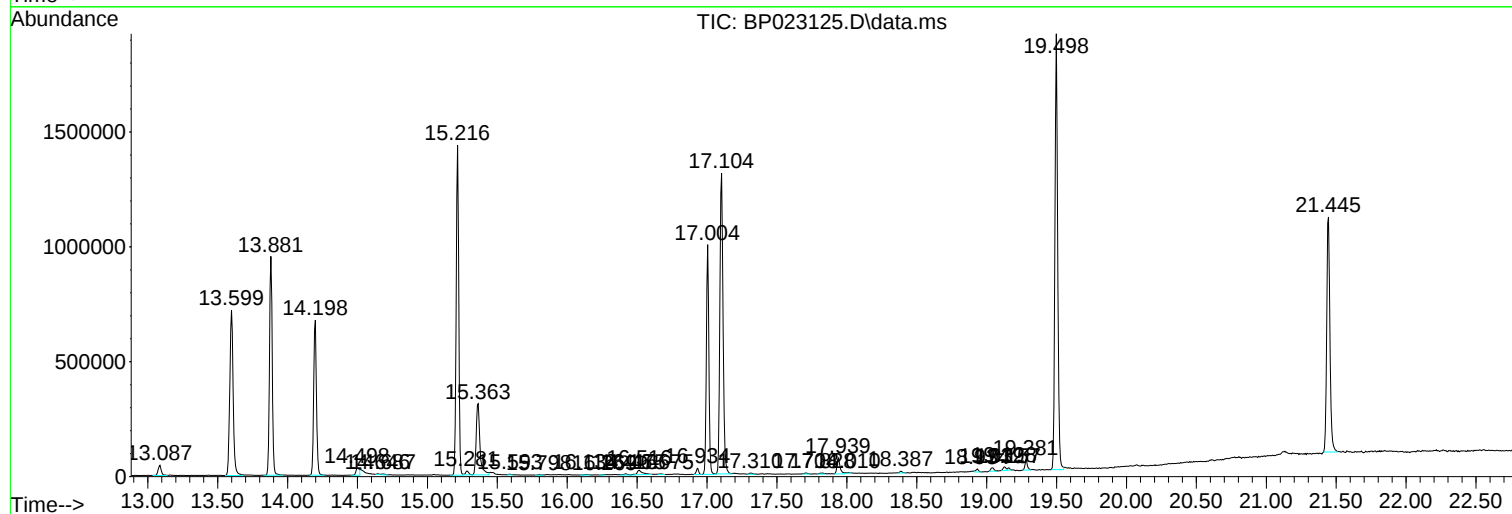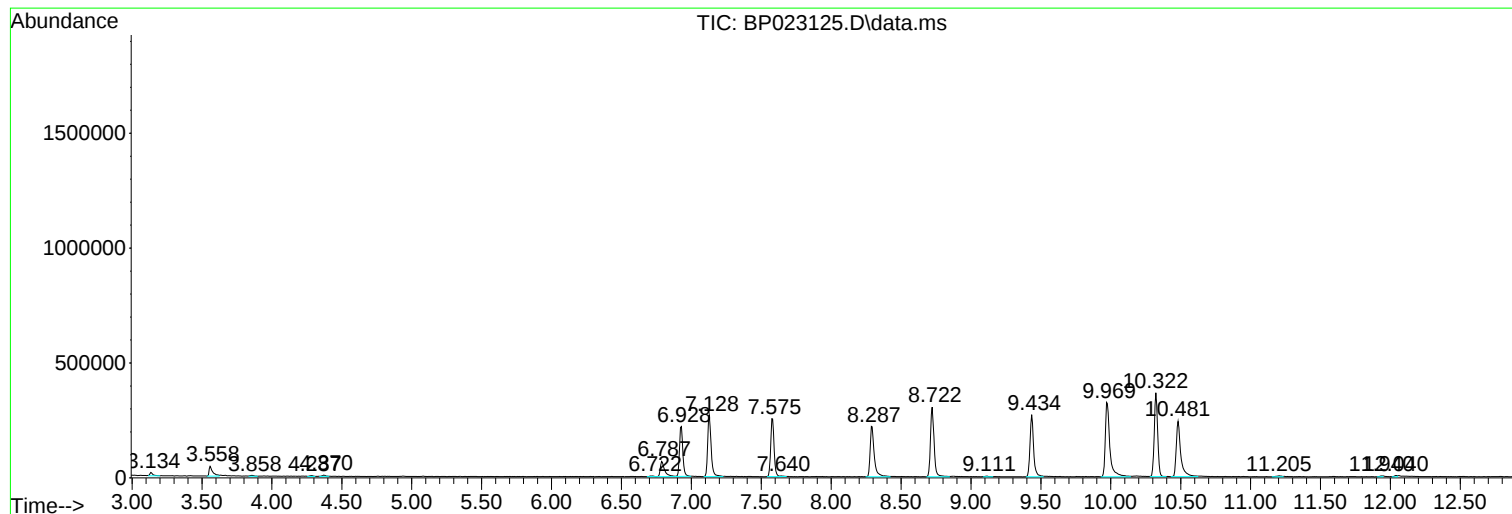

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023125.D
Acq On : 15 Nov 2024 05:16
Operator : RC/JU
Sample : P4740-04
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023125.D
Acq On : 15 Nov 2024 05:16
Operator : RC/JU
Sample : P4740-04
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------