

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023126.D
 Acq On : 15 Nov 2024 05:57
 Operator : RC/JU
 Sample : P4740-05
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023126.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	22	25	33	rBV	13921	18637	0.60%	0.078%
2	3.558	94	97	112	rBV	32673	66462	2.13%	0.277%
3	3.858	144	148	152	rVB4	3101	4213	0.14%	0.018%
4	4.281	216	220	225	rBV2	3550	5006	0.16%	0.021%
5	4.369	228	235	252	rVB	816143	1168057	37.46%	4.873%
6	6.711	627	633	640	rBV7	3034	6495	0.21%	0.027%
7	6.787	640	646	663	rBV2	52458	123922	3.97%	0.517%
8	6.928	663	670	682	rVV	208704	331412	10.63%	1.382%
9	7.122	696	703	721	rBV	228569	423925	13.59%	1.768%
10	7.575	774	780	792	rBV	236602	399078	12.80%	1.665%
11	8.293	892	902	921	rBV2	181680	378527	12.14%	1.579%
12	8.722	968	975	990	rBV	270023	493454	15.82%	2.058%
13	9.110	1034	1041	1044	rVB7	2012	4284	0.14%	0.018%
14	9.434	1087	1096	1114	rBV	250563	447880	14.36%	1.868%
15	9.975	1181	1188	1214	rBV	300689	661352	21.21%	2.759%
16	10.328	1239	1248	1260	rBV	316331	538320	17.26%	2.246%
17	10.487	1268	1275	1301	rBV	147473	347817	11.15%	1.451%
18	11.946	1517	1523	1531	rBV5	3397	7179	0.23%	0.030%
19	13.081	1708	1716	1723	rBV3	14845	29109	0.93%	0.121%
20	13.610	1800	1806	1820	rBV	905902	1198696	38.44%	5.000%
21	13.892	1847	1854	1867	rBV	756073	1194382	38.30%	4.982%
22	14.198	1899	1906	1918	rBV	501819	844714	27.09%	3.524%
23	14.510	1953	1959	1971	rBV3	29683	99236	3.18%	0.414%
24	14.687	1987	1989	1996	rVB7	2966	4132	0.13%	0.017%
25	15.204	2069	2077	2091	rBV	1041223	1724317	55.29%	7.193%
26	15.363	2099	2104	2116	rBV	411347	638832	20.49%	2.665%
27	15.445	2116	2118	2127	rVB5	9233	16369	0.52%	0.068%
28	16.763	2336	2342	2346	rBV8	1879	3847	0.12%	0.016%
29	16.934	2367	2371	2374	rVB6	3465	3956	0.13%	0.017%
30	17.004	2374	2383	2394	rBV	692938	1190157	38.16%	4.965%
31	17.116	2394	2402	2414	rBV	1367500	2208821	70.83%	9.214%
32	17.945	2538	2543	2550	rBV3	24663	39724	1.27%	0.166%
33	19.039	2725	2729	2733	rBV4	19518	28819	0.92%	0.120%
34	19.110	2738	2741	2745	rVB	17999	24411	0.78%	0.102%
35	19.233	2760	2762	2766	rBV3	3094	3812	0.12%	0.016%
36	19.280	2766	2770	2775	rBV7	10582	17971	0.58%	0.075%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023126.D
Acq On : 15 Nov 2024 05:57
Operator : RC/JU
Sample : P4740-05
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CC2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	19.486	2799	2805	2815	rBV	2230824	2920865	93.66%	12.184%
38	21.439	3132	3137	3151	rVB	955730	1561676	50.08%	6.515%
39	24.439	3637	3647	3664	rVB	1164044	3118452	100.00%	13.009%
40	24.663	3676	3685	3704	rVB	510908	1673901	53.68%	6.983%




Sum of corrected areas: 23972219

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023126.D
Acq On : 15 Nov 2024 05:57
Operator : RC/JU
Sample : P4740-05
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

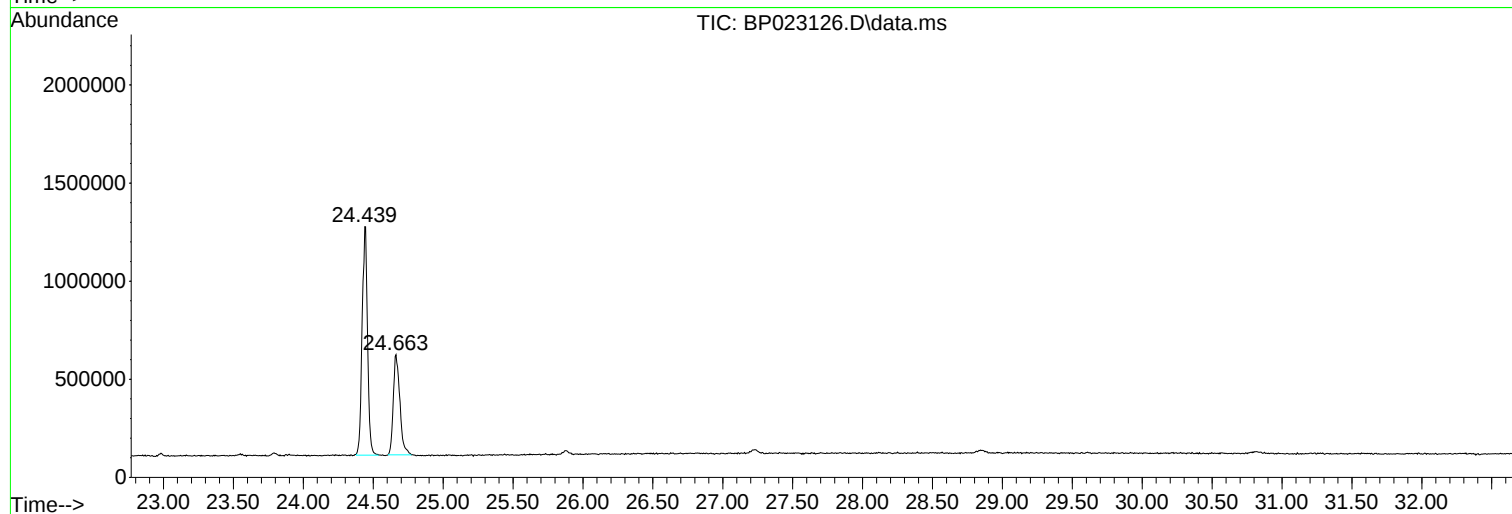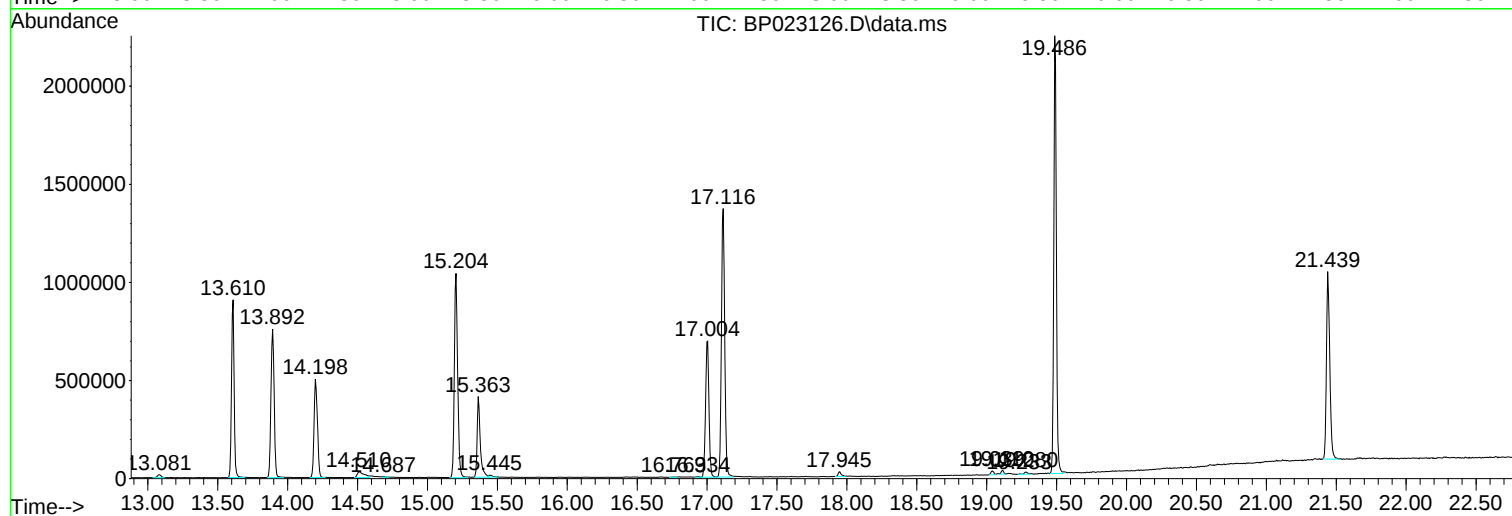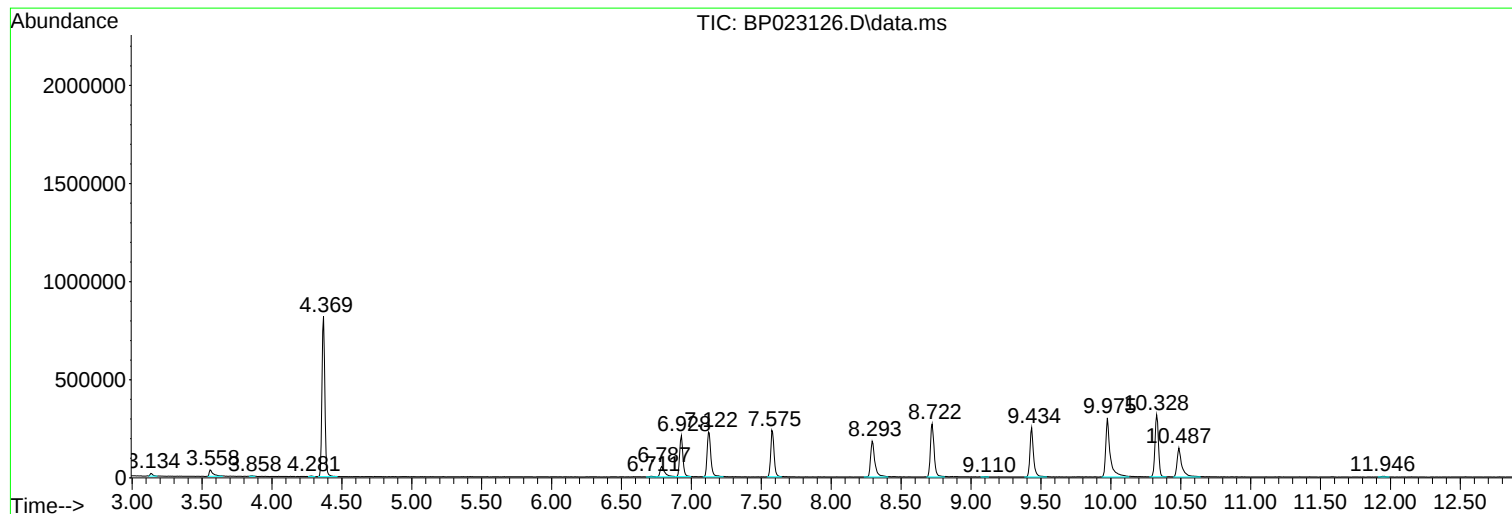

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023126.D
Acq On : 15 Nov 2024 05:57
Operator : RC/JU
Sample : P4740-05
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CC2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.369	58.54 ng/ul	1168060	1,4-Dichlorobenzene-d4	7.575

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

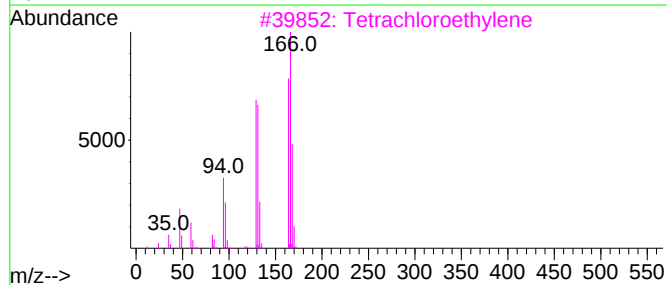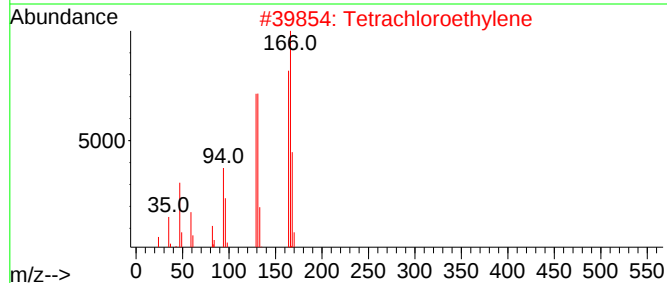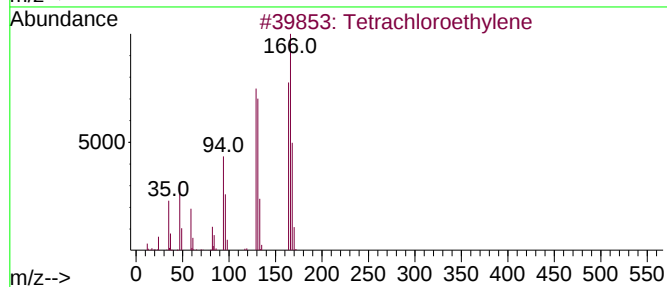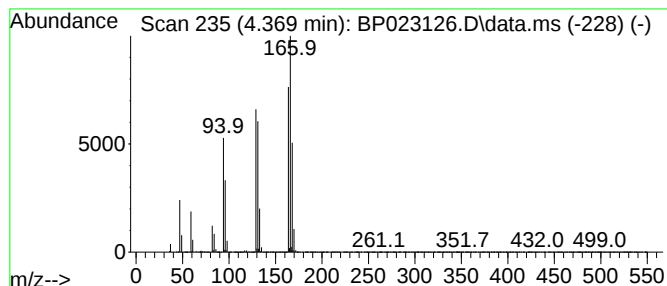

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023126.D
Acq On : 15 Nov 2024 05:57
Operator : RC/JU
Sample : P4740-05
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.369	58.5	ng/ul	1168060	1	7.575	399078	20.0