

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023127.D
 Acq On : 15 Nov 2024 06:38
 Operator : RC/JU
 Sample : P4740-06
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023127.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	31	rBV2	13571	17393	0.61%	0.080%
2	3.558	94	97	110	rBV	62158	115181	4.02%	0.527%
3	3.864	144	149	157	rVB5	2947	5836	0.20%	0.027%
4	4.287	218	221	226	rVB3	2389	3406	0.12%	0.016%
5	4.375	230	236	243	rBV	33690	48680	1.70%	0.223%
6	6.716	629	634	641	rBV6	2243	4388	0.15%	0.020%
7	6.793	641	647	661	rBV	57234	131393	4.59%	0.601%
8	6.928	664	670	681	rVB	193073	308197	10.77%	1.410%
9	7.134	697	705	723	rBV	227893	407111	14.22%	1.862%
10	7.581	775	781	793	rBV	230934	374770	13.09%	1.714%
11	8.299	897	903	920	rBV	224648	394204	13.77%	1.803%
12	8.728	968	976	992	rBV	272455	466588	16.30%	2.134%
13	9.110	1037	1041	1046	rVB5	2827	4046	0.14%	0.019%
14	9.440	1088	1097	1113	rBV	232388	417676	14.59%	1.910%
15	9.981	1180	1189	1216	rBV	277712	636396	22.24%	2.911%
16	10.328	1239	1248	1257	rBV	290911	509828	17.81%	2.332%
17	10.487	1267	1275	1297	rBV	223606	527387	18.43%	2.412%
18	11.204	1390	1397	1399	rBV5	1721	3507	0.12%	0.016%
19	11.957	1516	1525	1528	rBV6	3048	7372	0.26%	0.034%
20	12.534	1618	1623	1627	rBV7	1561	2959	0.10%	0.014%
21	13.075	1709	1715	1725	rVB4	4460	10328	0.36%	0.047%
22	13.540	1789	1794	1801	rBV10	1352	3041	0.11%	0.014%
23	13.616	1801	1807	1826	rVV	828714	1132588	39.57%	5.180%
24	13.892	1842	1854	1866	rBV	757839	1166347	40.75%	5.334%
25	14.198	1895	1906	1919	rBV	491031	803542	28.08%	3.675%
26	14.504	1952	1958	1970	rBV	33296	105524	3.69%	0.483%
27	14.651	1979	1983	1987	rBV7	4194	5103	0.18%	0.023%
28	14.981	2036	2039	2042	rBV3	2251	3134	0.11%	0.014%
29	15.051	2048	2051	2053	rBV4	1840	3026	0.11%	0.014%
30	15.204	2068	2077	2089	rBV	959379	1599130	55.87%	7.314%
31	15.298	2090	2093	2099	rVV8	4292	7630	0.27%	0.035%
32	15.369	2099	2105	2118	rVV	359828	553590	19.34%	2.532%
33	15.457	2118	2120	2133	rVB6	10932	20469	0.72%	0.094%
34	15.592	2138	2143	2155	rVB8	8260	14837	0.52%	0.068%
35	15.786	2172	2176	2177	rBV4	2709	3656	0.13%	0.017%
36	15.851	2185	2187	2191	rVB5	2573	3213	0.11%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023127.D
 Acq On : 15 Nov 2024 06:38
 Operator : RC/JU
 Sample : P4740-06
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CE7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

37	16.133	2228	2235	2238	rBV7	4240	7495	0.26%	0.034%
38	16.416	2280	2283	2285	rBV3	3137	3580	0.13%	0.016%
39	16.486	2290	2295	2300	rBV8	3838	7355	0.26%	0.034%
40	16.763	2338	2342	2345	rBV5	4311	5993	0.21%	0.027%
41	16.933	2366	2371	2376	rBV	53821	72498	2.53%	0.332%
42	16.992	2376	2381	2393	rVB	742800	1114513	38.94%	5.097%
43	17.110	2393	2401	2414	rBV2	981272	1930482	67.45%	8.829%
44	17.239	2420	2423	2429	rVB8	4739	7762	0.27%	0.036%
45	17.310	2431	2435	2441	rVB2	9172	14761	0.52%	0.068%
46	17.510	2466	2469	2476	rVB6	4297	6221	0.22%	0.028%
47	17.710	2498	2503	2509	rVB3	9971	16413	0.57%	0.075%
48	17.945	2537	2543	2549	rBV	83835	133840	4.68%	0.612%
49	18.157	2575	2579	2590	rVB	14390	22568	0.79%	0.103%
50	18.392	2614	2619	2625	rBV	110536	129100	4.51%	0.590%
51	19.045	2726	2730	2734	rBV3	19116	27101	0.95%	0.124%
52	19.122	2738	2743	2747	rVV2	20050	31418	1.10%	0.144%
53	19.280	2765	2770	2781	rBV6	31710	51500	1.80%	0.236%
54	19.498	2801	2807	2816	rBV2	1862309	2543685	88.88%	11.634%
55	21.451	3132	3139	3149	rBV2	816189	1455769	50.87%	6.658%
56	24.445	3639	3648	3660	rVB	1165552	2861983	100.00%	13.090%
57	24.680	3678	3688	3705	rVB2	533023	1598727	55.86%	7.312%



Sum of corrected areas: 21864240

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023127.D
Acq On : 15 Nov 2024 06:38
Operator : RC/JU
Sample : P4740-06
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

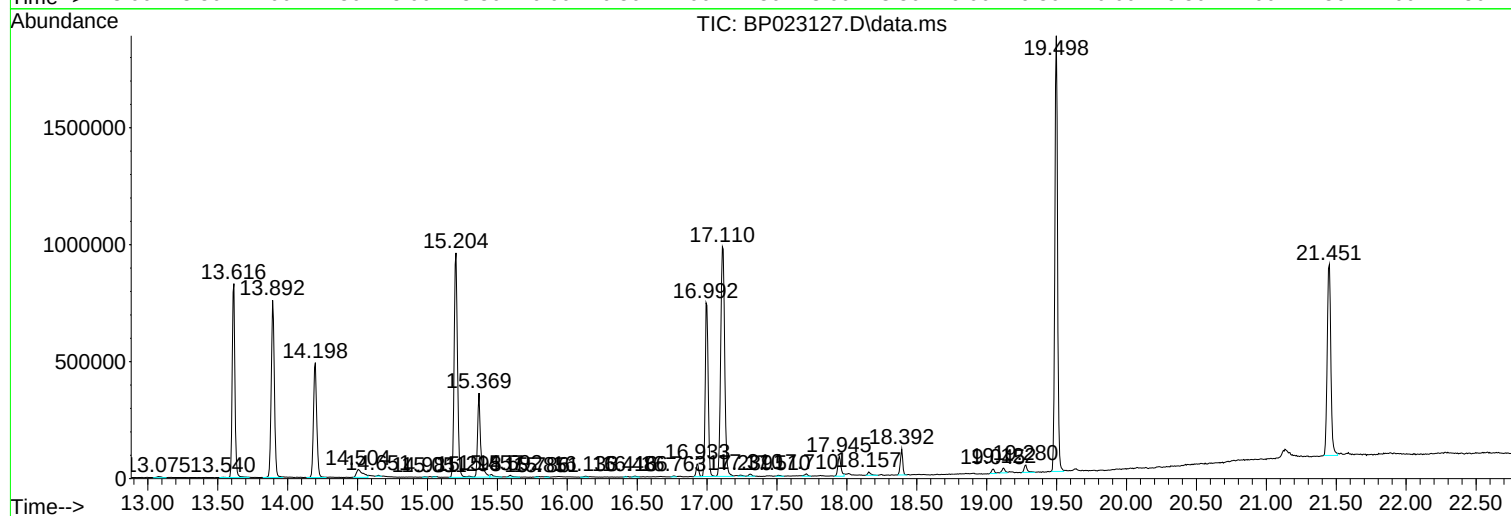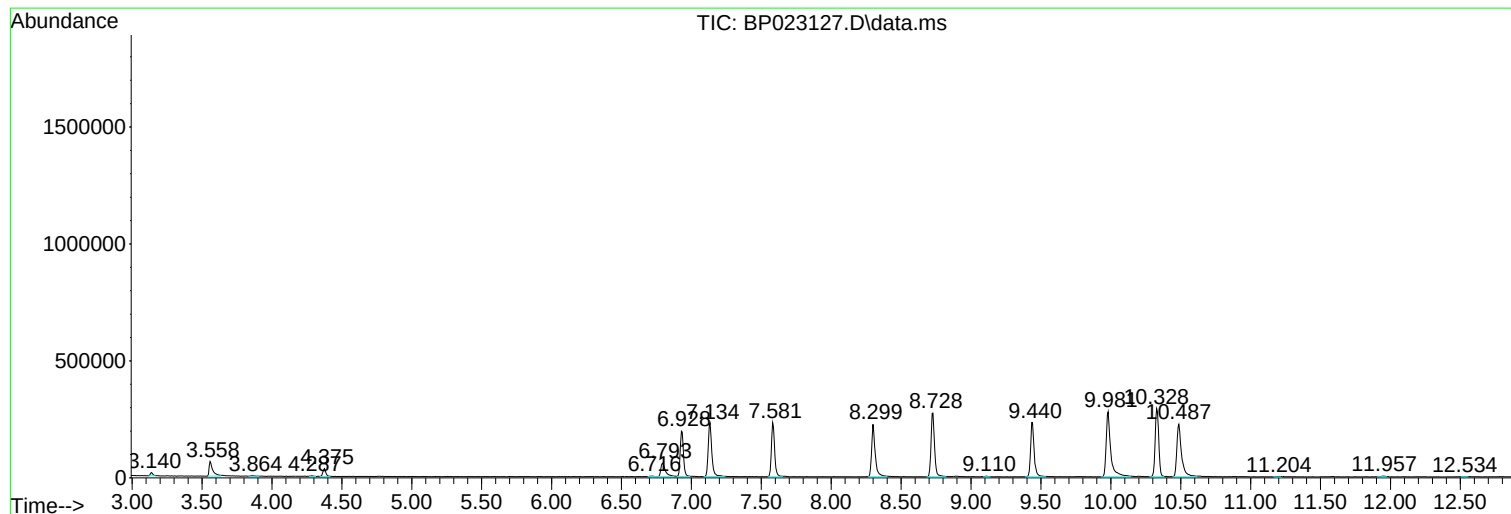

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023127.D
Acq On : 15 Nov 2024 06:38
Operator : RC/JU
Sample : P4740-06
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.375	2.60 ng/ul	48680	1,4-Dichlorobenzene-d4	7.581

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	95
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	93
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	93
5			Ethyne, dichloro-	94	C2Cl2	007572-29-4	18

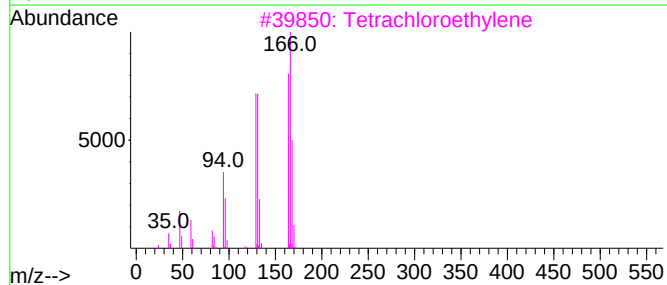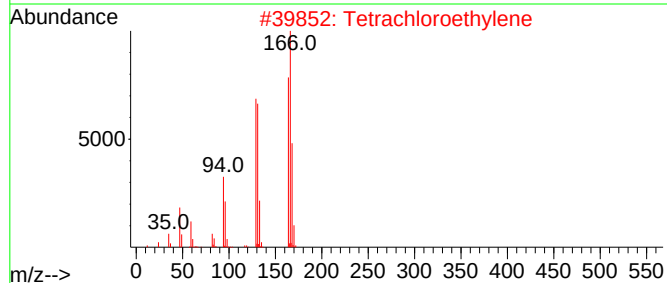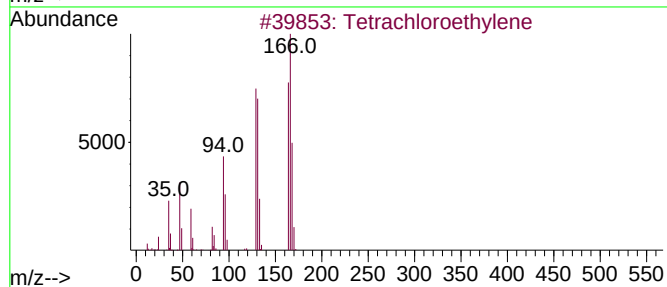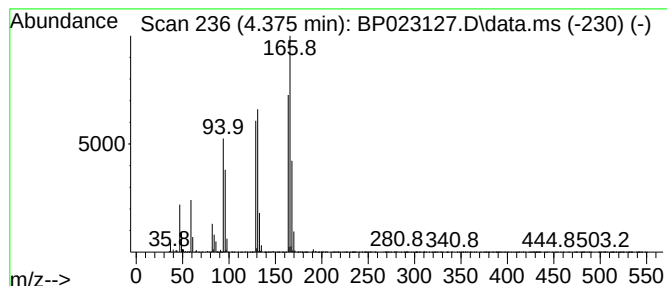

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023127.D
Acq On : 15 Nov 2024 06:38
Operator : RC/JU
Sample : P4740-06
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 n-Hexadecanoic acid Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.945	2.40 ng/ul	133840	Phenanthrene-d10	16.992

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	n-Hexadecanoic acid	256	C16H32O2	000057-10-3	97		
2	n-Hexadecanoic acid	256	C16H32O2	000057-10-3	94		
3	n-Hexadecanoic acid	256	C16H32O2	000057-10-3	93		
4	Tetradecanoic acid	228	C14H28O2	000544-63-8	91		
5	Tetradecanoic acid	228	C14H28O2	000544-63-8	86		

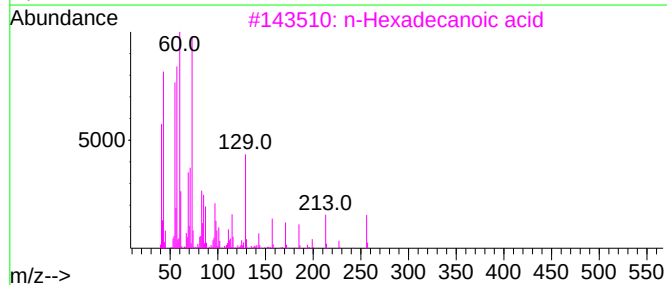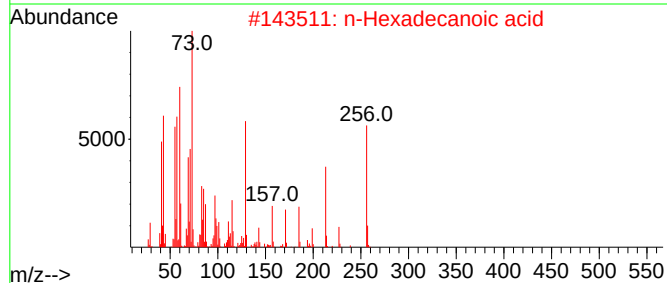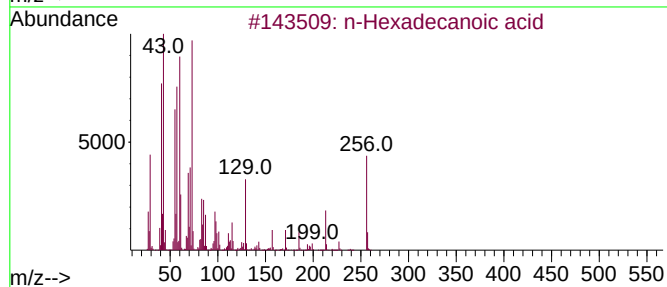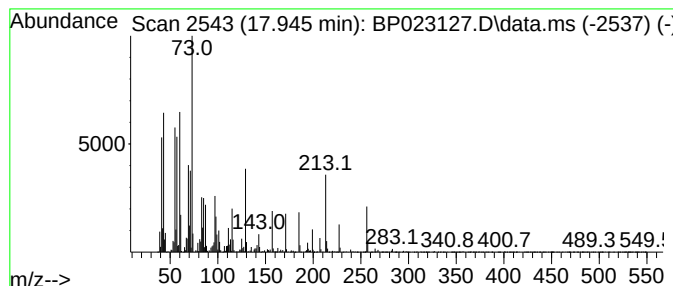

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023127.D
Acq On : 15 Nov 2024 06:38
Operator : RC/JU
Sample : P4740-06
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.375	2.6	ng/ul	48680	1	7.581	374770	20.0
n-Hexadecanoic ...	17.945	2.4	ng/ul	133840	4	16.992	1114510	20.0