

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023128.D
 Acq On : 15 Nov 2024 07:18
 Operator : RC/JU
 Sample : P4784-03
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E27N1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023128.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	32	rVB	15261	19456	0.58%	0.078%
2	3.552	93	96	110	rBV	77137	136499	4.07%	0.547%
3	3.858	144	148	153	rVB	9105	12063	0.36%	0.048%
4	4.287	216	221	225	rVB2	3175	4290	0.13%	0.017%
5	6.710	629	633	638	rVB7	3753	7129	0.21%	0.029%
6	6.787	640	646	664	rVV	79471	171843	5.12%	0.689%
7	6.928	664	670	685	rVB	222650	346646	10.34%	1.389%
8	7.122	696	703	719	rBV	253672	450109	13.42%	1.804%
9	7.581	774	781	791	rBV	266670	430377	12.83%	1.725%
10	8.293	896	902	921	rBV	246380	486006	14.49%	1.948%
11	8.722	968	975	987	rBV	310137	510314	15.21%	2.045%
12	8.857	993	998	1009	rVB6	5921	13864	0.41%	0.056%
13	9.110	1037	1041	1047	rVB7	3406	5207	0.16%	0.021%
14	9.434	1088	1096	1109	rBV	255842	464338	13.84%	1.861%
15	9.734	1141	1147	1154	rBV10	3415	8929	0.27%	0.036%
16	9.969	1180	1187	1211	rBV	317283	708650	21.13%	2.840%
17	10.151	1214	1218	1224	rBV6	5860	13740	0.41%	0.055%
18	10.322	1239	1247	1259	rBV	357472	589544	17.58%	2.362%
19	10.475	1264	1273	1291	rBV	280000	617913	18.42%	2.476%
20	11.169	1385	1391	1398	rBV8	4518	11205	0.33%	0.045%
21	11.687	1473	1479	1484	rVB4	2465	4933	0.15%	0.020%
22	11.928	1516	1520	1529	rVB4	4314	8666	0.26%	0.035%
23	12.522	1617	1621	1626	rBV8	2976	5640	0.17%	0.023%
24	12.781	1660	1665	1672	rBV7	2825	5920	0.18%	0.024%
25	13.075	1710	1715	1722	rVB7	3203	7171	0.21%	0.029%
26	13.610	1800	1806	1819	rBV	829574	1232180	36.74%	4.938%
27	13.886	1844	1853	1865	rBV	776373	1252636	37.35%	5.020%
28	14.198	1897	1906	1921	rBV	495245	928875	27.69%	3.722%
29	14.504	1948	1958	1961	rBV5	34285	91826	2.74%	0.368%
30	14.969	2034	2037	2041	rBV3	4908	7203	0.21%	0.029%
31	15.010	2041	2044	2047	rVV2	3958	5291	0.16%	0.021%
32	15.039	2047	2049	2056	rVB	7171	9617	0.29%	0.039%
33	15.198	2068	2076	2090	rBV	1166676	1781892	53.13%	7.140%
34	15.363	2098	2104	2117	rBV	403857	662279	19.75%	2.654%
35	15.592	2137	2143	2146	rBV3	6843	10567	0.32%	0.042%
36	15.798	2171	2178	2182	rBV9	4060	9409	0.28%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023128.D
 Acq On : 15 Nov 2024 07:18
 Operator : RC/JU
 Sample : P4784-03
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E27N1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

37	16.128	2229	2234	2241	rBV4	5394	9451	0.28%	0.038%
38	16.475	2289	2293	2298	rVV8	3573	6069	0.18%	0.024%
39	16.539	2298	2304	2306	rVV7	1997	3914	0.12%	0.016%
40	16.751	2336	2340	2345	rBV8	2586	6229	0.19%	0.025%
41	16.928	2365	2370	2375	rVV2	80809	89983	2.68%	0.361%
42	16.992	2375	2381	2390	rBV	877085	1312013	39.12%	5.257%
43	17.104	2393	2400	2414	rBV2	1249860	2199222	65.57%	8.813%
44	17.304	2430	2434	2440	rVB2	9968	14316	0.43%	0.057%
45	17.427	2448	2455	2458	rBV9	3531	8248	0.25%	0.033%
46	17.522	2467	2471	2475	rVB7	2286	4002	0.12%	0.016%
47	17.704	2496	2502	2506	rBV5	9720	15588	0.46%	0.062%
48	17.945	2537	2543	2550	rBV2	51174	92712	2.76%	0.372%
49	18.004	2551	2553	2559	rVB	7790	12333	0.37%	0.049%
50	18.386	2614	2618	2623	rBV2	60668	73366	2.19%	0.294%
51	19.039	2725	2729	2735	rBV2	21623	31790	0.95%	0.127%
52	19.116	2738	2742	2748	rBV	22456	35384	1.05%	0.142%
53	19.269	2764	2768	2775	rBV3	37586	52770	1.57%	0.211%
54	19.492	2800	2806	2818	rBV	2152475	2944564	87.79%	11.799%
55	21.439	3131	3137	3150	rBV2	1123653	1782701	53.15%	7.144%
56	24.433	3637	3646	3660	rVB	1459295	3354040	100.00%	13.440%
57	24.662	3676	3685	3695	rBV	765340	1874399	55.88%	7.511%




Sum of corrected areas: 24955321

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023128.D
Acq On : 15 Nov 2024 07:18
Operator : RC/JU
Sample : P4784-03
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27N1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

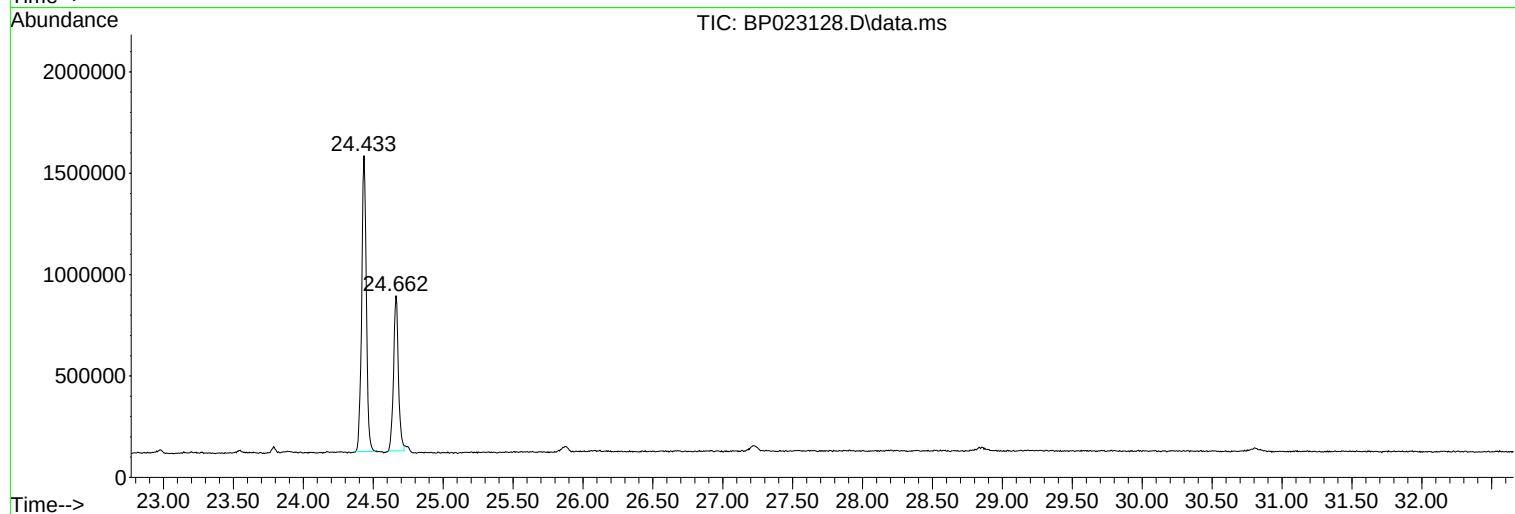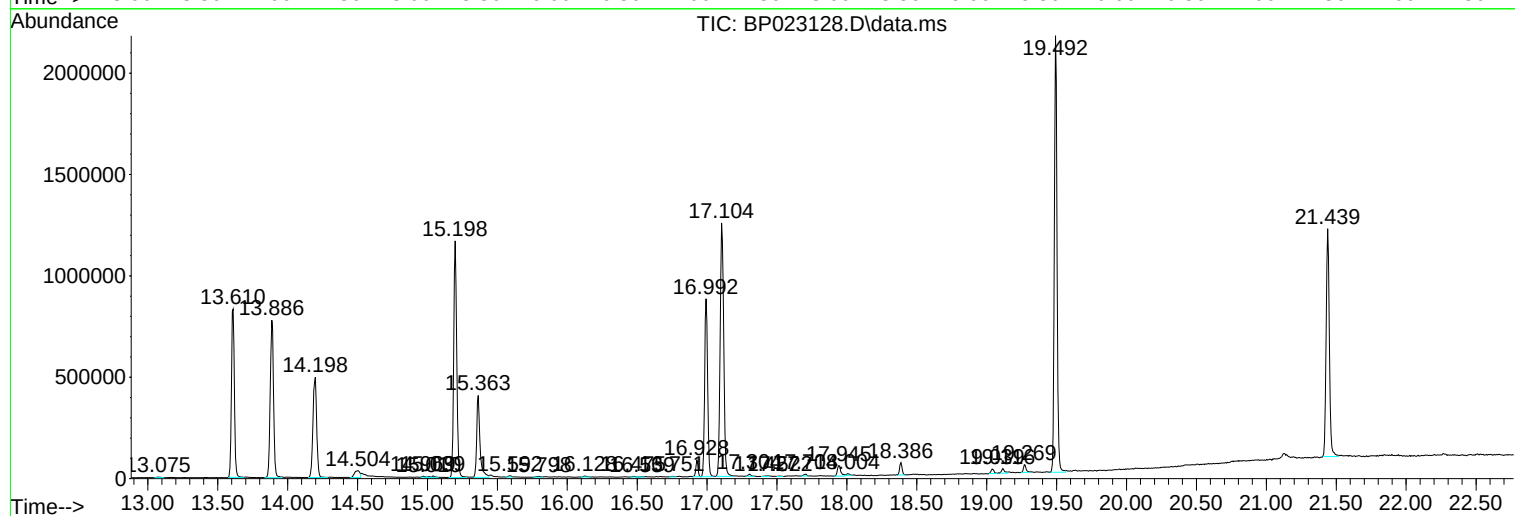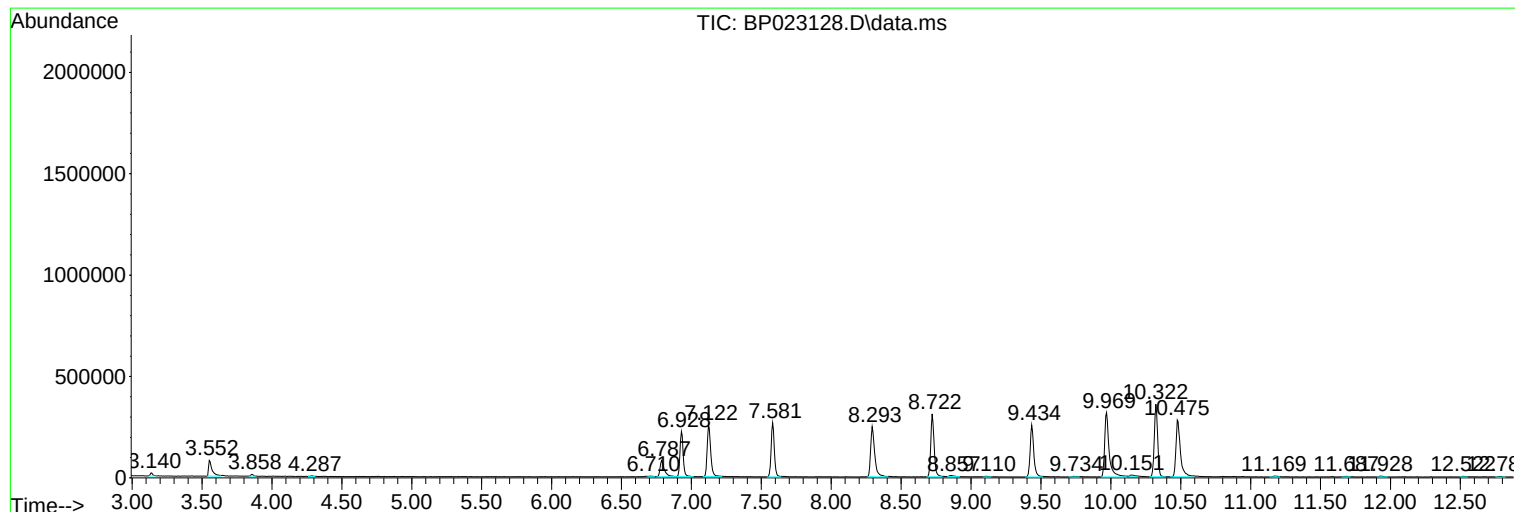

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023128.D
Acq On : 15 Nov 2024 07:18
Operator : RC/JU
Sample : P4784-03
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27N1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023128.D
Acq On : 15 Nov 2024 07:18
Operator : RC/JU
Sample : P4784-03
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27N1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc