

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023135.D
 Acq On : 15 Nov 2024 12:01
 Operator : RC/JU
 Sample : PB164977BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK977

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023135.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	34	rVB	17569	25082	0.97%	0.111%
2	3.552	92	96	115	rBV	192191	337945	13.08%	1.497%
3	3.858	144	148	153	rBV4	4389	6285	0.24%	0.028%
4	6.787	640	646	663	rBV	231268	453562	17.55%	2.010%
5	6.922	663	669	684	rVB	195990	327119	12.66%	1.449%
6	7.128	697	704	718	rBV	272678	458578	17.74%	2.032%
7	7.575	773	780	794	rBV	225189	389656	15.08%	1.726%
8	8.287	894	901	919	rVV	318184	581179	22.49%	2.575%
9	8.716	968	974	991	rBV	264798	483380	18.70%	2.142%
10	8.869	995	1000	1008	rBV2	21458	39199	1.52%	0.174%
11	9.434	1088	1096	1109	rBV	225294	424141	16.41%	1.879%
12	9.981	1181	1189	1214	rBV	290892	668202	25.86%	2.961%
13	10.328	1241	1248	1258	rBV	323542	549894	21.28%	2.436%
14	10.481	1266	1274	1296	rBV	263550	594773	23.01%	2.635%
15	11.957	1518	1525	1533	rBV6	4508	11392	0.44%	0.050%
16	13.599	1798	1804	1823	rBV	676452	1140111	44.12%	5.052%
17	13.887	1846	1853	1868	rBV	861859	1239090	47.95%	5.490%
18	14.204	1899	1907	1919	rBV	612232	879094	34.02%	3.895%
19	14.487	1948	1955	1976	rBV	151045	470304	18.20%	2.084%
20	15.228	2073	2081	2093	rBV	1027837	1671563	64.68%	7.406%
21	15.363	2097	2104	2121	rBV	321662	525830	20.35%	2.330%
22	15.598	2140	2144	2150	rVV9	2293	4020	0.16%	0.018%
23	16.028	2212	2217	2220	rVB6	1890	3490	0.14%	0.015%
24	16.657	2320	2324	2327	rBV6	1524	2788	0.11%	0.012%
25	16.687	2327	2329	2334	rVV5	2280	3687	0.14%	0.016%
26	16.792	2345	2347	2353	rVB6	2844	3520	0.14%	0.016%
27	17.016	2378	2385	2394	rBV	922095	1214347	46.99%	5.381%
28	17.104	2394	2400	2420	rVB2	1330158	1991550	77.06%	8.824%
29	17.704	2499	2502	2506	rBV6	2366	3741	0.14%	0.017%
30	17.963	2540	2546	2547	rBV5	3076	4559	0.18%	0.020%
31	18.263	2593	2597	2598	rBV4	2181	2751	0.11%	0.012%
32	19.034	2723	2728	2735	rBV2	24720	38534	1.49%	0.171%
33	19.128	2740	2744	2747	rVV3	13359	18512	0.72%	0.082%
34	19.498	2800	2807	2817	rBV	1431853	2434290	94.19%	10.786%
35	21.451	3134	3139	3148	rBV2	884766	1443739	55.87%	6.397%
36	24.451	3640	3649	3669	rVB	879732	2584319	100.00%	11.451%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023135.D
Acq On : 15 Nov 2024 12:01
Operator : RC/JU
Sample : PB164977BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK977

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	24.674	3679	3687	3707	rVB	501385	1539082	59.55%	6.819%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 22569308

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023135.D
Acq On : 15 Nov 2024 12:01
Operator : RC/JU
Sample : PB164977BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK977

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

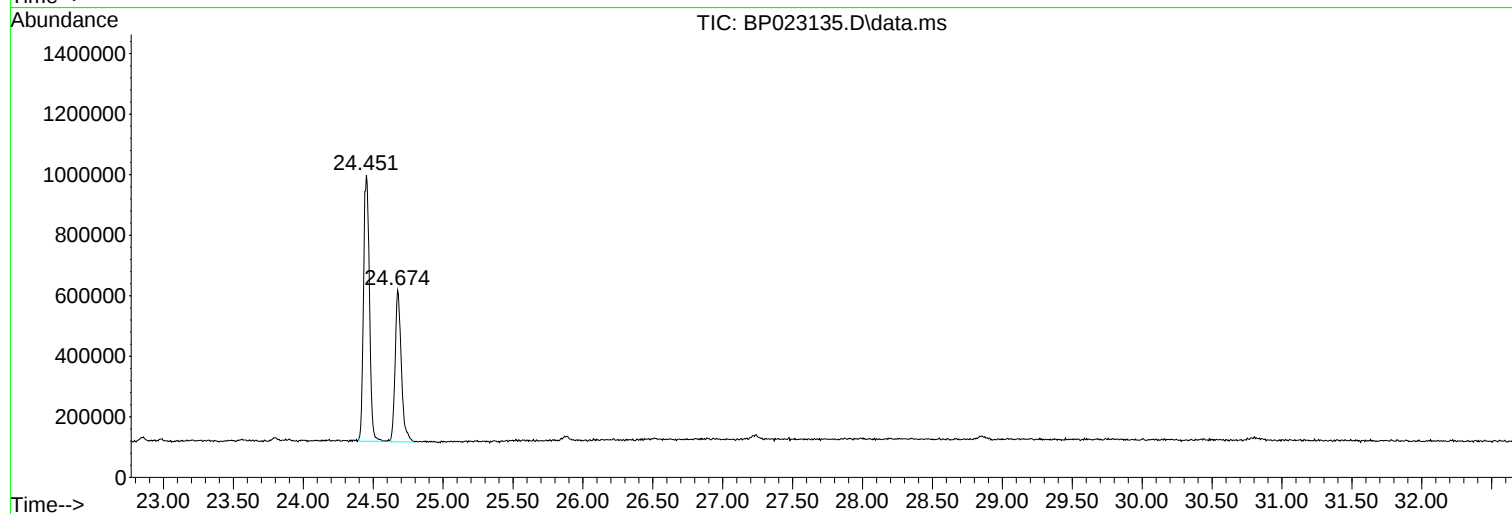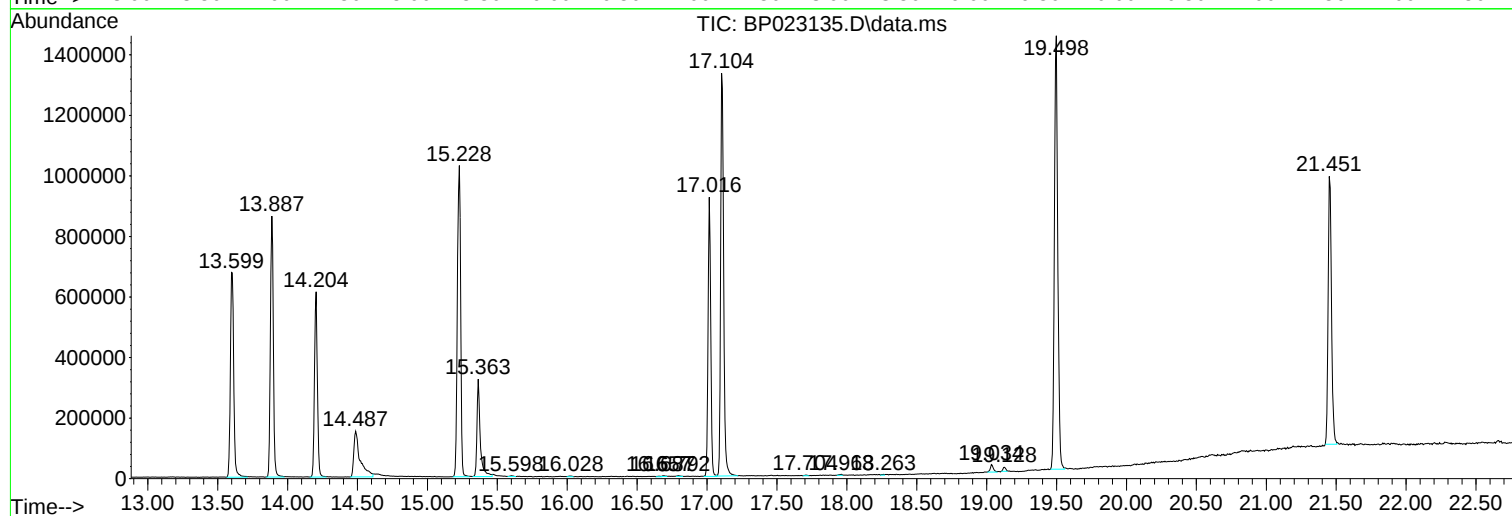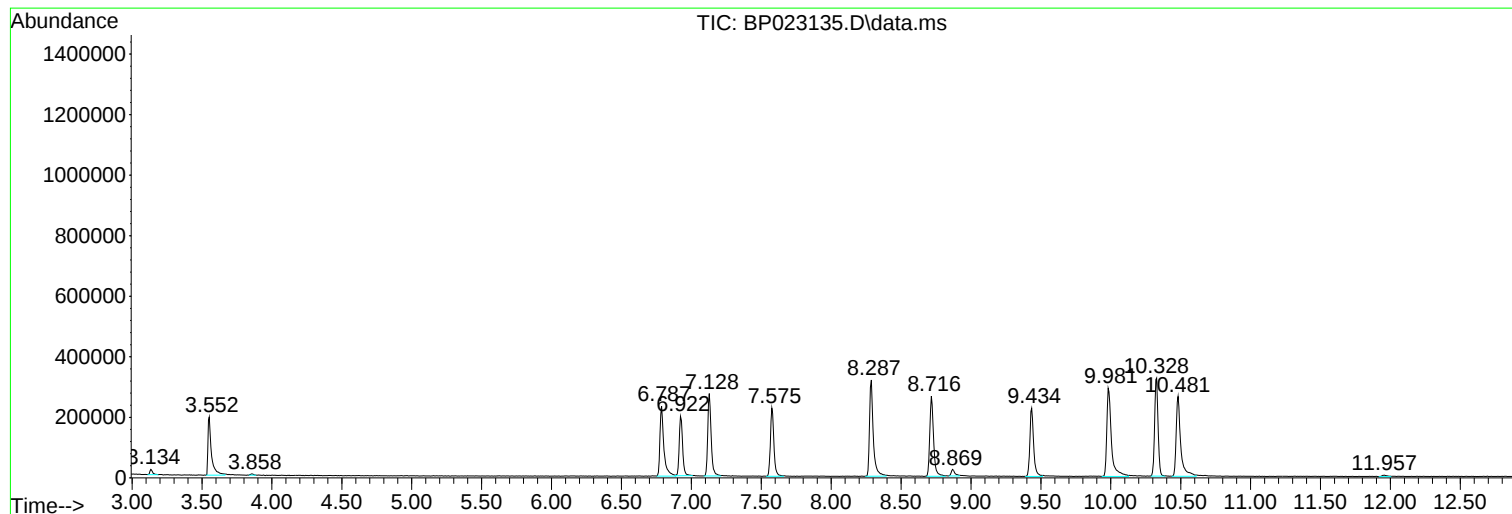

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023135.D
Acq On : 15 Nov 2024 12:01
Operator : RC/JU
Sample : PB164977BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK977

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023135.D
Acq On : 15 Nov 2024 12:01
Operator : RC/JU
Sample : PB164977BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK977

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
