

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023143.D
 Acq On : 15 Nov 2024 17:26
 Operator : RC/JU
 Sample : P4784-18
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E27P6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.052	9	11	16	rVB6	1785	2543	0.19%	0.030%
2	3.134	22	25	35	rVB	9124	13478	1.02%	0.160%
3	3.570	96	99	108	rBV	17873	37883	2.87%	0.450%
4	3.793	135	137	141	rBV5	953	1481	0.11%	0.018%
5	3.858	144	148	158	rVB8	3143	6875	0.52%	0.082%
6	5.869	486	490	493	rBV5	909	1523	0.12%	0.018%
7	6.205	543	547	549	rVB5	960	1415	0.11%	0.017%
8	6.493	594	596	602	rBV7	875	1372	0.10%	0.016%
9	6.805	643	649	666	rBV3	16969	54198	4.11%	0.644%
10	6.934	666	671	682	rVV	39884	68410	5.19%	0.812%
11	7.128	699	704	716	rBV	43479	86081	6.53%	1.022%
12	7.581	774	781	800	rBV	175226	352266	26.72%	4.183%
13	8.316	898	906	926	rBV2	37752	106438	8.07%	1.264%
14	8.734	969	977	993	rBV	46250	100732	7.64%	1.196%
15	9.446	1089	1098	1116	rBV3	33686	86061	6.53%	1.022%
16	10.010	1186	1194	1214	rBV2	34198	123444	9.36%	1.466%
17	10.328	1238	1248	1260	rBV	259031	471532	35.77%	5.599%
18	10.504	1271	1278	1287	rBV2	36484	97062	7.36%	1.152%
19	13.181	1728	1733	1738	rBV3	3446	4976	0.38%	0.059%
20	13.604	1797	1805	1819	rBV	129490	241265	18.30%	2.865%
21	13.887	1845	1853	1868	rVV	153890	247318	18.76%	2.936%
22	13.987	1868	1870	1876	rVB7	930	1328	0.10%	0.016%
23	14.198	1900	1906	1920	rBV	515717	736104	55.84%	8.740%
24	14.451	1944	1949	1952	rVB5	904	1532	0.12%	0.018%
25	14.557	1962	1967	1975	rBV6	6799	17699	1.34%	0.210%
26	15.216	2072	2079	2091	rBV	254544	352578	26.74%	4.186%
27	15.381	2098	2107	2120	rBV3	28748	70985	5.38%	0.843%
28	15.475	2120	2123	2129	rVB8	1982	3451	0.26%	0.041%
29	15.604	2141	2145	2149	rVB6	2425	3108	0.24%	0.037%
30	15.869	2187	2190	2193	rVB5	1361	1605	0.12%	0.019%
31	16.310	2259	2265	2267	rBV7	921	1508	0.11%	0.018%
32	17.010	2377	2384	2395	rBV	699801	1020491	77.41%	12.117%
33	17.110	2395	2401	2420	rVB2	245629	418591	31.75%	4.970%
34	17.263	2426	2427	2431	rVB4	1894	1676	0.13%	0.020%
35	17.386	2446	2448	2449	rBV2	2177	1485	0.11%	0.018%
36	17.410	2449	2452	2454	rVV4	1410	1752	0.13%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023143.D
Acq On : 15 Nov 2024 17:26
Operator : RC/JU
Sample : P4784-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27P6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	17.481	2462	2464	2467	rVB3	1426	1458	0.11%	0.017%
38	17.510	2467	2469	2471	rBV3	1331	1332	0.10%	0.016%
39	17.945	2539	2543	2551	rBV7	9780	15448	1.17%	0.183%
40	18.016	2553	2555	2563	rVB9	1830	2928	0.22%	0.035%
41	18.198	2584	2586	2591	rBV6	1458	1991	0.15%	0.024%
42	18.322	2604	2607	2609	rBV4	1503	2144	0.16%	0.025%
43	18.345	2609	2611	2614	rVV4	1453	1730	0.13%	0.021%
44	19.039	2725	2729	2734	rBV8	6713	14335	1.09%	0.170%
45	19.080	2734	2736	2737	rBV2	2584	1786	0.14%	0.021%
46	19.422	2792	2794	2795	rBV2	2965	2008	0.15%	0.024%
47	19.504	2802	2808	2815	rBV	349613	520712	39.50%	6.183%
48	21.439	3131	3137	3152	rBV2	742474	1289896	97.84%	15.315%
49	24.439	3639	3647	3656	rVB	211225	507950	38.53%	6.031%
50	24.651	3675	3683	3694	rBV	451100	1318317	100.00%	15.653%


Sum of corrected areas: 8422281

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023143.D
Acq On : 15 Nov 2024 17:26
Operator : RC/JU
Sample : P4784-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27P6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

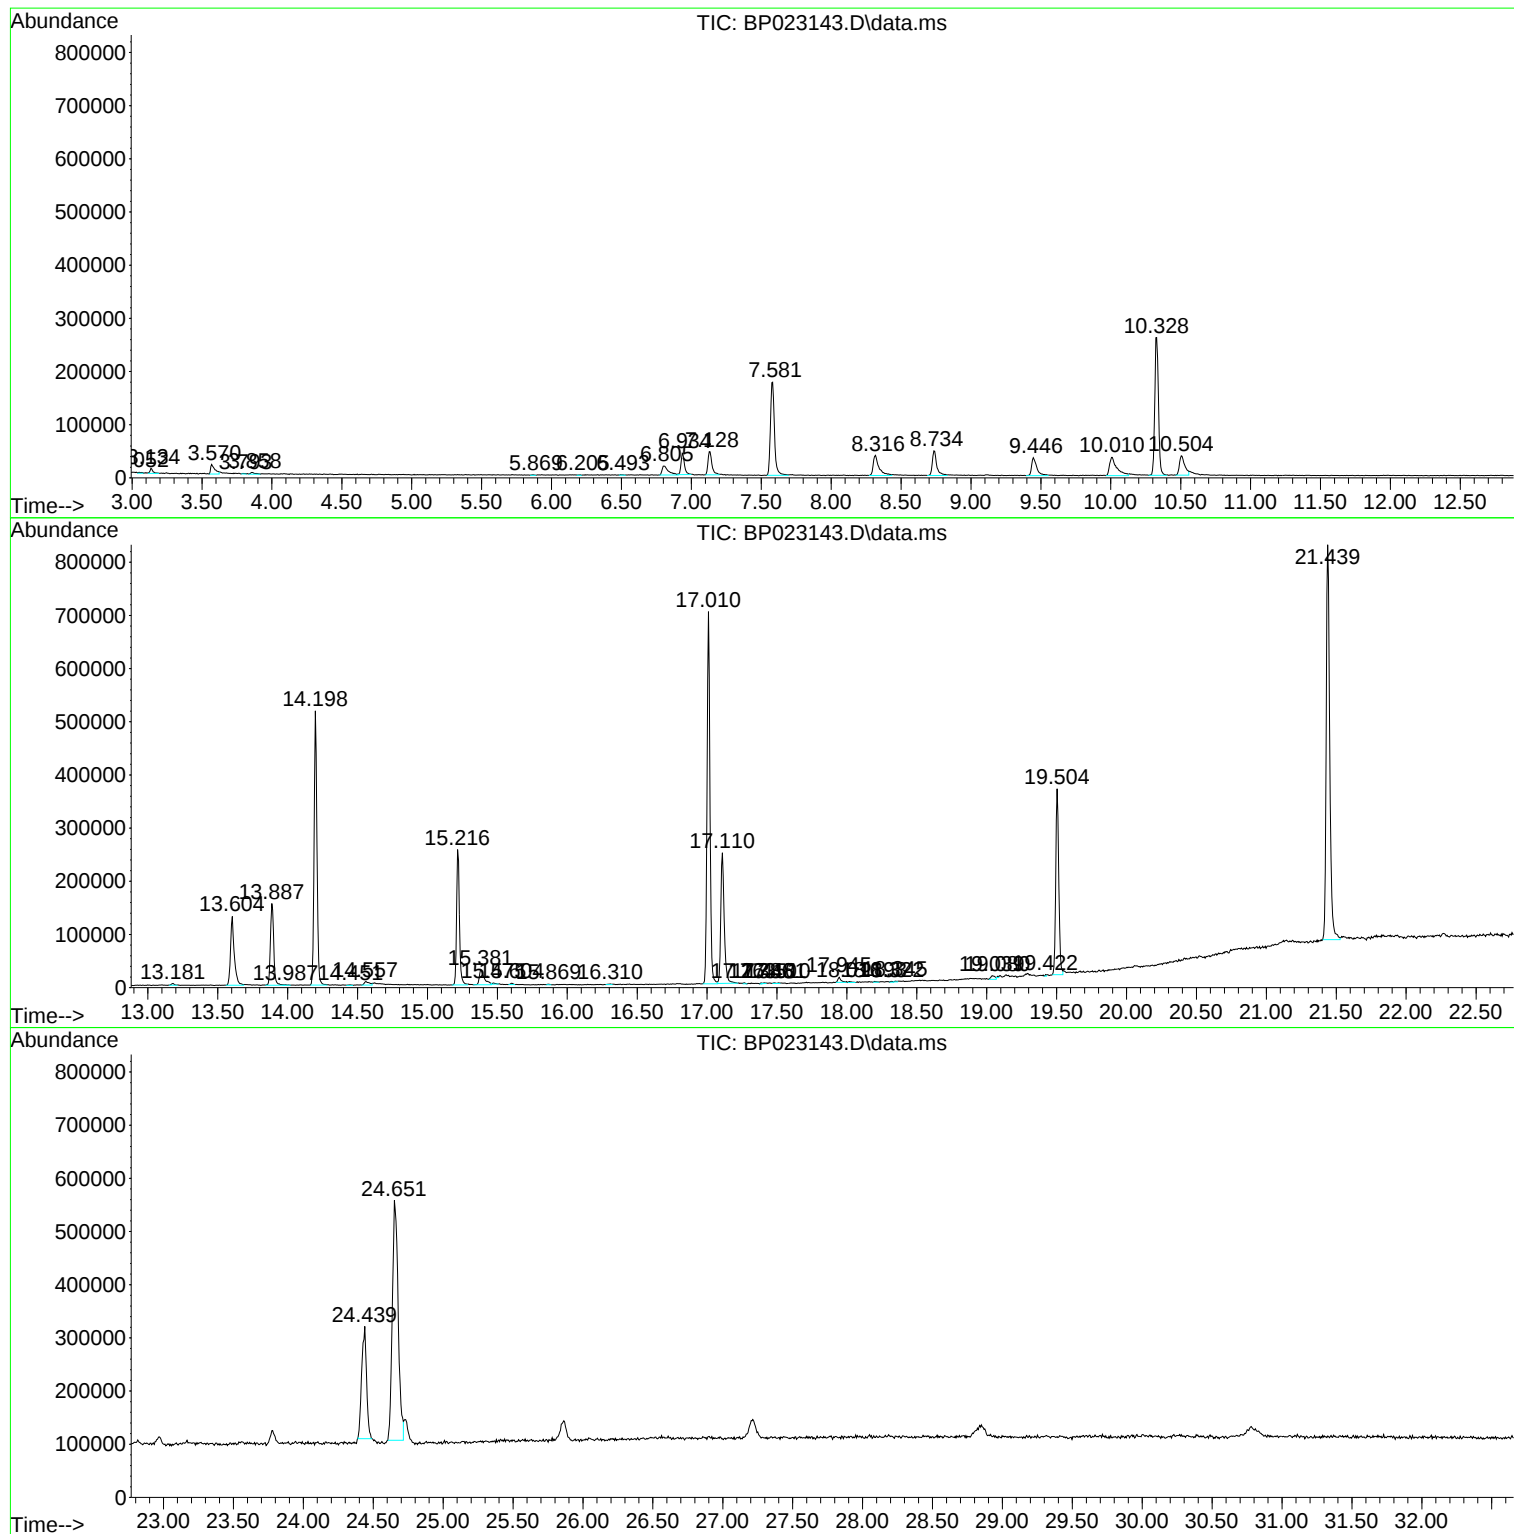

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023143.D
Acq On : 15 Nov 2024 17:26
Operator : RC/JU
Sample : P4784-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27P6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023143.D
Acq On : 15 Nov 2024 17:26
Operator : RC/JU
Sample : P4784-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27P6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
