

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
 Data File : BP023157.D
 Acq On : 16 Nov 2024 03:42
 Operator : RC/JU
 Sample : P4784-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E27P5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023157.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	33	rVB	18707	25637	0.97%	0.133%
2	3.558	93	97	107	rBV	35753	69381	2.62%	0.359%
3	4.275	217	219	226	rVB3	2729	3932	0.15%	0.020%
4	6.716	629	634	636	rBV4	2247	3337	0.13%	0.017%
5	6.787	640	646	663	rBV	66654	162070	6.12%	0.839%
6	6.922	663	669	680	rVV	176515	276422	10.43%	1.431%
7	7.122	697	703	721	rBV	215681	375148	14.16%	1.942%
8	7.575	773	780	792	rBV	184599	325934	12.30%	1.687%
9	8.281	894	900	923	rBV	210923	427997	16.15%	2.216%
10	8.716	967	974	989	rBV	219888	420990	15.89%	2.179%
11	8.869	995	1000	1003	rBV5	1641	2749	0.10%	0.014%
12	9.110	1035	1041	1043	rBV6	2106	3567	0.13%	0.018%
13	9.428	1084	1095	1104	rBV	205234	374201	14.12%	1.937%
14	9.975	1181	1188	1214	rBV	249992	593748	22.41%	3.074%
15	10.322	1240	1247	1264	rVB	258993	443168	16.73%	2.294%
16	10.469	1265	1272	1291	rBV	202454	452449	17.08%	2.342%
17	11.181	1389	1393	1397	rBV7	1454	2788	0.11%	0.014%
18	11.945	1518	1523	1527	rBV6	2503	4772	0.18%	0.025%
19	13.163	1724	1730	1736	rBV6	1739	3439	0.13%	0.018%
20	13.604	1798	1805	1820	rBV	779728	1029153	38.84%	5.328%
21	13.886	1844	1853	1869	rBV	656524	1039462	39.23%	5.381%
22	14.198	1898	1906	1915	rBV	388622	702403	26.51%	3.636%
23	14.381	1930	1937	1943	rVB	4161	7088	0.27%	0.037%
24	14.504	1954	1958	1974	rBV5	24395	108817	4.11%	0.563%
25	14.616	1974	1977	1982	rVV5	18898	32288	1.22%	0.167%
26	14.686	1985	1989	1995	rVB8	4889	9329	0.35%	0.048%
27	14.875	2015	2021	2033	rBV	72084	108061	4.08%	0.559%
28	14.981	2035	2039	2043	rVV7	2573	4621	0.17%	0.024%
29	15.039	2046	2049	2055	rVB6	1977	2721	0.10%	0.014%
30	15.210	2070	2078	2094	rBV	849940	1532796	57.85%	7.935%
31	15.363	2098	2104	2116	rBV	362404	584241	22.05%	3.024%
32	16.692	2325	2330	2333	rBV7	2551	4380	0.17%	0.023%
33	17.004	2376	2383	2395	rBV	619811	1018225	38.43%	5.271%
34	17.116	2395	2402	2415	rVV	1311831	2054990	77.56%	10.638%
35	17.463	2456	2461	2463	rBV5	1922	3742	0.14%	0.019%
36	17.945	2538	2543	2552	rBV8	12778	21124	0.80%	0.109%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023157.D
Acq On : 16 Nov 2024 03:42
Operator : RC/JU
Sample : P4784-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27P5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Title : SVOA CALIBRATION

37	18.027	2553	2557	2559	rVV3	2581	3703	0.14%	0.019%
38	18.163	2575	2580	2584	rBV7	3456	6778	0.26%	0.035%
39	18.710	2670	2673	2676	rBV4	2305	3088	0.12%	0.016%
40	19.033	2724	2728	2735	rVB2	22775	30944	1.17%	0.160%
41	19.110	2737	2741	2746	rBV2	13621	24386	0.92%	0.126%
42	19.151	2746	2748	2752	rVB4	3864	4528	0.17%	0.023%
43	19.286	2767	2771	2775	rBV5	12715	20011	0.76%	0.104%
44	19.486	2798	2805	2818	rBV	1730976	2649686	100.00%	13.716%
45	21.445	3133	3138	3152	rBV	787576	1316353	49.68%	6.814%
46	24.439	3638	3647	3648	rBV	974174	1501983	56.69%	7.775%
47	24.674	3678	3687	3709	rVB	477364	1521117	57.41%	7.874%




Sum of corrected areas: 19317747

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023157.D
Acq On : 16 Nov 2024 03:42
Operator : RC/JU
Sample : P4784-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27P5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

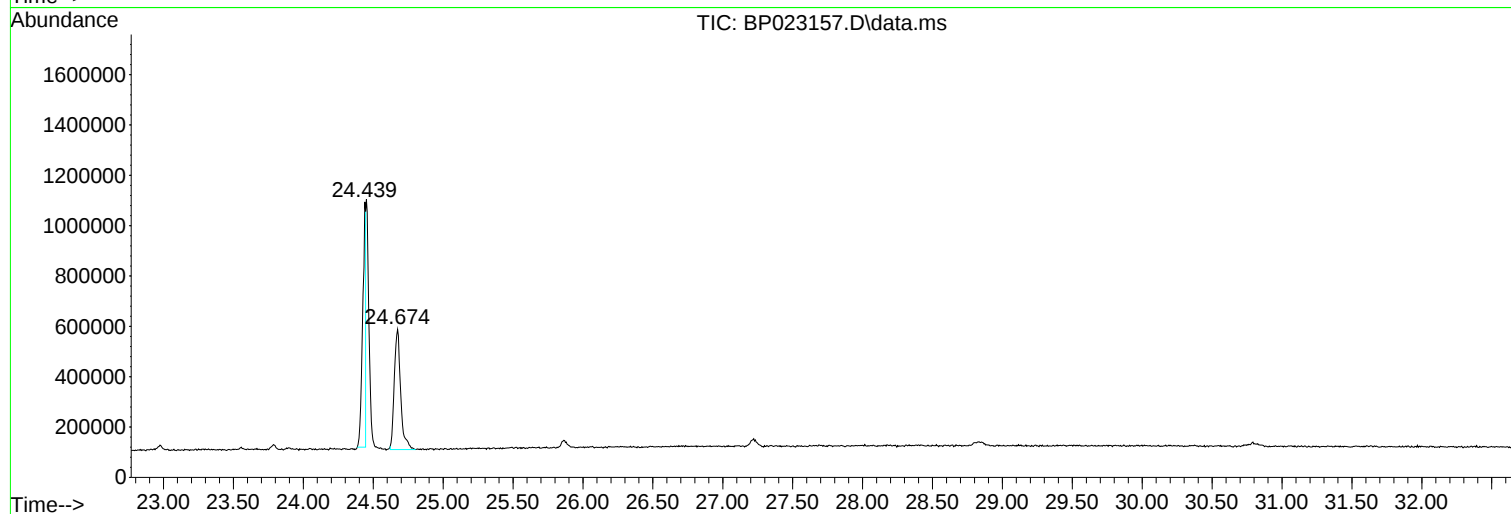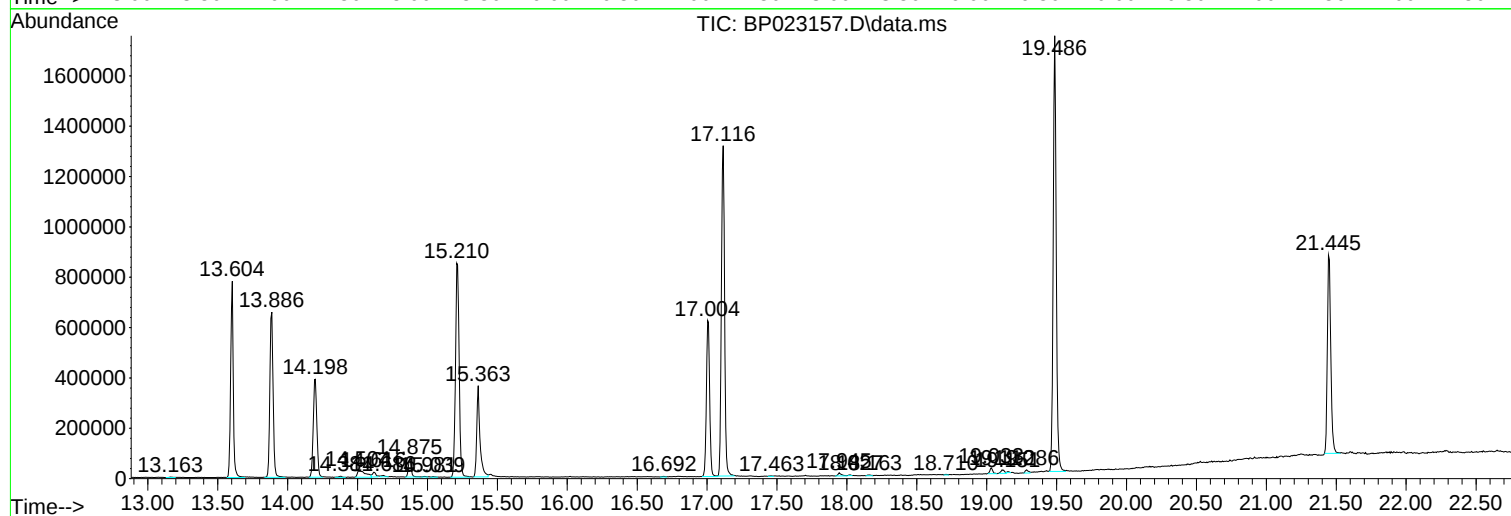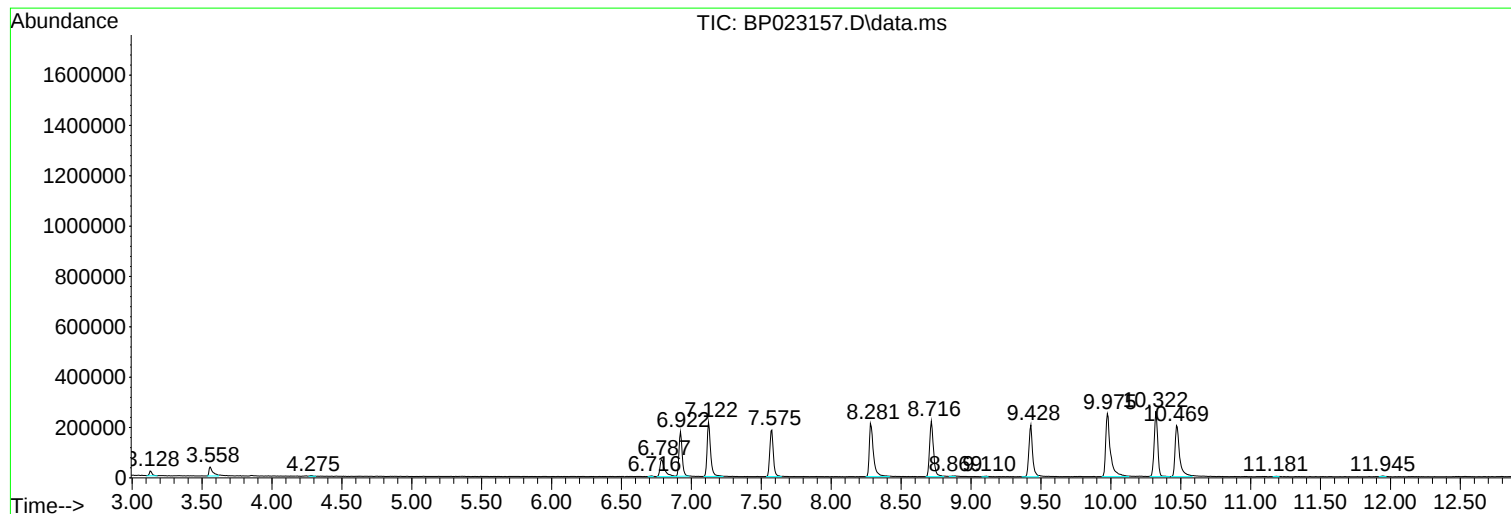

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023157.D
Acq On : 16 Nov 2024 03:42
Operator : RC/JU
Sample : P4784-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27P5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP111324\
Data File : BP023157.D
Acq On : 16 Nov 2024 03:42
Operator : RC/JU
Sample : P4784-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E27P5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP110924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc