

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012811.D
 Acq On : 28 Nov 2022 11:53
 Operator : CG/JU
 Sample : N5710-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KY4

Quant Time: Nov 28 22:37:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	455542	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	2059023	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	1402869	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.410	188	3156943	20.000	ng/ul	0.00
79) Chrysene-d12	21.492	240	3224649	20.000	ng/ul	0.00
88) Perylene-d12	24.010	264	3241506	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	41726	3.925	ng/uL	0.00
4) Pyridine-d5	3.822	84	217475	6.836	ng/ul	0.00
7) Phenol-d5	7.163	99	181018	4.836	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	608311	26.372	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	559359	19.611	ng/ul	0.00
15) 4-Methylphenol-d8	8.716	113	373504	12.384	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	347221	27.552	ng/ul	0.00
24) 2-Nitrophenol-d4	9.904	143	332149	24.822	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.446	165	727721	23.308	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	931806	21.794	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	2948266	30.532	ng/ul	0.00
49) Acenaphthylene-d8	14.345	160	3057884	27.141	ng/ul	0.00
54) 4-Nitrophenol-d4	14.834	143	49562	2.879	ng/ul	0.00
60) Fluorene-d10	15.645	176	2583591	30.551	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	214460	14.213	ng/ul	0.00
73) Anthracene-d10	17.504	188	4400604	31.667	ng/ul	0.00
81) Pyrene-d10	19.733	212	5272065	28.137	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.851	264	4969941	31.214	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.187	94	69674	1.775	ng/ul	96
16) Acetophenone	8.840	105	61049	1.277	ng/ul	98
59) Diethylphthalate	15.463	149	1231264	12.566	ng/ul	100
78) Di-n-butylphthalate	18.351	149	288467	1.730	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012811.D
Acq On : 28 Nov 2022 11:53
Operator : CG/JU
Sample : N5710-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COKY4

Quant Time: Nov 28 22:37:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration




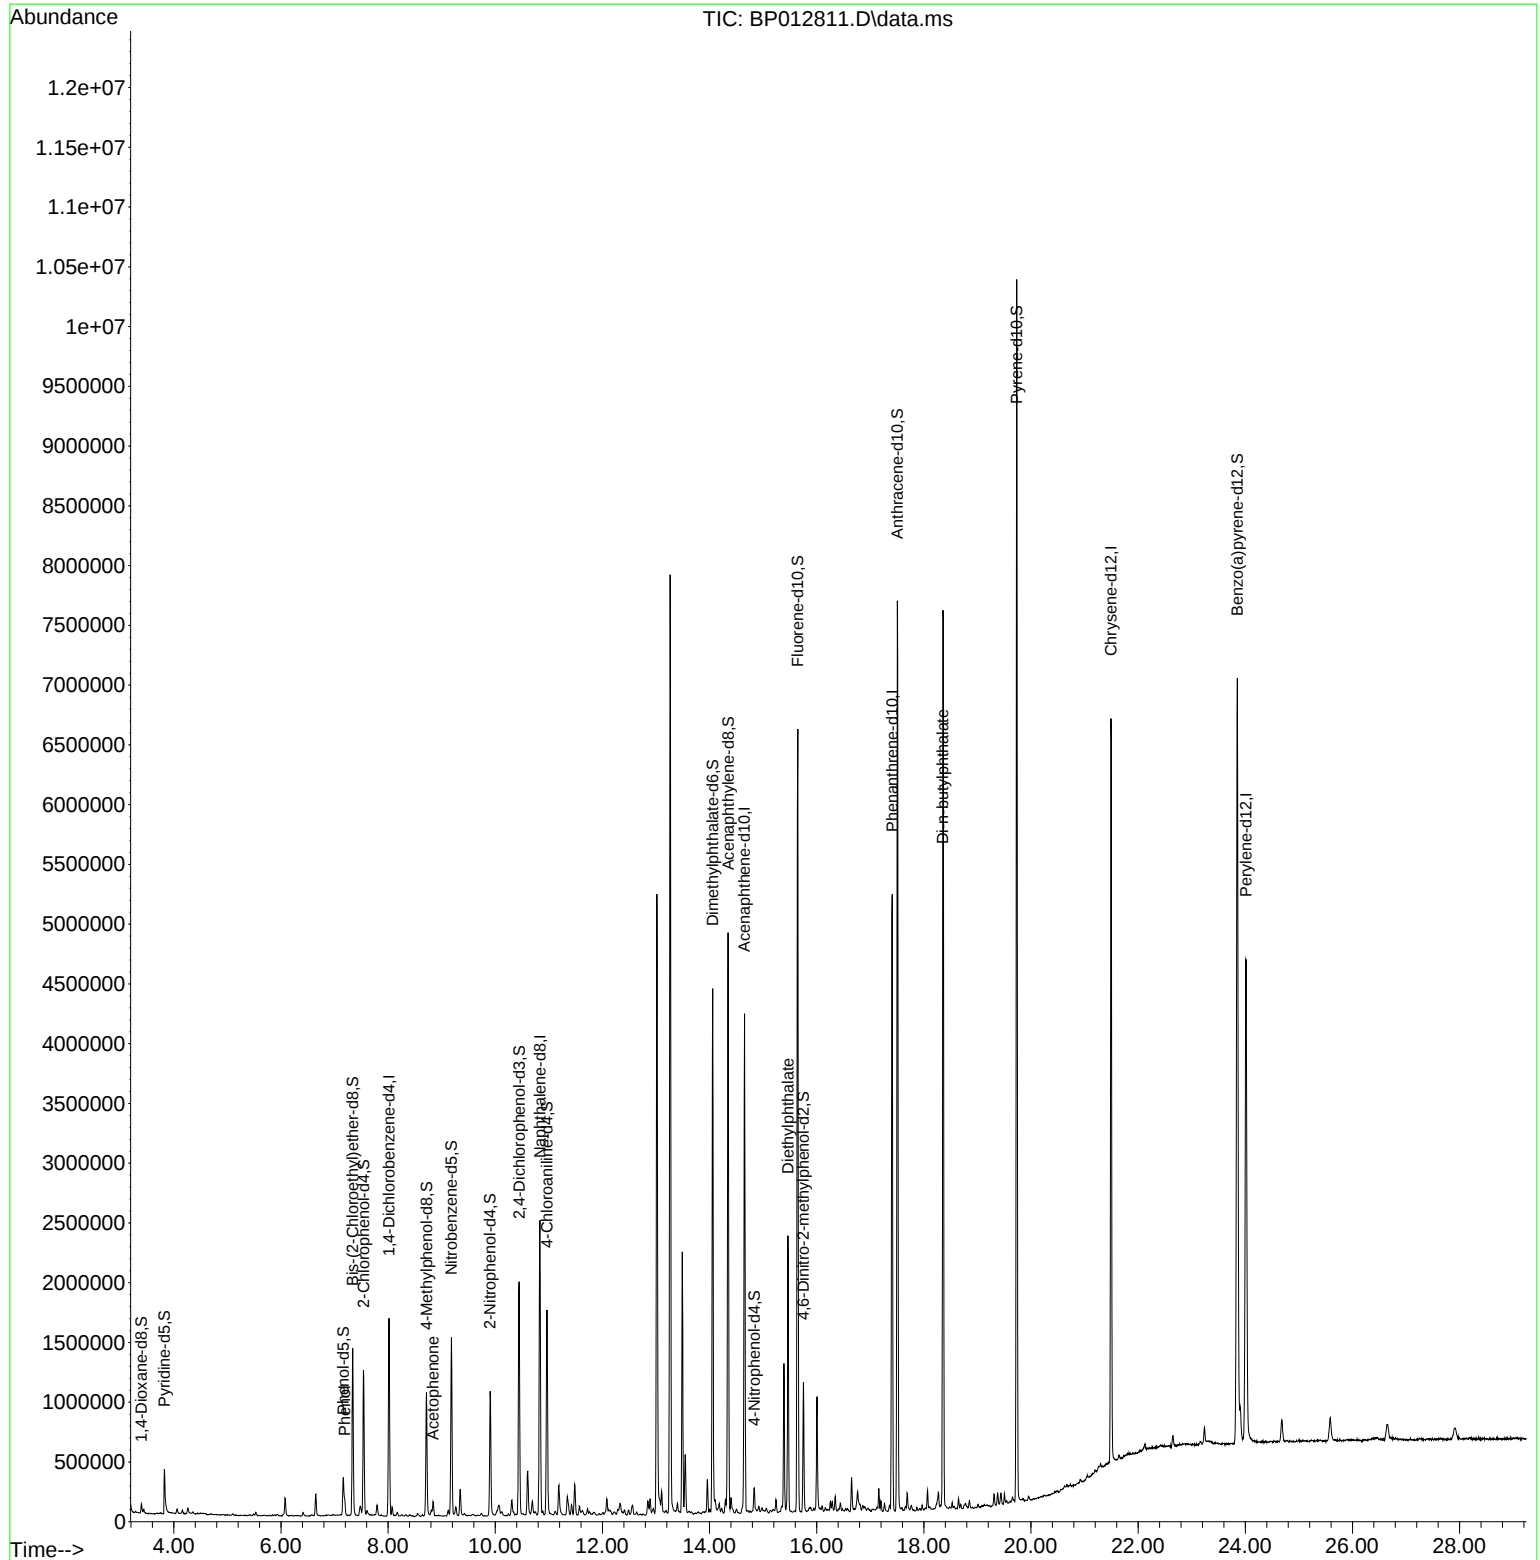


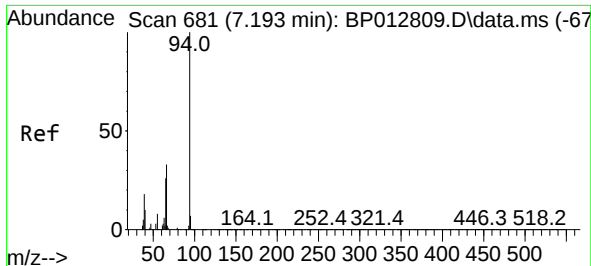

#8
Phenol
Concen: 1.775 ng/ul
RT: 7.187 min Scan# 61
Delta R.T. -0.006 min
Lab File: BP012811.D
Acq: 28 Nov 2022 11:53




Instrument :
BNA_P
ClientSampleId :
COKY4


Tgt Ion: 94 Resp: 69674
Ion Ratio Lower Upper
94 100
65 30.1 20.9 31.3
66 32.7 26.0 39.0

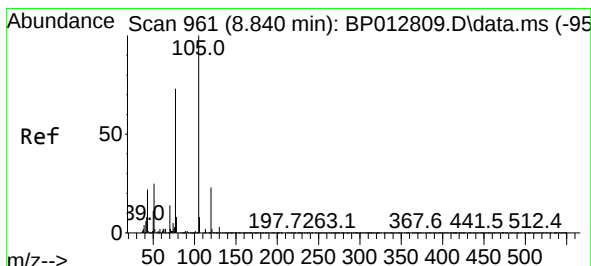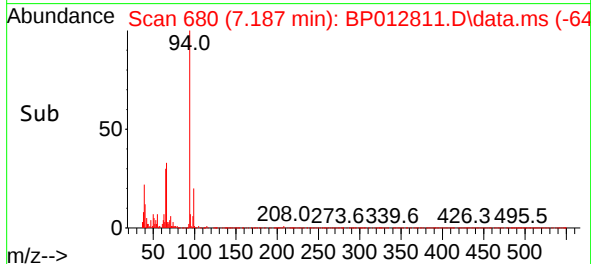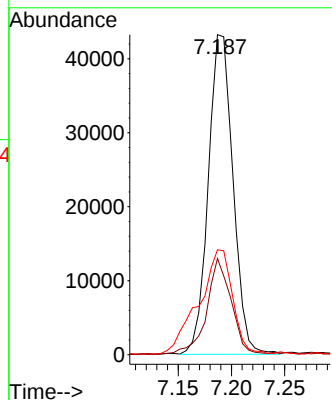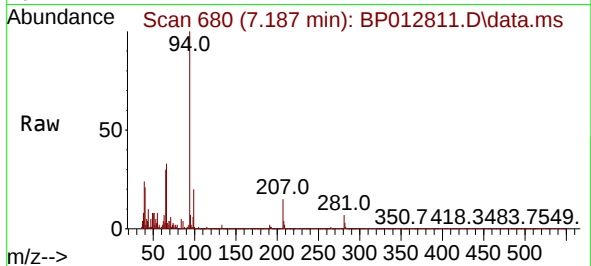

#16
Acetophenone
Concen: 1.277 ng/ul
RT: 8.840 min Scan# 961
Delta R.T. -0.006 min
Lab File: BP012811.D
Acq: 28 Nov 2022 11:53

Tgt Ion: 105 Resp: 61049
Ion Ratio Lower Upper
105 100
77 72.1 59.7 89.5
51 25.9 20.9 31.3


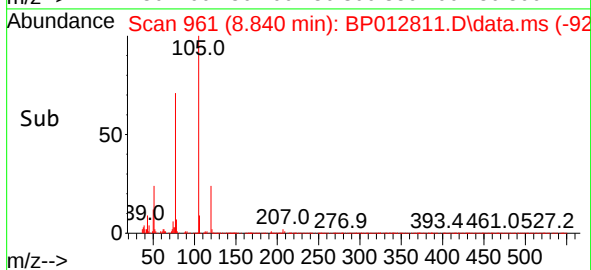
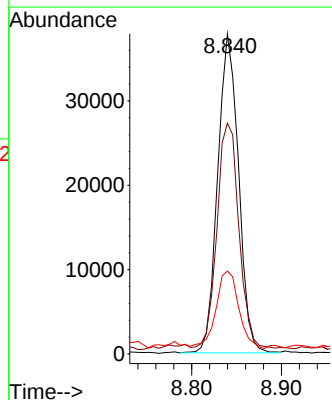
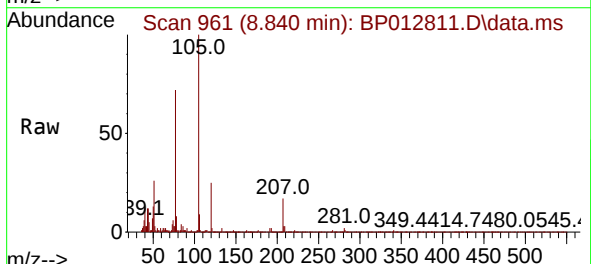


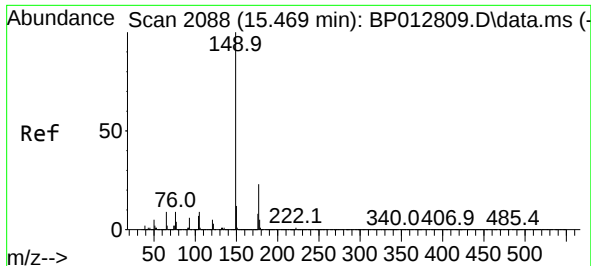

#59
Diethylphthalate
Concen: 12.566 ng/ul
RT: 15.463 min Scan# 2088
Delta R.T. -0.012 min
Lab File: BP012811.D
Acq: 28 Nov 2022 11:53

Instrument :
BNA_P
ClientSampleId :
C0KY4

Tgt Ion:149 Resp: 1231264
Ion Ratio Lower Upper
149 100
177 22.6 18.1 27.1
150 12.2 9.8 14.8

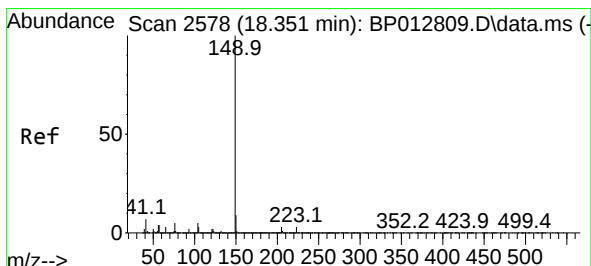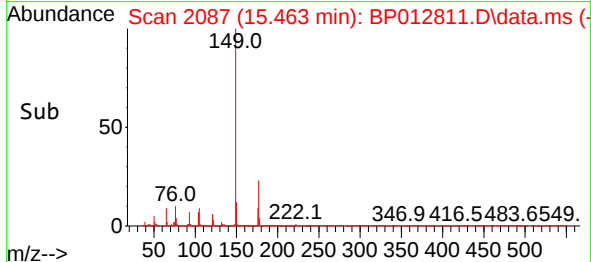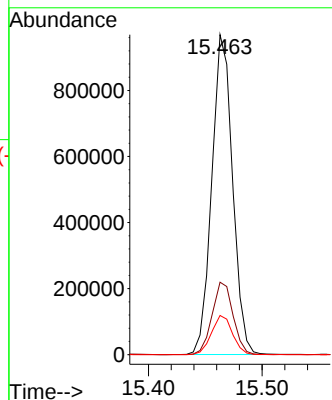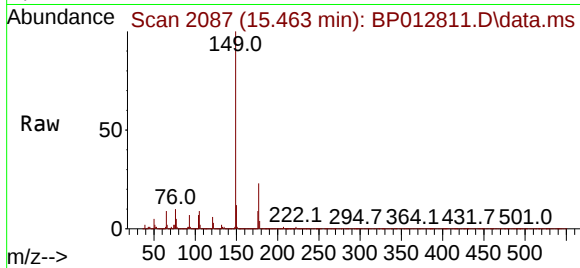

#78
Di-n-butylphthalate
Concen: 1.730 ng/ul
RT: 18.351 min Scan# 2578
Delta R.T. -0.006 min
Lab File: BP012811.D
Acq: 28 Nov 2022 11:53

Tgt Ion:149 Resp: 288467
Ion Ratio Lower Upper
149 100
150 12.4 7.2 10.8#
104 5.0 3.7 5.5

