

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012812.D
 Acq On : 28 Nov 2022 12:27
 Operator : CG/JU
 Sample : N5710-17
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0L03

Quant Time: Nov 28 22:38:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	538150	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	2425844	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	1648134	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.404	188	3697504	20.000	ng/ul	0.00
79) Chrysene-d12	21.492	240	3769716	20.000	ng/ul	0.00
88) Perylene-d12	24.010	264	3765340	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	51894	4.132	ng/uL	0.00
4) Pyridine-d5	3.822	84	265925	7.076	ng/ul	0.00
7) Phenol-d5	7.163	99	267788	6.056	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	810834	29.757	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	777869	23.085	ng/ul	0.00
15) 4-Methylphenol-d8	8.716	113	524959	14.734	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	483520	32.566	ng/ul	0.00
24) 2-Nitrophenol-d4	9.910	143	474295	30.085	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.446	165	984852	26.773	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	1241523	24.647	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	3740613	32.973	ng/ul	0.00
49) Acenaphthylene-d8	14.345	160	4099181	30.969	ng/ul	0.00
54) 4-Nitrophenol-d4	14.834	143	81669	4.038	ng/ul	0.00
60) Fluorene-d10	15.645	176	3276904	32.983	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	324519	18.363	ng/ul	0.00
73) Anthracene-d10	17.504	188	5536654	34.017	ng/ul	0.00
81) Pyrene-d10	19.733	212	6681870	30.505	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.845	264	6360563	34.391	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.193	94	98983	2.135	ng/ul	98
16) Acetophenone	8.840	105	80769	1.430	ng/ul	95
59) Diethylphthalate	15.463	149	1572094	13.657	ng/ul	100
78) Di-n-butylphthalate	18.351	149	387386	1.984	ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012812.D
Acq On : 28 Nov 2022 12:27
Operator : CG/JU
Sample : N5710-17
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
COL03

Quant Time: Nov 28 22:38:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration




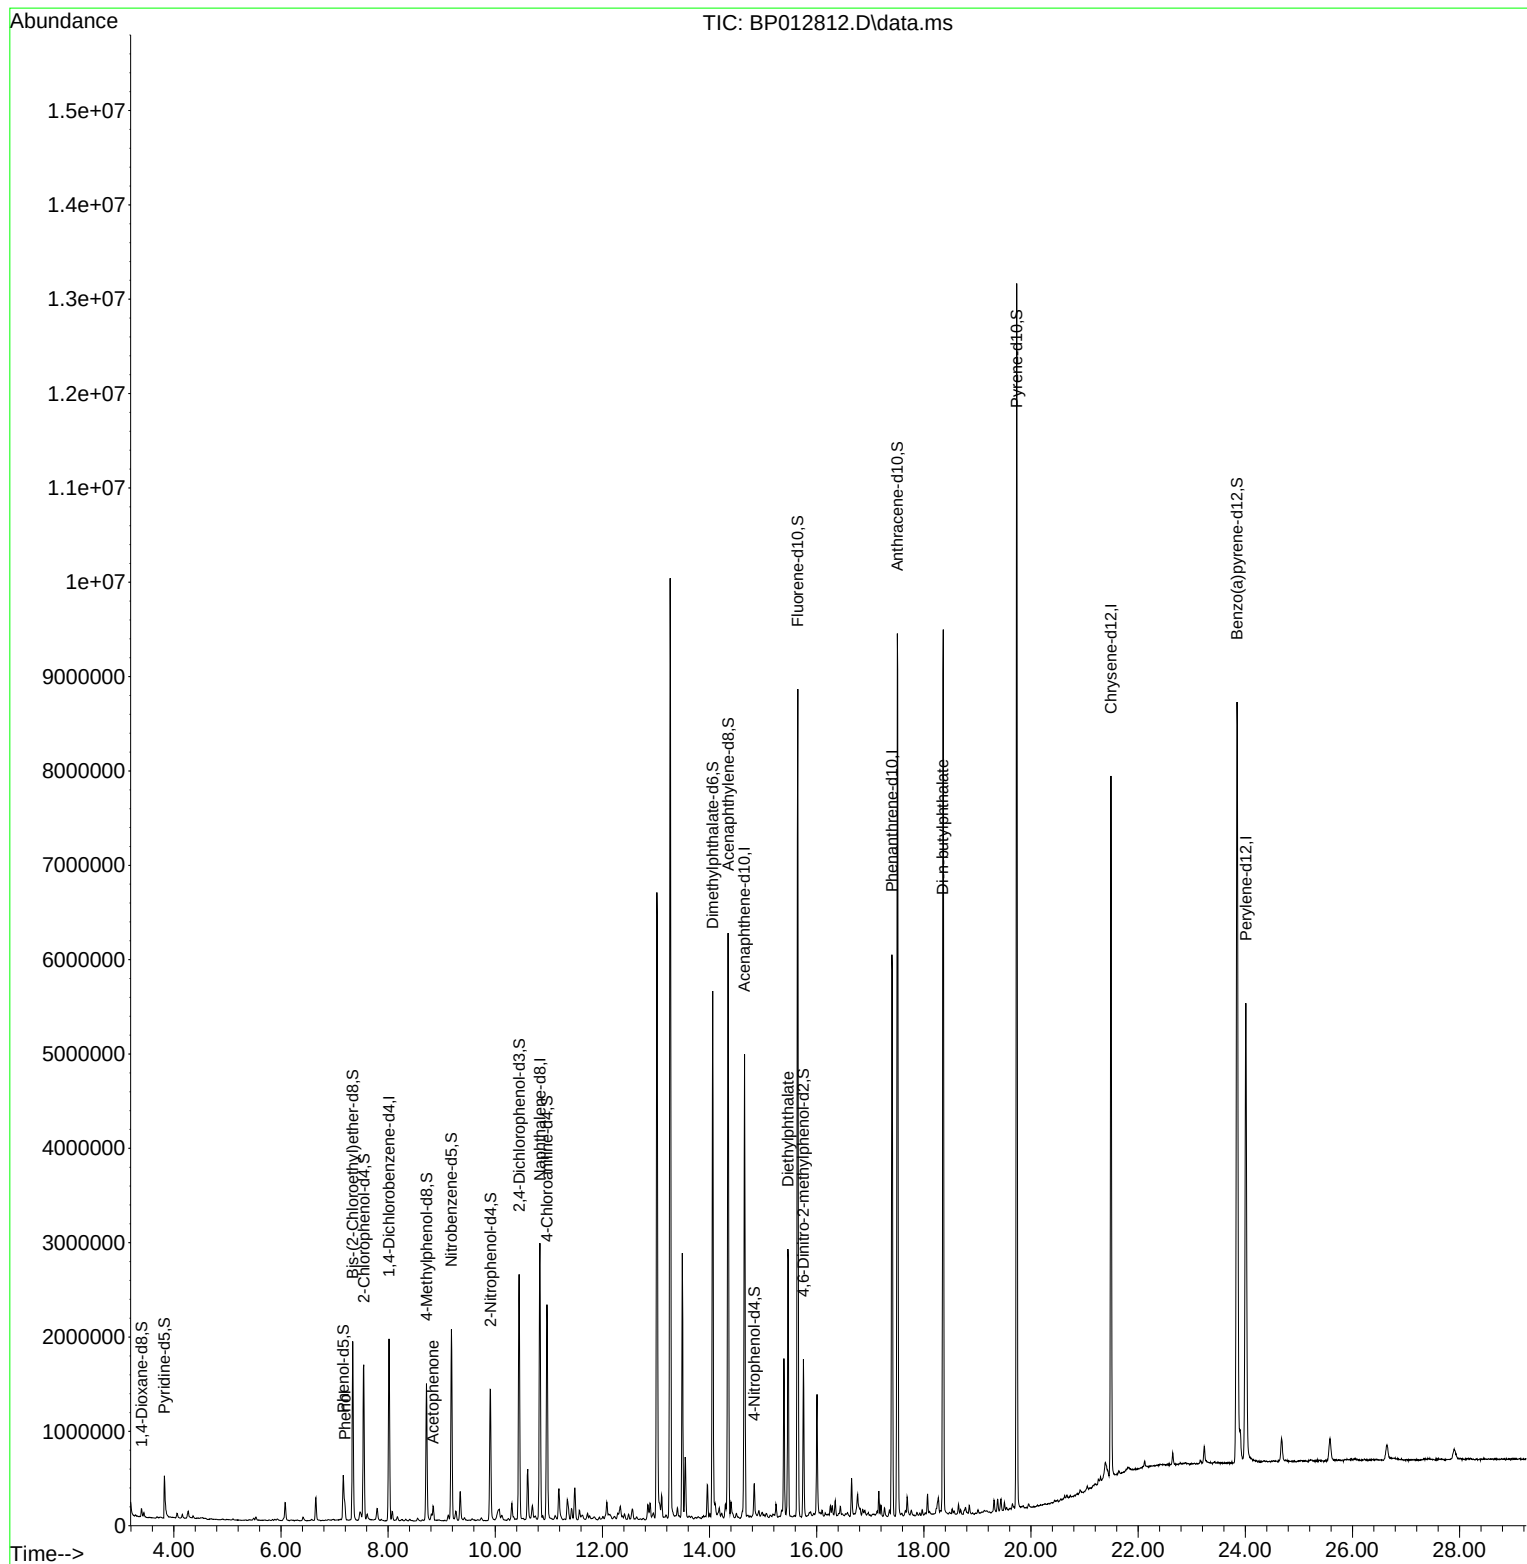


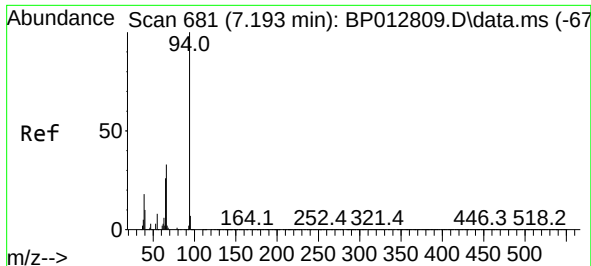

#8
Phenol
Concen: 2.135 ng/ul
RT: 7.193 min Scan# 681
Delta R.T. -0.000 min
Lab File: BP012812.D
Acq: 28 Nov 2022 12:27




Instrument :
BNA_P
ClientSampleId :
COL03


Tgt Ion: 94 Resp: 98983
Ion Ratio Lower Upper
94 100
65 26.7 20.9 31.3
66 34.2 26.0 39.0

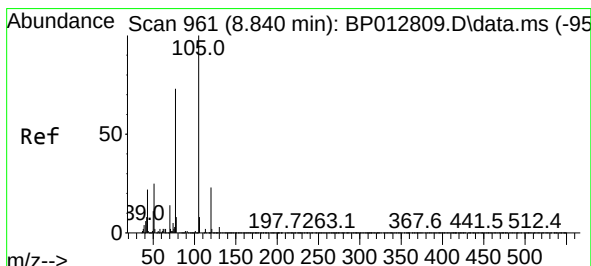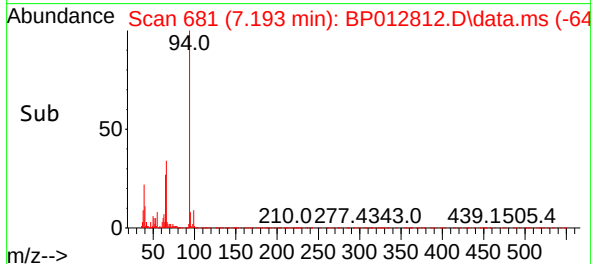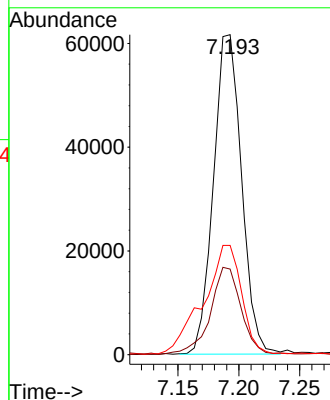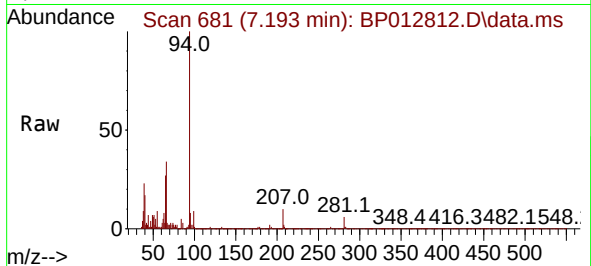

#16
Acetophenone
Concen: 1.430 ng/ul
RT: 8.840 min Scan# 961
Delta R.T. -0.006 min
Lab File: BP012812.D
Acq: 28 Nov 2022 12:27

Tgt Ion: 105 Resp: 80769
Ion Ratio Lower Upper
105 100
77 78.5 59.7 89.5
51 28.8 20.9 31.3


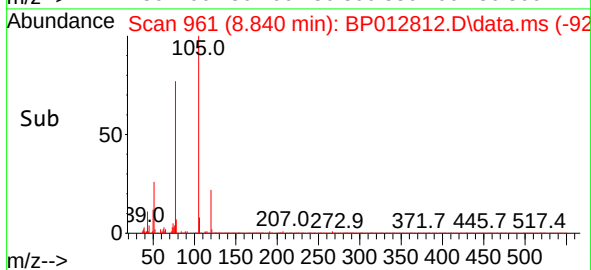
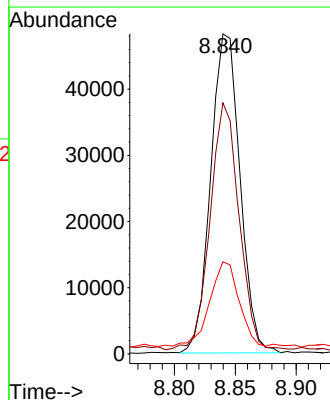
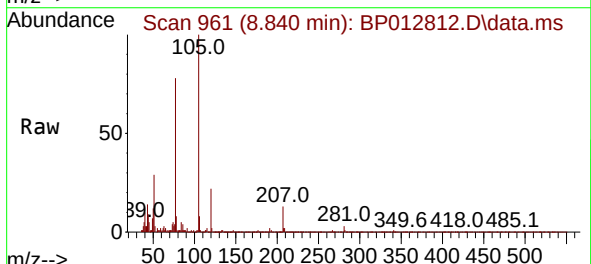


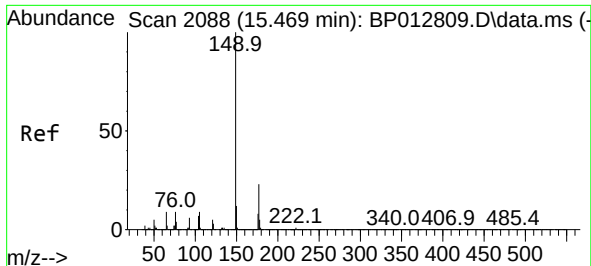

#59
Diethylphthalate
Concen: 13.657 ng/ul
RT: 15.463 min Scan# 2088
Delta R.T. -0.012 min
Lab File: BP012812.D
Acq: 28 Nov 2022 12:27

Instrument :
BNA_P
ClientSampleId :
COL03

Tgt Ion:149 Resp: 1572094
Ion Ratio Lower Upper
149 100
177 22.6 18.1 27.1
150 12.3 9.8 14.8

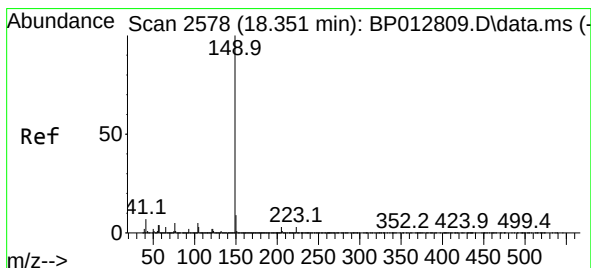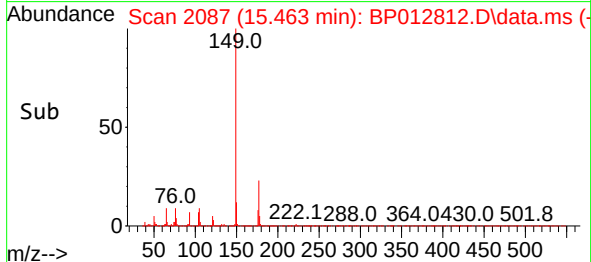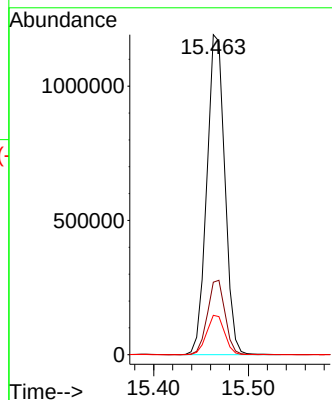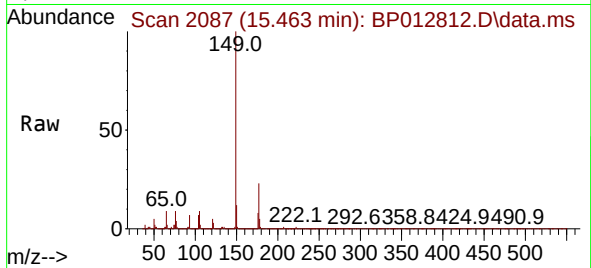

#78
Di-n-butylphthalate
Concen: 1.984 ng/ul
RT: 18.351 min Scan# 2578
Delta R.T. -0.006 min
Lab File: BP012812.D
Acq: 28 Nov 2022 12:27

Tgt Ion:149 Resp: 387386
Ion Ratio Lower Upper
149 100
150 11.3 7.2 10.8#
104 5.2 3.7 5.5

