




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012813.D
 Acq On : 28 Nov 2022 13:02
 Operator : CG/JU
 Sample : N5710-09DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KY8DL

Manual IntegrationsAPPROVED

Quant Time: Nov 28 22:38:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/29/2022
 Supervised By :mohammad ahmed 11/30/2022

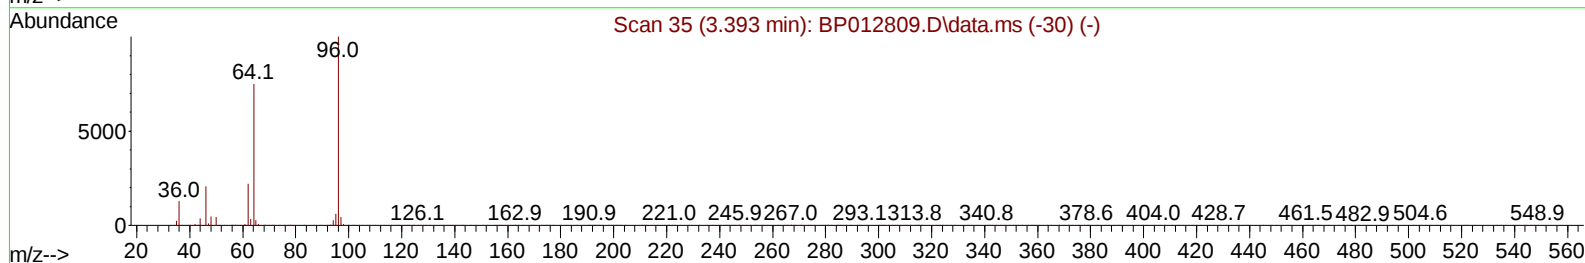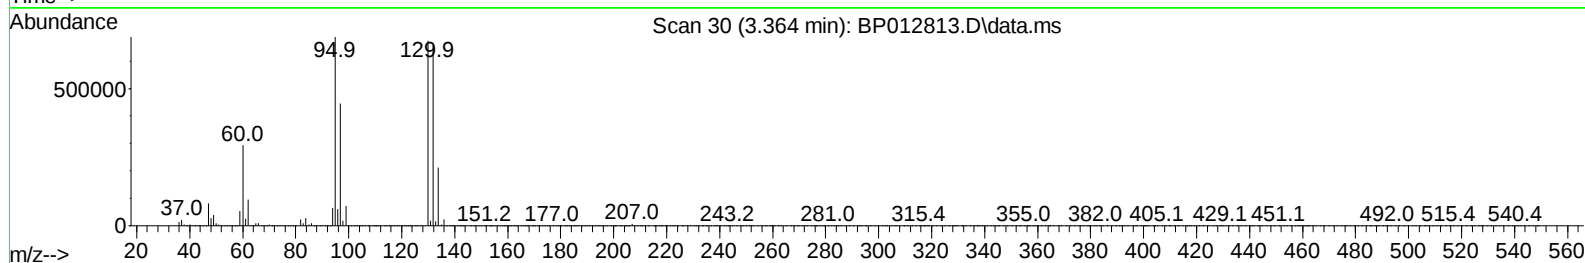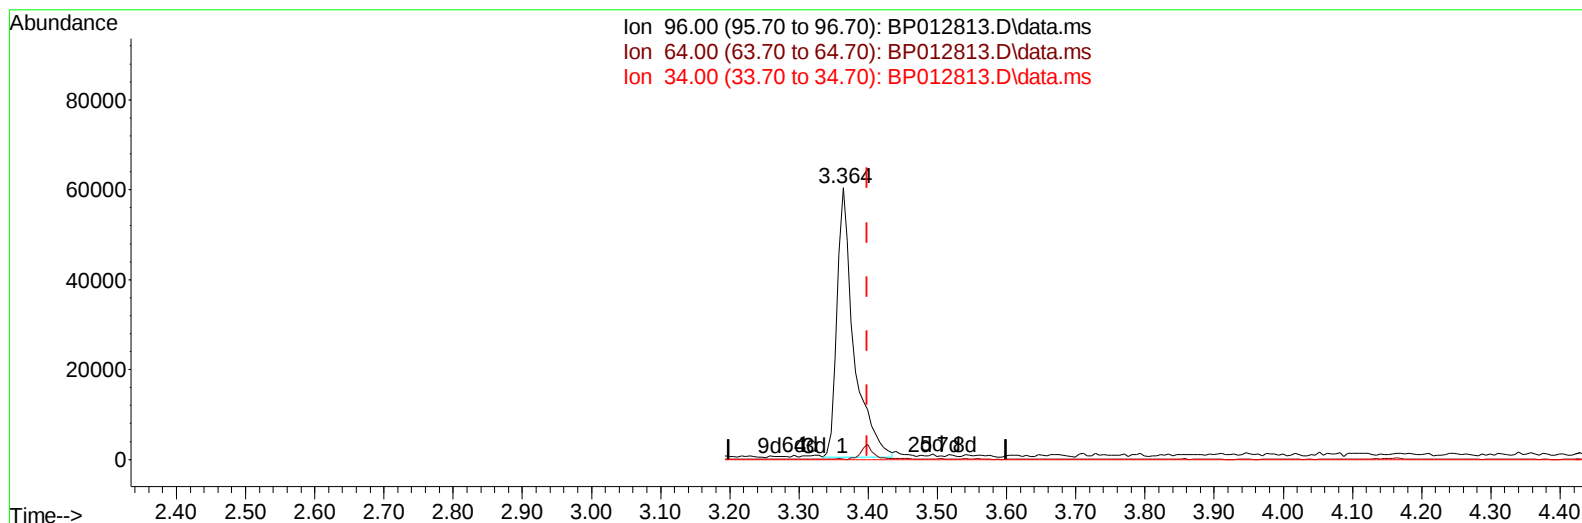

TIC: BP012813.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.364min (-0.035) 8.93 ng/uL

response 101482

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.90	0.22#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012813.D
 Acq On : 28 Nov 2022 13:02
 Operator : CG/JU
 Sample : N5710-09DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KY8DL

Manual IntegrationsAPPROVED

Quant Time: Nov 28 22:38:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/29/2022
 Supervised By :mohammad ahmed 11/30/2022

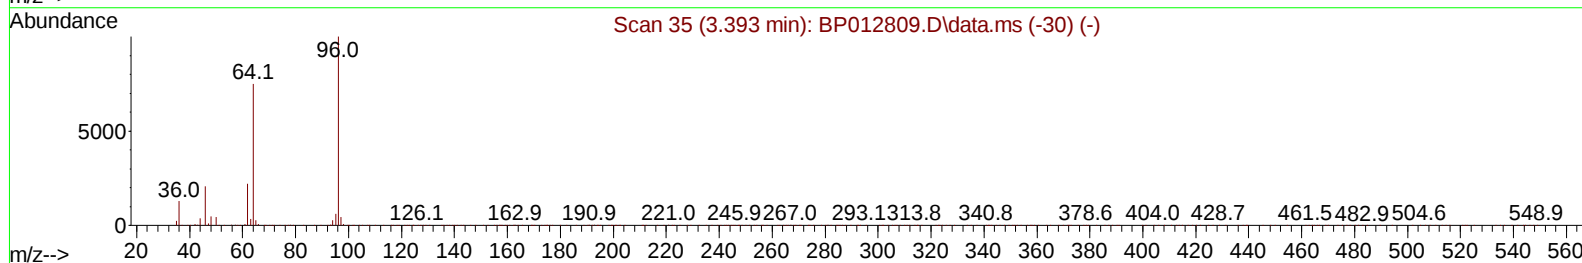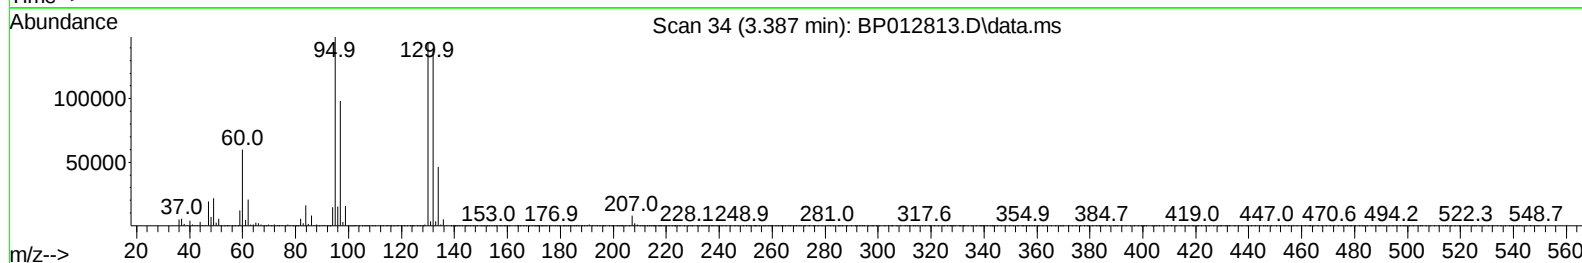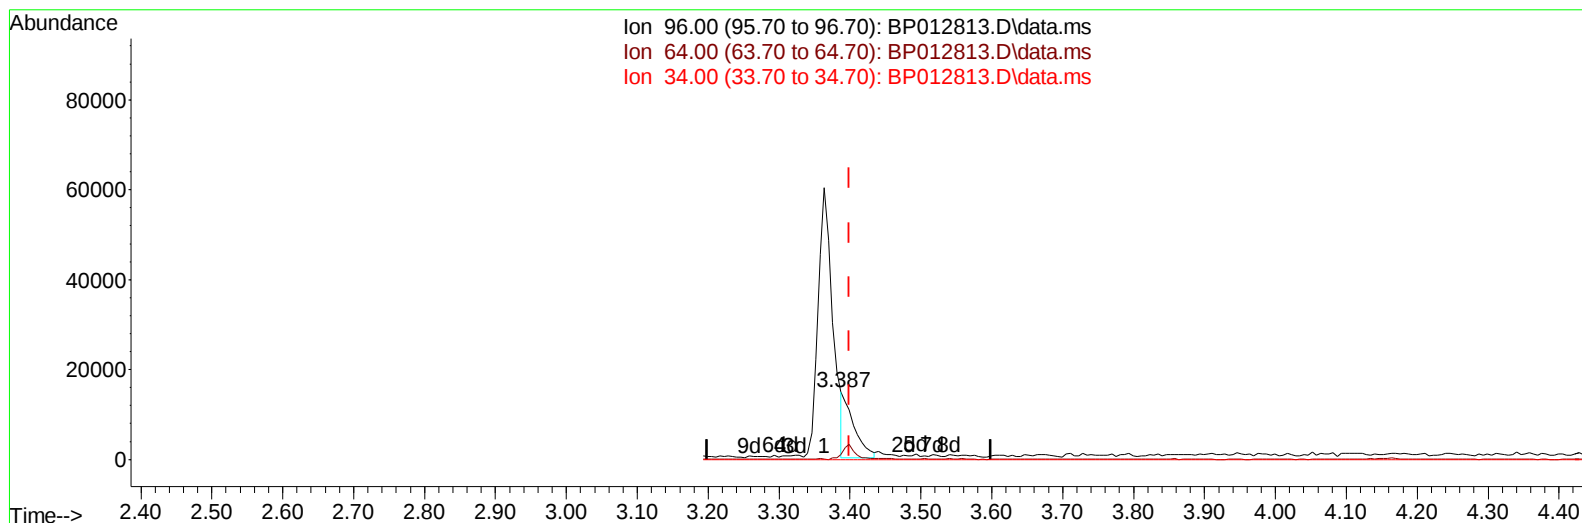

TIC: BP012813.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.387min (-0.012) 1.35 ng/uL m

response 15360

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.90	7.55#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012813.D
 Acq On : 28 Nov 2022 13:02
 Operator : CG/JU
 Sample : N5710-09DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KY8DL

Manual IntegrationsAPPROVED

Quant Time: Nov 28 22:38:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/29/2022
 Supervised By :mohammad ahmed 11/30/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	486804	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	2158495	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	1447752	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.404	188	3246596	20.000	ng/ul	0.00
79) Chrysene-d12	21.492	240	3419403	20.000	ng/ul	0.00
88) Perylene-d12	24.010	264	3360935	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	15360m	1.352	ng/uL	-0.01
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.164	99	44850	1.121	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	148036	6.006	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	134002	4.396	ng/ul	0.00
15) 4-Methylphenol-d8	8.716	113	75920	2.356	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	66234	5.013	ng/ul	0.00
24) 2-Nitrophenol-d4	9.905	143	63961	4.560	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.446	165	147258	4.499	ng/ul	0.00
31) 4-Chloroaniline-d4	10.969	131	63658	1.420	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	610712	6.128	ng/ul	0.00
49) Acenaphthylene-d8	14.346	160	505998	4.352	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.640	176	556571	6.377	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.504	188	867670	6.071	ng/ul	0.00
81) Pyrene-d10	19.733	212	1097160	5.522	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.839	264	958846	5.808	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.434	88	189561	15.537	ng/uL	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012813.D
Acq On : 28 Nov 2022 13:02
Operator : CG/JU
Sample : N5710-09DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY8DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

Quant Time: Nov 28 22:38:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

