

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012821.D
 Acq On : 28 Nov 2022 17:39
 Operator : CG/JU
 Sample : N5666-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB29

Quant Time: Nov 28 22:42:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	611784	20.000	ng/u1	0.00
20) Naphthalene-d8	10.834	136	2670969	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	1714762	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.404	188	3147943	20.000	ng/u1	0.00
79) Chrysene-d12	21.492	240	1753862	20.000	ng/u1	0.00
88) Perylene-d12	24.003	264	1879063	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	63547	4.451	ng/uL	0.00
4) Pyridine-d5	3.828	84	158312	3.705	ng/u1	0.00
7) Phenol-d5	7.163	99	322205	6.409	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	976310	31.517	ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	946904	24.719	ng/u1	0.00
15) 4-Methylphenol-d8	8.716	113	620643	15.323	ng/u1	0.00
21) Nitrobenzene-d5	9.181	128	602836	36.876	ng/u1	0.00
24) 2-Nitrophenol-d4	9.910	143	606893	34.963	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.445	165	1128990	27.875	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	1213323	21.876	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	3845602	32.582	ng/u1	0.00
49) Acenaphthylene-d8	14.345	160	4528038	32.879	ng/u1	0.00
54) 4-Nitrophenol-d4	14.827	143	61047	2.901	ng/u1	0.00
60) Fluorene-d10	15.645	176	3422016	33.105	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	310420	20.632	ng/u1	0.00
73) Anthracene-d10	17.504	188	4836282	34.901	ng/u1	0.00
81) Pyrene-d10	19.733	212	4323549	42.425	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.839	264	3179731	34.451	ng/u1	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.098	107	83077	1.955	ng/u1	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012821.D
Acq On : 28 Nov 2022 17:39
Operator : CG/JU
Sample : N5666-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB29

Quant Time: Nov 28 22:42:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

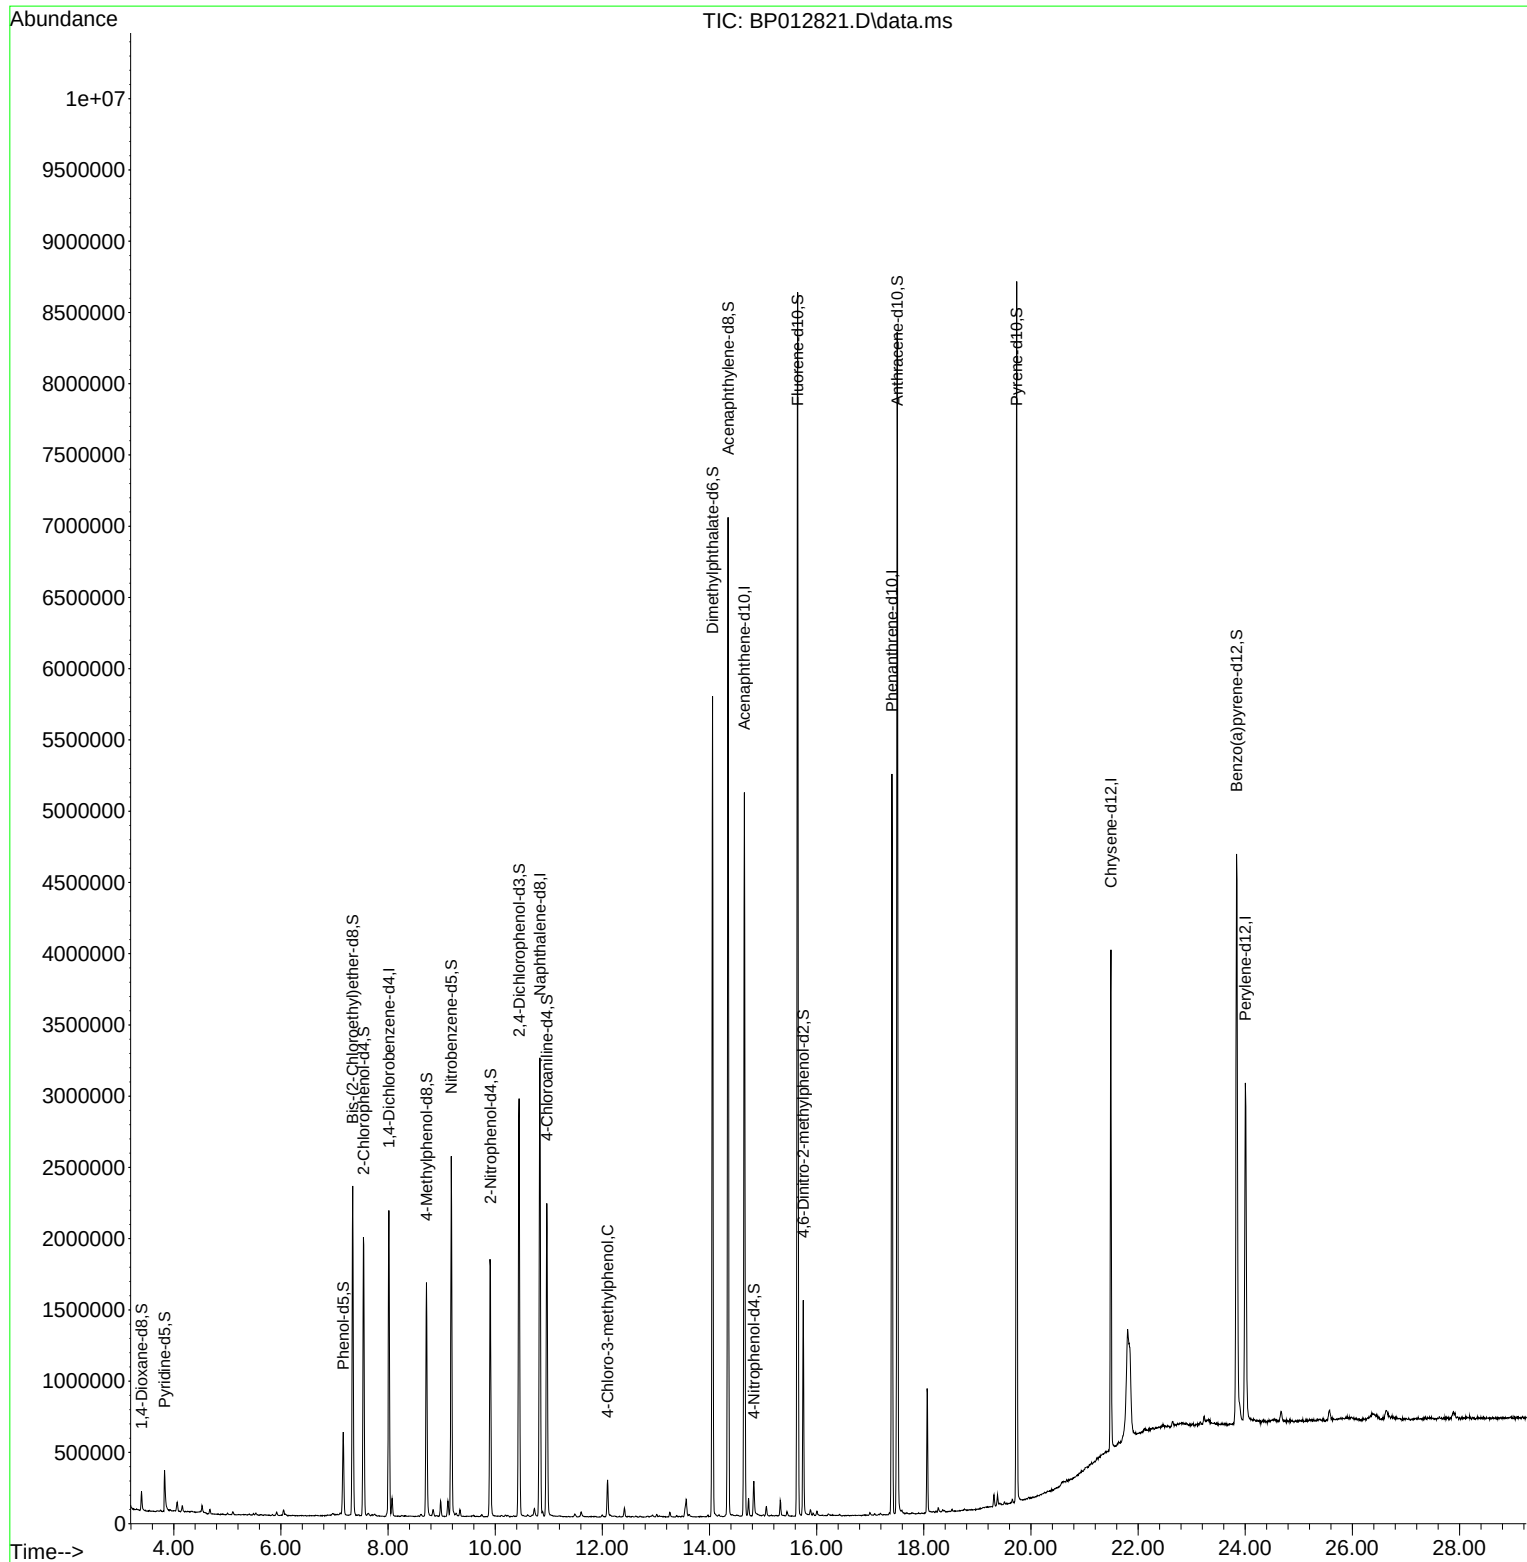

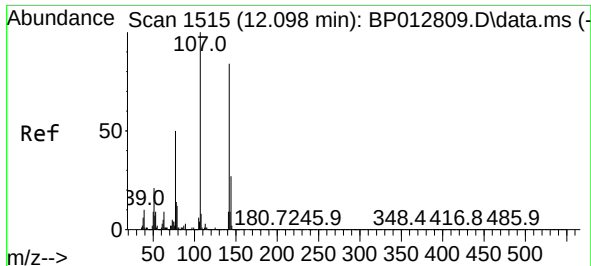

#35
 4-Chloro-3-methylphenol
 Concen: 1.955 ng/ul
 RT: 12.098 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BP012821.D
 Acq: 28 Nov 2022 17:39

Instrument :
 BNA_P
 ClientSampleId :
 BHB29

Tgt Ion:107 Resp: 83077
 Ion Ratio Lower Upper
 107 100
 144 26.8 21.4 32.2
 142 86.6 66.6 100.0

