

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012823.D
 Acq On : 28 Nov 2022 18:47
 Operator : CG/JU
 Sample : N5666-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB36

Quant Time: Nov 28 22:42:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	570491	20.000	ng/u1	0.00
20) Naphthalene-d8	10.834	136	2572815	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	1734845	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.404	188	3592341	20.000	ng/u1	0.00
79) Chrysene-d12	21.492	240	2481728	20.000	ng/u1	0.00
88) Perylene-d12	24.004	264	1994173	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	54159	4.068	ng/uL	0.00
4) Pyridine-d5	3.823	84	277105	6.955	ng/u1	0.00
7) Phenol-d5	7.164	99	672372	14.343	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	1092359	37.816	ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	1118931	31.324	ng/u1	0.00
15) 4-Methylphenol-d8	8.716	113	898872	23.798	ng/u1	0.00
21) Nitrobenzene-d5	9.181	128	687502	43.659	ng/u1	0.00
24) 2-Nitrophenol-d4	9.905	143	561332	33.572	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.446	165	1326265	33.995	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	1802358	33.737	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	5129716	42.958	ng/u1	0.00
49) Acenaphthylene-d8	14.346	160	5698287	40.898	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	126935	5.962	ng/u1	0.00
60) Fluorene-d10	15.645	176	4483855	42.876	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	68863	4.011	ng/u1	0.00
73) Anthracene-d10	17.504	188	7339197	46.412	ng/u1	0.00
81) Pyrene-d10	19.733	212	7609605	52.770	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.845	264	4807686	49.082	ng/u1	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.099	107	79760	1.949	ng/u1	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012823.D
Acq On : 28 Nov 2022 18:47
Operator : CG/JU
Sample : N5666-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB36

Quant Time: Nov 28 22:42:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

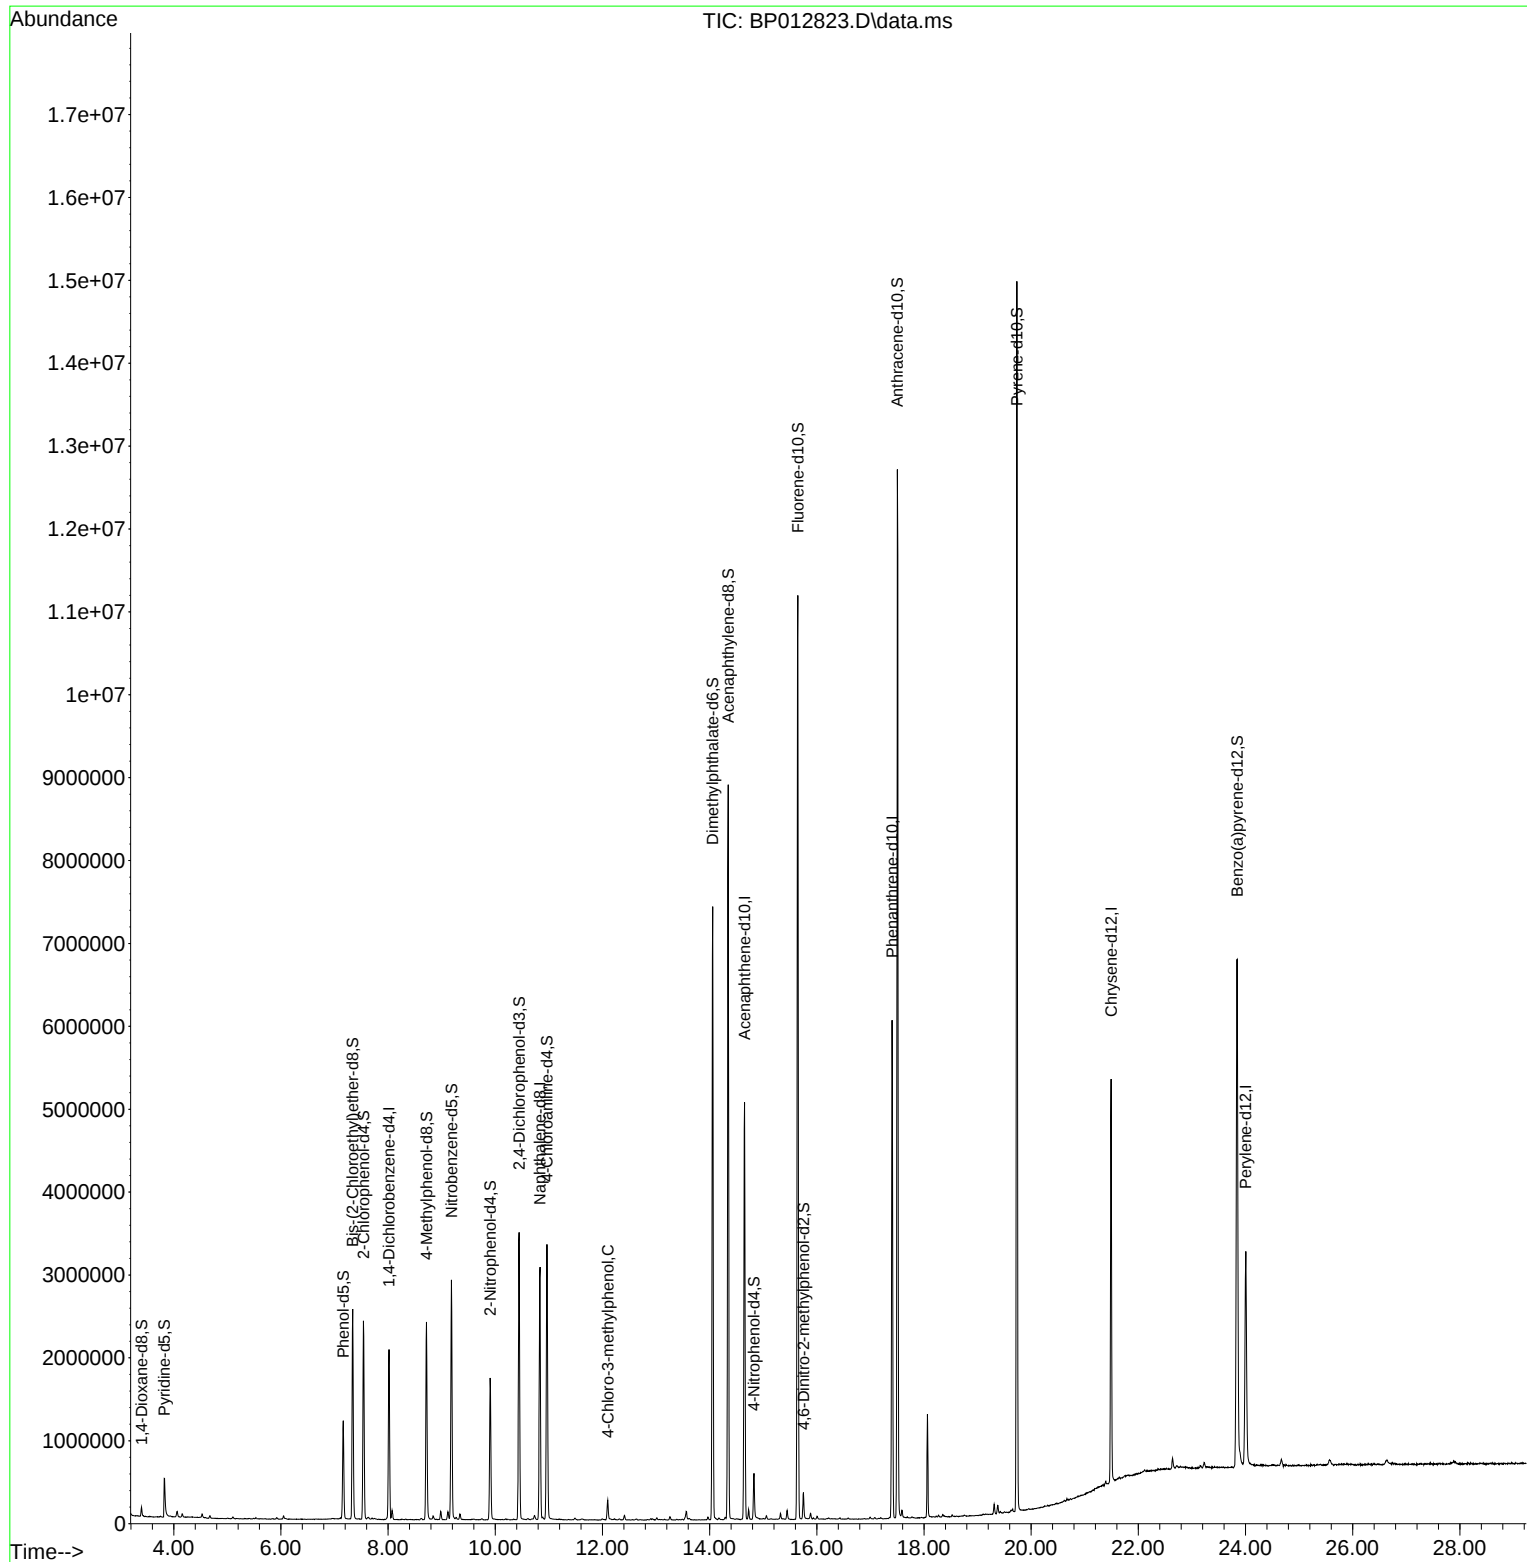

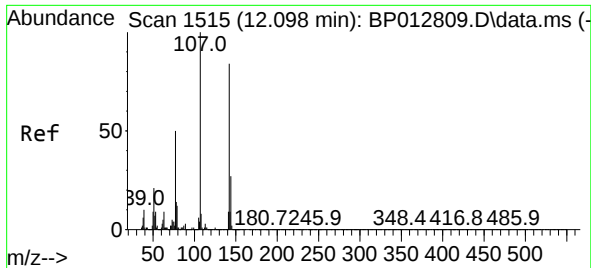

#35
 4-Chloro-3-methylphenol
 Concen: 1.949 ng/ul
 RT: 12.099 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BP012823.D
 Acq: 28 Nov 2022 18:47

Instrument :
 BNA_P
 ClientSampleId :
 BHB36

Tgt Ion:107 Resp: 79760
 Ion Ratio Lower Upper
 107 100
 144 24.9 21.4 32.2
 142 82.6 66.6 100.0

