

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012825.D
 Acq On : 28 Nov 2022 19:56
 Operator : CG/JU
 Sample : PB149200BS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS200

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/29/2022
 Supervised By :mohammad ahmed 11/30/2022

Quant Time: Nov 28 22:43:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	639035	20.000	ng/u1	0.00
20) Naphthalene-d8	10.834	136	2917885	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	1929126	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.404	188	3978805	20.000	ng/u1	0.00
79) Chrysene-d12	21.492	240	3069346	20.000	ng/u1	0.00
88) Perylene-d12	24.004	264	2237298	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	81050	5.435	ng/uL	0.00
4) Pyridine-d5	3.822	84	1108572	24.840	ng/u1	0.00
7) Phenol-d5	7.163	99	1538792	29.304	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	932559	28.821	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	1194754	29.859	ng/u1	0.00
15) 4-Methylphenol-d8	8.722	113	1241046	29.333	ng/u1	0.00
21) Nitrobenzene-d5	9.181	128	579965	32.474	ng/u1	0.00
24) 2-Nitrophenol-d4	9.910	143	646453	34.090	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.445	165	1290151	29.159	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	1605377	26.496	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	3831527	28.855	ng/u1	0.00
49) Acenaphthylene-d8	14.345	160	4452107	28.736	ng/u1	0.00
54) 4-Nitrophenol-d4	14.839	143	690036	29.148	ng/u1	0.00
60) Fluorene-d10	15.645	176	3366968	28.953	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	604570	31.792	ng/u1	0.00
73) Anthracene-d10	17.504	188	5085749	29.038	ng/u1	0.00
81) Pyrene-d10	19.733	212	5473973	30.693	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.845	264	3337730	30.372	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.434	88	162350	10.137	ng/uL	98
5) Pyridine	3.840	79	1124363	25.748	ng/u1	99
6) Benzaldehyde	7.151	77	835323	32.580	ng/u1	97
8) Phenol	7.193	94	1560275	28.337	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.434	93	1244859	27.594	ng/u1	100
12) 2-Chlorophenol	7.575	128	1234489	28.363	ng/u1	100
13) 2-Methylphenol	8.451	108	1192946	27.876	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.546	45	1758309	27.021	ng/u1	99
16) Acetophenone	8.846	105	1912699	28.523	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.834	70	942960	28.546	ng/u1	97
18) 4-Methylphenol	8.787	108	1322800	28.067	ng/u1	97
19) Hexachloroethane	9.104	117	466121	27.926	ng/u1	98
22) Nitrobenzene	9.228	77	1359153	29.017	ng/u1	99
23) Isophorone	9.757	82	2767474	26.801	ng/u1	98
25) 2-Nitrophenol	9.940	139	714336	31.383	ng/u1	96
26) 2,4-Dimethylphenol	9.992	107	1304334	25.788	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.234	93	1720844	27.182	ng/u1	99
29) 2,4-Dichlorophenol	10.475	162	1276067	27.840	ng/u1	99
30) Naphthalene	10.887	128	4097300	26.816	ng/u1	100
32) 4-Chloroaniline	10.987	127	1583277	25.444	ng/u1	99
33) Hexachlorobutadiene	11.169	225	818549	26.812	ng/u1	99
34) Caprolactam	11.769	113	397250m	28.224	ng/u1	
35) 4-Chloro-3-methylphenol	12.104	107	1320491	28.450	ng/u1	97
36) 2-Methylnaphthalene	12.486	142	2872249	27.299	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012825.D
 Acq On : 28 Nov 2022 19:56
 Operator : CG/JU
 Sample : PB149200BS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS200


Quant Time: Nov 28 22:43:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 11/29/2022
 Supervised By :mohammad ahmed 11/30/2022


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.704	142	2867893	27.197	ng/u1	99
39) 1,2,4,5-Tetrachloroben...	12.845	216	1648042	26.790	ng/u1	99
40) Hexachlorocyclopentadiene	12.828	237	778550	26.266	ng/u1	99
41) 2,4,6-Trichlorophenol	13.081	196	1083534	28.150	ng/u1	99
42) 2,4,5-Trichlorophenol	13.151	196	1188093	28.713	ng/u1	98
43) 1,1'-Biphenyl	13.486	154	3825516	27.222	ng/u1	100
44) 2-Chloronaphthalene	13.528	162	3025283	26.909	ng/u1	100
45) 2-Nitroaniline	13.728	65	769328	34.975	ng/u1	96
47) Dimethylphthalate	14.104	163	3846050	27.631	ng/u1	99
48) 2,6-Dinitrotoluene	14.222	165	740735	34.005	ng/u1	99
50) Acenaphthylene	14.375	152	4668268	27.555	ng/u1	100
51) 3-Nitroaniline	14.551	138	725644	28.763	ng/u1	98
52) Acenaphthene	14.716	153	3239532	27.161	ng/u1	98
53) 2,4-Dinitrophenol	14.751	184	396531	28.328	ng/u1	98
55) 4-Nitrophenol	14.851	109	469753	27.312	ng/u1	96
56) Dibenzofuran	15.051	168	4521623	27.504	ng/u1	100
57) 2,4-Dinitrotoluene	15.010	165	1062033	33.038	ng/u1	97
58) 2,3,4,6-Tetrachlorophenol	15.275	232	1029755	28.874	ng/u1	97
59) Diethylphthalate	15.469	149	3735705	27.726	ng/u1	99
61) Fluorene	15.704	166	3651973	27.700	ng/u1	100
62) 4-Chlorophenyl-phenyle...	15.692	204	1898697	27.757	ng/u1	99
63) 4-Nitroaniline	15.716	138	709908	33.016	ng/u1	99
66) 4,6-Dinitro-2-methylph...	15.769	198	621549	30.450	ng/u1	98
67) N-Nitrosodiphenylamine	15.904	169	3182904	28.148	ng/u1	99
68) 4-Bromophenyl-phenylether	16.592	248	1155071	29.496	ng/u1	99
69) Hexachlorobenzene	16.704	284	1404312	28.136	ng/u1	100
70) Atrazine	16.863	200	1083060	27.916	ng/u1	100
71) Pentachlorophenol	17.051	266	835166	27.248	ng/u1	99
72) Phenanthrene	17.451	178	5830127	27.493	ng/u1	99
74) Anthracene	17.545	178	5803530	27.664	ng/u1	100
75) 1,2,3,4-Tetrachloroben...	13.451	216	1651838	26.854	ng/uL	99
76) Pentachlorobenzene	14.969	250	1612537	25.219	ng/uL	99
77) Carbazole	17.804	167	5171960	29.142	ng/u1	100
78) Di-n-butylphthalate	18.351	149	6037223	28.736	ng/u1	99
80) Fluoranthene	19.410	202	6496200	29.284	ng/u1	98
82) Pyrene	19.763	202	6599735	28.765	ng/u1	98
83) Butylbenzylphthalate	20.627	149	2061563	38.397	ng/u1	96
84) 3,3'-Dichlorobenzidine	21.404	252	1554173	27.573	ng/u1	99
85) Benzo(a)anthracene	21.474	228	5537427	26.084	ng/u1	100
86) Bis(2-ethylhexyl)phtha...	21.392	149	2737281	33.337	ng/u1	100
87) Chrysene	21.533	228	5196093	25.315	ng/u1	100
89) Di-n-octyl phthalate	22.357	149	3702419	28.979	ng/u1	100
90) Benzo(b)fluoranthene	23.233	252	4521273	27.290	ng/u1	99
91) Benzo(k)fluoranthene	23.286	252	4251702	25.710	ng/u1	99
93) Benzo(a)pyrene	23.892	252	3704528	27.192	ng/u1	100
94) Indeno(1,2,3-cd)pyrene	26.645	276	4069937	30.965	ng/u1	99
95) Dibenzo(a,h)anthracene	26.662	278	3588696	30.090	ng/u1	98
96) Benzo(g,h,i)perylene	27.445	276	3586532	31.724	ng/u1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

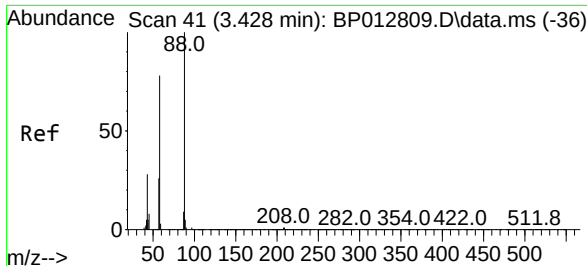

#2
1,4-Dioxane
Concen: 10.137 ng/uL
RT: 3.434 min Scan# 41
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200

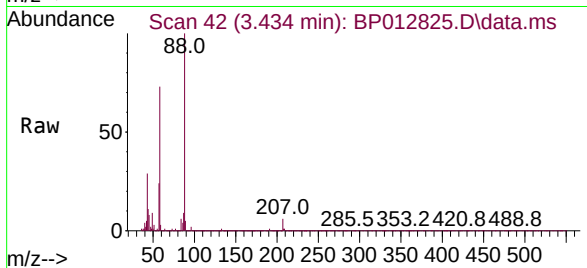


Tgt Ion: 88 Resp: 162350
Ion Ratio Lower Upper
88 100
43 28.9 22.6 34.0
58 72.6 59.6 89.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

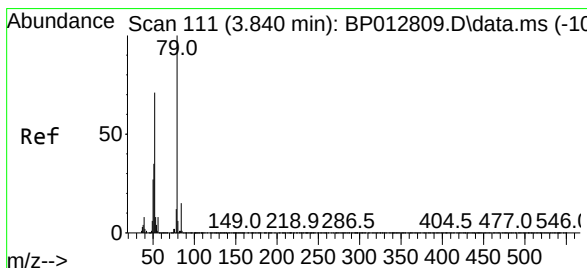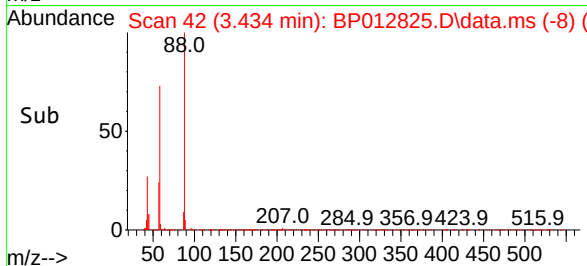


#5
Pyridine
Concen: 25.748 ng/uL
RT: 3.840 min Scan# 111
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56

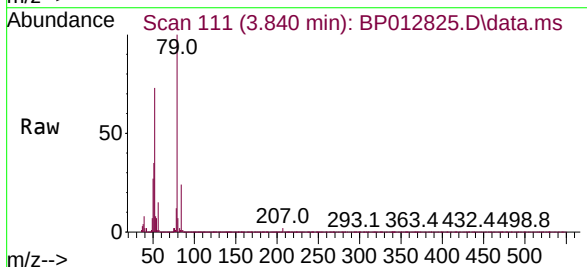


Tgt Ion: 79 Resp: 1124363
Ion Ratio Lower Upper
79 100
52 73.4 58.9 88.3
51 34.7 27.3 40.9

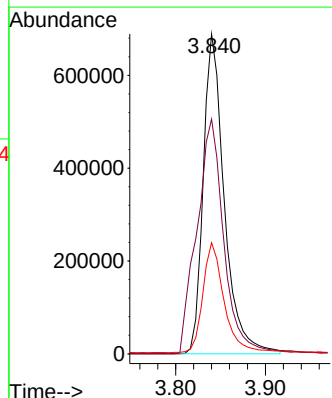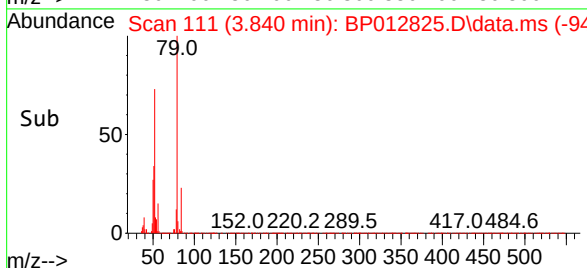



#6
Benzaldehyde
Concen: 32.580 ng/ul
RT: 7.151 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200



Tgt Ion: 77 Resp: 835323
Ion Ratio Lower Upper
77 100
105 103.5 81.4 122.2
106 100.7 77.4 116.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

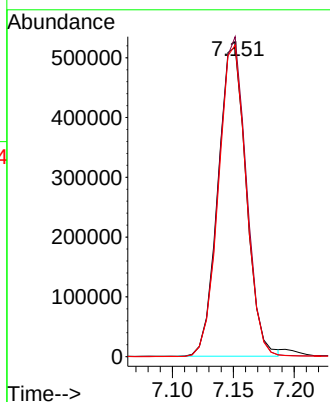

#8
Phenol
Concen: 28.337 ng/ul
RT: 7.193 min Scan# 681
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion: 94 Resp: 1560275
Ion Ratio Lower Upper
94 100
65 26.5 20.9 31.3
66 33.1 26.0 39.0





#10
Bis(2-Chloroethyl)ether
Concen: 27.594 ng/ul
RT: 7.434 min Scan# 722
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200



Tgt Ion: 93 Resp: 1244859
Ion Ratio Lower Upper
93 100
63 74.7 59.7 89.5
95 32.7 25.8 38.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022



#12
2-Chlorophenol
Concen: 28.363 ng/ul
RT: 7.575 min Scan# 746
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56

Tgt Ion:128 Resp: 1234489
Ion Ratio Lower Upper
128 100
64 44.8 35.6 53.4
130 32.5 26.0 39.0





#13

2-Methylphenol

Concen: 27.876 ng/ul

RT: 8.451 min Scan# 895

Delta R.T. -0.006 min

Lab File: BP012825.D

Acq: 28 Nov 2022 19:56

Instrument :

BNA_P

ClientSampleId :

SLCS200

Tgt Ion:108 Resp: 1192946

Ion Ratio Lower Upper





108 100

107 88.4 69.3 103.9

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

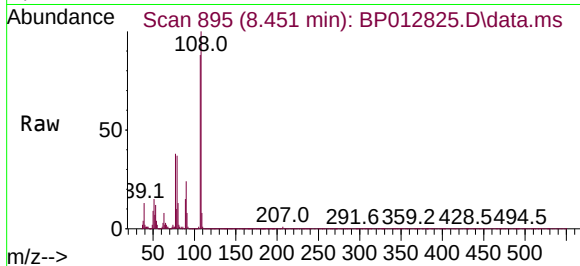

#14

2,2'-oxybis(1-Chloropropane)

Concen: 27.021 ng/ul

RT: 8.546 min Scan# 911

Delta R.T. -0.000 min

Lab File: BP012825.D

Acq: 28 Nov 2022 19:56




Tgt Ion: 45 Resp: 1758309


Ion Ratio Lower Upper

45 100

77 13.6 11.3 16.9

79 10.5 8.6 12.8

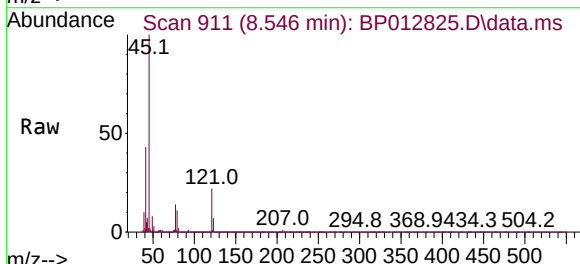







#16
Acetophenone
Concen: 28.523 ng/ul
RT: 8.846 min Scan# 90
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56

Instrument :
BNA_P
ClientSampleId :
SLCS200

Tgt Ion:105 Resp: 1912699
Ion Ratio Lower Upper
105 100
77 73.4 59.7 89.5
51 25.0 20.9 31.3




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022



#17
N-Nitroso-di-n-propylamine
Concen: 28.546 ng/ul
RT: 8.834 min Scan# 960
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion: 70 Resp: 942960
Ion Ratio Lower Upper
70 100
42 56.3 46.1 69.1
101 9.9 7.4 11.2
130 22.1 15.8 23.6

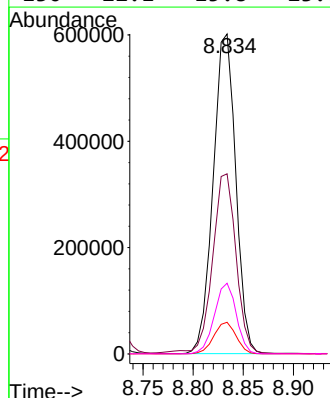



#18
4-Methylphenol
Concen: 28.067 ng/ul
RT: 8.787 min Scan# 91
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200



Tgt Ion:108 Resp: 1322800
Ion Ratio Lower Upper
108 100
107 109.2 90.2 135.2




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022



#19
Hexachloroethane
Concen: 27.926 ng/ul
RT: 9.104 min Scan# 1006
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion:117 Resp: 466121
Ion Ratio Lower Upper
117 100
201 108.8 85.7 128.5
199 67.3 52.9 79.3





#22
Nitrobenzene
Concen: 29.017 ng/ul
RT: 9.228 min Scan# 1026
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200




Tgt Ion: 77 Resp: 135915
Ion Ratio Lower Upper
77 100
123 48.5 38.2 57.2
65 13.0 10.2 15.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022




#23
Isophorone
Concen: 26.801 ng/ul
RT: 9.757 min Scan# 1117
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56



Tgt Ion: 82 Resp: 2767474
Ion Ratio Lower Upper
82 100
95 6.4 5.2 7.8
138 19.0 14.5 21.7

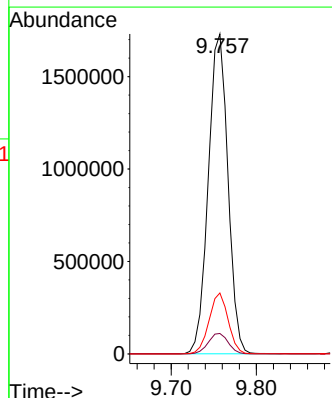







#25
2-Nitrophenol
Concen: 31.383 ng/ul
RT: 9.940 min Scan# 1148
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56

Instrument :
BNA_P
ClientSampleId :
SLCS200

Tgt Ion:139 Resp: 714336
Ion Ratio Lower Upper
139 100
65 45.7 39.5 59.3
109 25.8 21.4 32.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022



#26
2,4-Dimethylphenol
Concen: 25.788 ng/ul
RT: 9.992 min Scan# 1157
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion:107 Resp: 1304334
Ion Ratio Lower Upper
107 100
121 51.9 41.8 62.6
122 89.7 72.3 108.5





#27
Bis(2-Chloroethoxy)methane
Concen: 27.182 ng/ul
RT: 10.234 min Scan# 1198
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200

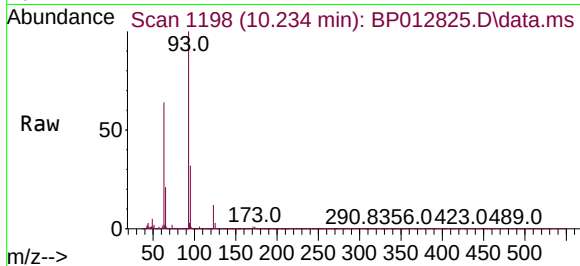

Tgt Ion: 93 Resp: 1720844
Ion Ratio Lower Upper
93 100
95 32.5 26.1 39.1
123 11.8 9.0 13.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022



#29
2,4-Dichlorophenol
Concen: 27.840 ng/ul
RT: 10.475 min Scan# 1239
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion:162 Resp: 1276067
Ion Ratio Lower Upper
162 100
164 65.7 52.9 79.3
98 32.9 26.6 40.0

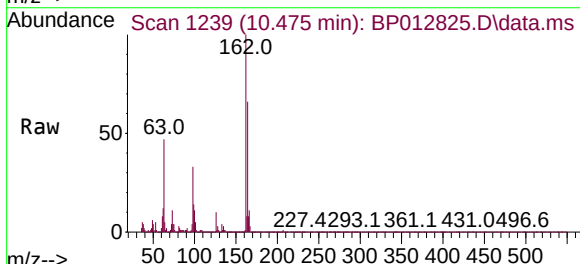



#30
Naphthalene
Concen: 26.816 ng/ul
RT: 10.887 min Scan# 1308
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200



Tgt Ion:128 Resp: 4097300
Ion Ratio Lower Upper
128 100
129 10.8 8.7 13.1
127 12.8 10.4 15.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

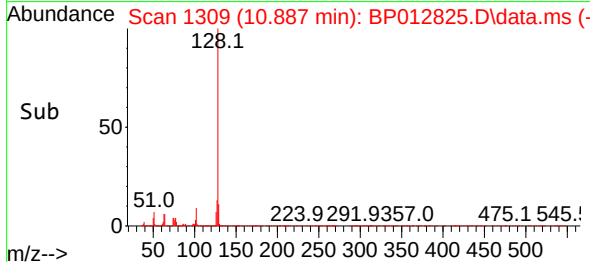

#32
4-Chloroaniline
Concen: 25.444 ng/ul
RT: 10.987 min Scan# 1326
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion:127 Resp: 1583277
Ion Ratio Lower Upper
127 100
129 32.8 25.7 38.5

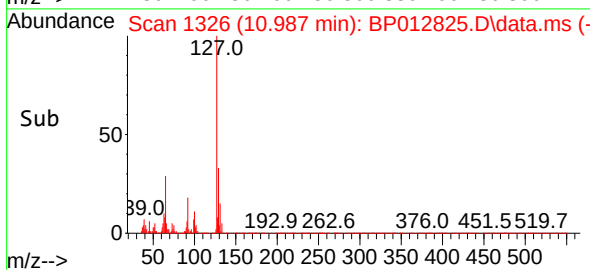



#33
Hexachlorobutadiene
Concen: 26.812 ng/ul
RT: 11.169 min Scan# 1357
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200

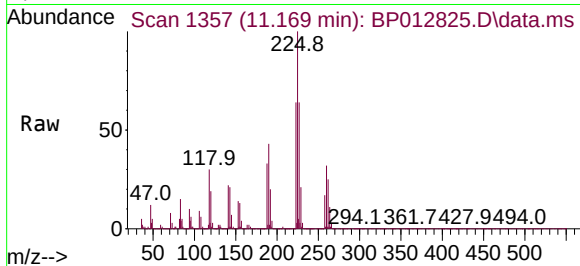


Tgt Ion:225 Resp: 818549
Ion Ratio Lower Upper
225 100
223 64.0 49.6 74.4
227 64.1 51.0 76.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022




#34
Caprolactam
Concen: 28.224 ng/ul m
RT: 11.769 min Scan# 1459
Delta R.T. 0.011 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56

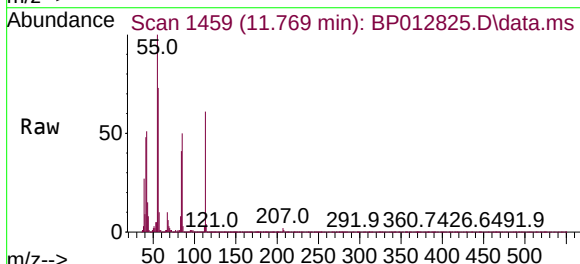


Tgt Ion:113 Resp: 397250
Ion Ratio Lower Upper
113 100
55 165.2 145.9 218.9
56 121.4 107.1 160.7

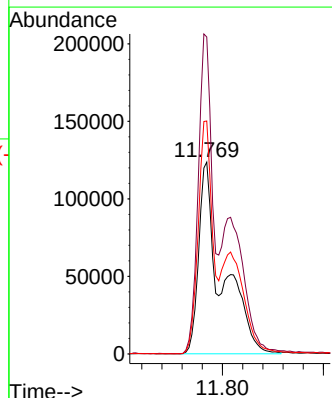



#35
4-Chloro-3-methylphenol
Concen: 28.450 ng/ul
RT: 12.104 min Scan# 1516
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200

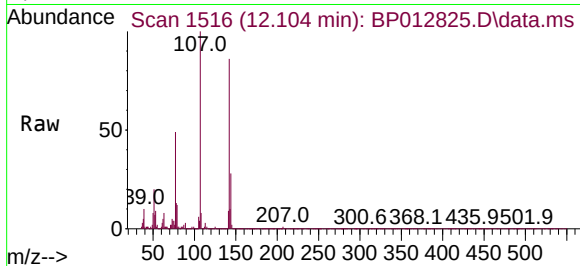

Tgt Ion:107 Resp: 1320491
Ion Ratio Lower Upper
107 100
144 28.4 21.4 32.2
142 85.9 66.6 100.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022



#36
2-Methylnaphthalene
Concen: 27.299 ng/ul
RT: 12.486 min Scan# 1581
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion:142 Resp: 2872249
Ion Ratio Lower Upper
142 100
141 89.0 70.2 105.2

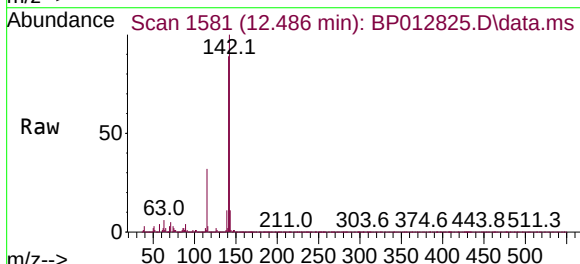



#37
1-Methylnaphthalene
Concen: 27.197 ng/ul
RT: 12.704 min Scan# 1618
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200




Tgt Ion:142 Resp: 2867893
Ion Ratio Lower Upper
142 100
141 92.2 73.3 109.9
116 3.6 2.9 4.3

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022




#39
1,2,4,5-Tetrachlorobenzene
Concen: 26.790 ng/ul
RT: 12.845 min Scan# 1642
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Tgt Ion:216 Resp: 1648042
Ion Ratio Lower Upper
216 100
214 78.6 63.0 94.6
179 19.8 16.2 24.4
108 15.3 12.7 19.1

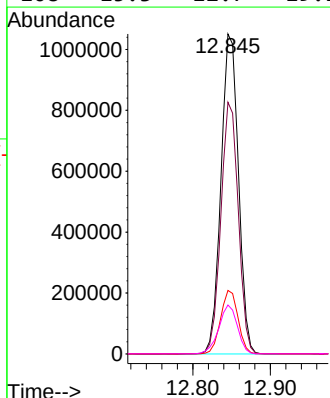



#40
Hexachlorocyclopentadiene
Concen: 26.266 ng/ul
RT: 12.828 min Scan# 1639
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200



Tgt Ion:237 Resp: 778550
Ion Ratio Lower Upper
237 100
235 62.2 50.2 75.4
272 12.7 10.2 15.2




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

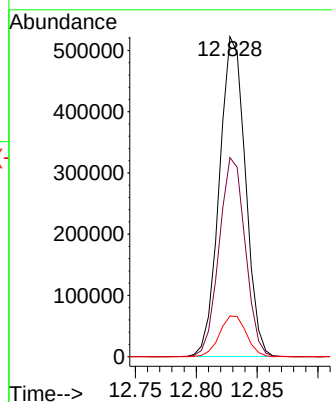

#41
2,4,6-Trichlorophenol
Concen: 28.150 ng/ul
RT: 13.081 min Scan# 1682
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion:196 Resp: 1083534
Ion Ratio Lower Upper
196 100
198 94.7 76.5 114.7
200 30.5 25.3 37.9

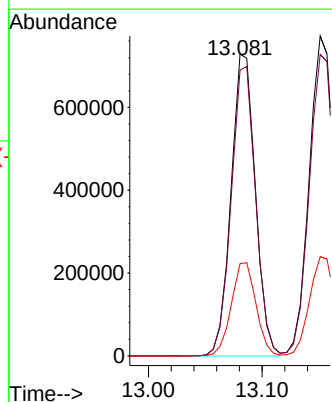



#42
2,4,5-Trichlorophenol
Concen: 28.713 ng/ul
RT: 13.151 min Scan# 1694
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200



Tgt Ion:196 Resp: 1188093
Ion Ratio Lower Upper
196 100
198 94.2 77.6 116.4
200 31.0 24.2 36.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

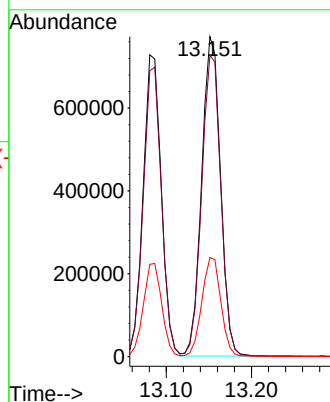

#43
1,1'-Biphenyl
Concen: 27.222 ng/ul
RT: 13.486 min Scan# 1751
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion:154 Resp: 3825516
Ion Ratio Lower Upper
154 100
153 40.0 32.0 48.0
76 12.6 10.2 15.4

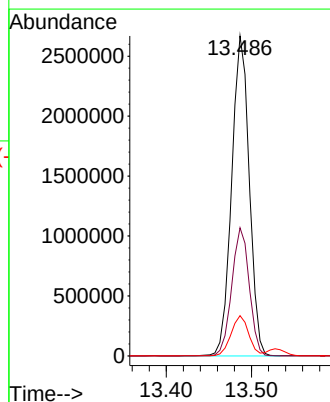



#44
2-Chloronaphthalene
Concen: 26.909 ng/ul
RT: 13.528 min Scan# 1758
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200




Tgt Ion:162 Resp: 3025283
Ion Ratio Lower Upper
162 100
164 33.1 26.5 39.7
127 36.3 28.8 43.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

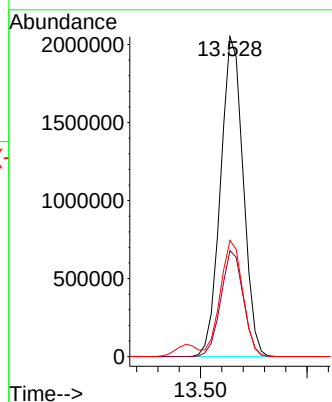


#45
2-Nitroaniline
Concen: 34.975 ng/ul
RT: 13.728 min Scan# 1792
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Tgt Ion: 65 Resp: 769328
Ion Ratio Lower Upper
65 100
92 71.1 57.8 86.8
138 112.7 94.6 142.0





#47
Dimethylphthalate
Concen: 27.631 ng/ul
RT: 14.104 min Scan# 1856
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200




Tgt Ion:163 Resp: 3846050
Ion Ratio Lower Upper
163 100
194 4.1 3.4 5.0
164 10.3 7.8 11.8

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022




#48
2,6-Dinitrotoluene
Concen: 34.005 ng/ul
RT: 14.222 min Scan# 1876
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Tgt Ion:165 Resp: 740735
Ion Ratio Lower Upper
165 100
89 54.4 42.7 64.1
121 21.2 16.9 25.3

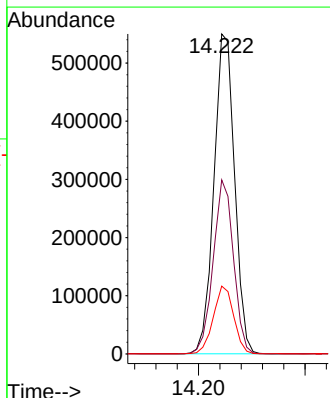



#50
Acenaphthylene
Concen: 27.555 ng/ul
RT: 14.375 min Scan# 1902
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument : BNA_P
ClientSampleId : SLCS200



Tgt Ion:152 Resp: 4668268
Ion Ratio Lower Upper
152 100
151 19.9 15.9 23.9
153 13.2 10.7 16.1




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

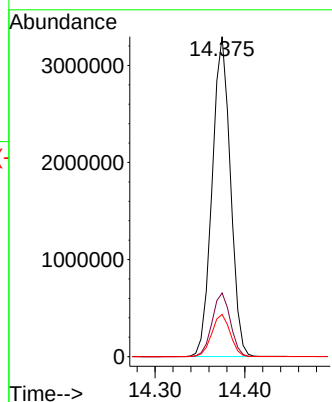

#51
3-Nitroaniline
Concen: 28.763 ng/ul
RT: 14.551 min Scan# 1932
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion:138 Resp: 725644
Ion Ratio Lower Upper
138 100
108 10.4 9.9 14.9
92 111.5 90.2 135.2

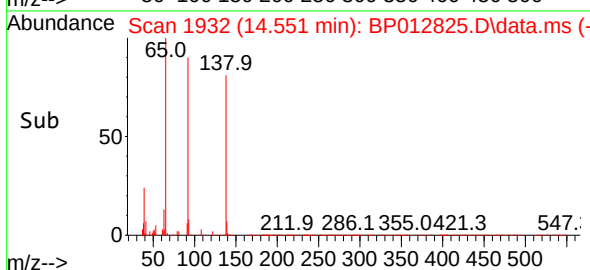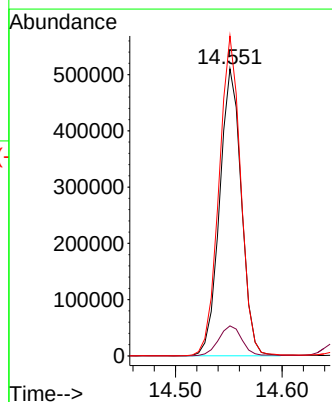



#52
Acenaphthene
Concen: 27.161 ng/ul
RT: 14.716 min Scan# 1960
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200




Tgt Ion:153 Resp: 3239532
Ion Ratio Lower Upper
153 100
152 47.2 38.2 57.4
154 89.0 69.8 104.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022




#53
2,4-Dinitrophenol
Concen: 28.328 ng/ul
RT: 14.751 min Scan# 1966
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56

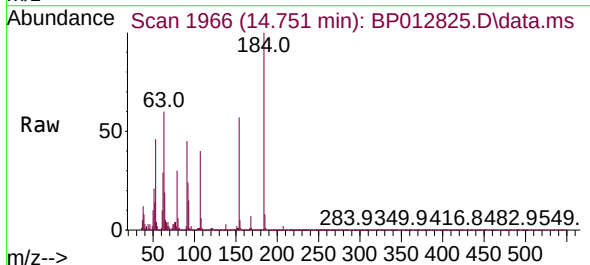


Tgt Ion:184 Resp: 396531
Ion Ratio Lower Upper
184 100
63 59.6 48.1 72.1
154 56.5 47.4 71.2

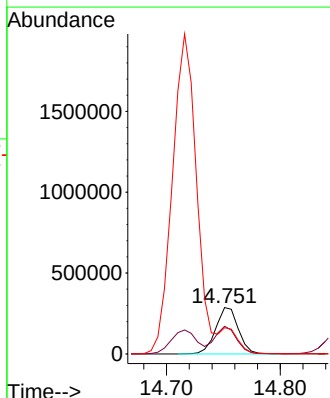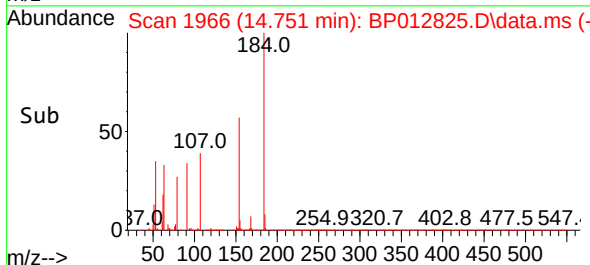



#55
4-Nitrophenol
Concen: 27.312 ng/ul
RT: 14.851 min Scan# 1982
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200

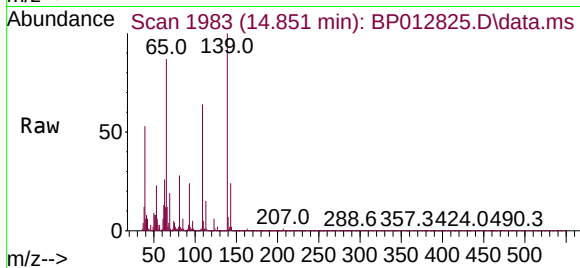

Tgt Ion:109 Resp: 469753
Ion Ratio Lower Upper
109 100
139 157.4 119.2 178.8
65 136.8 110.7 166.1




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

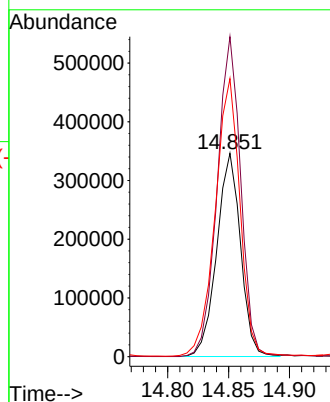

#56
Dibenzofuran
Concen: 27.504 ng/ul
RT: 15.051 min Scan# 2017
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion:168 Resp: 4521623
Ion Ratio Lower Upper
168 100
139 34.4 27.7 41.5

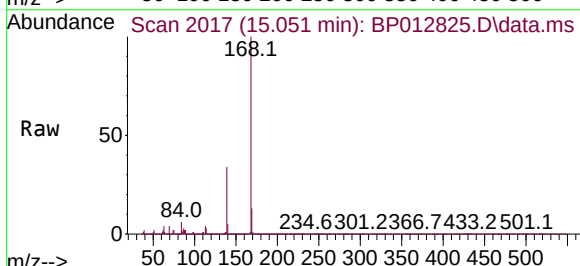



#57
2,4-Dinitrotoluene
Concen: 33.038 ng/ul
RT: 15.010 min Scan# 2009
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200

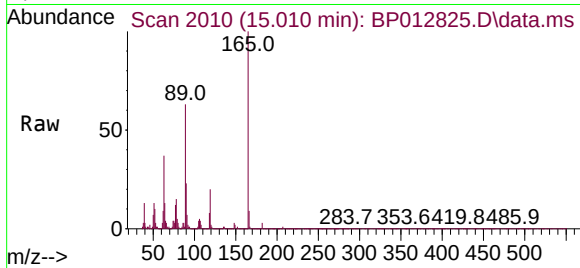


Tgt Ion:165 Resp: 1062033
Ion Ratio Lower Upper
165 100
63 36.7 31.0 46.4
182 2.7 2.0 3.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

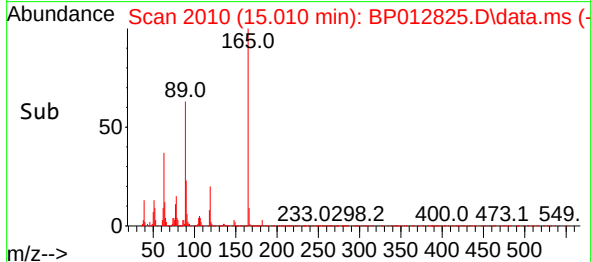


#58
2,3,4,6-Tetrachlorophenol
Concen: 28.874 ng/ul
RT: 15.275 min Scan# 2055
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56

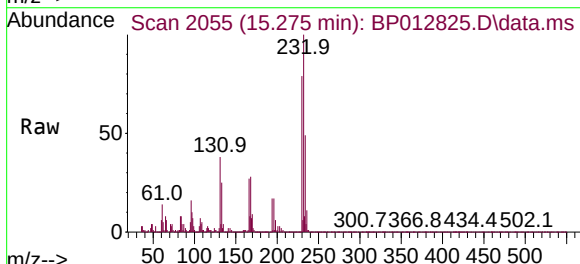


Tgt Ion:232 Resp: 1029755
Ion Ratio Lower Upper
232 100
131 37.8 32.0 48.0
130 1.8 1.5 2.3
166 27.3 23.2 34.8

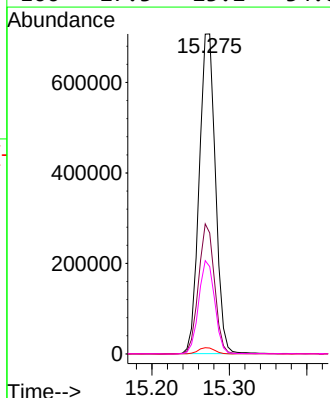



#59
Diethylphthalate
Concen: 27.726 ng/ul
RT: 15.469 min Scan# 2088
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200



Tgt Ion:149 Resp: 3735705
Ion Ratio Lower Upper
149 100
177 23.3 18.1 27.1
150 12.8 9.8 14.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022



#61
Fluorene
Concen: 27.700 ng/ul
RT: 15.704 min Scan# 2128
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion:166 Resp: 3651973
Ion Ratio Lower Upper
166 100
165 97.6 78.2 117.2
167 13.4 10.9 16.3





#62
4-Chlorophenyl-phenylether
Concen: 27.757 ng/ul
RT: 15.692 min Scan# 2126
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200




Tgt Ion:204 Resp: 1898697
Ion Ratio Lower Upper
204 100
206 32.8 26.0 39.0
141 50.0 40.7 61.1

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022




#63
4-Nitroaniline
Concen: 33.016 ng/ul
RT: 15.716 min Scan# 2130
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56



Tgt Ion:138 Resp: 709908
Ion Ratio Lower Upper
138 100
92 47.7 38.6 57.8
108 69.6 56.4 84.6

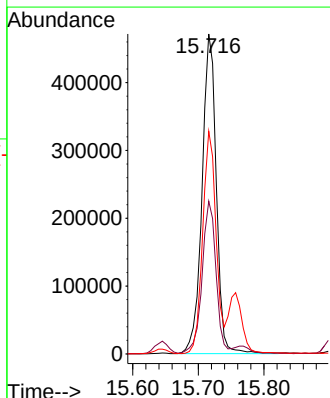







#66
4,6-Dinitro-2-methylphenol
Concen: 30.450 ng/ul
RT: 15.769 min Scan# 2139
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56

Instrument :
BNA_P
ClientSampleId :
SLCS200

Tgt Ion:198 Resp: 621549
Ion Ratio Lower Upper
198 100
182 4.3 4.1 6.1
77 22.5 18.9 28.3




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

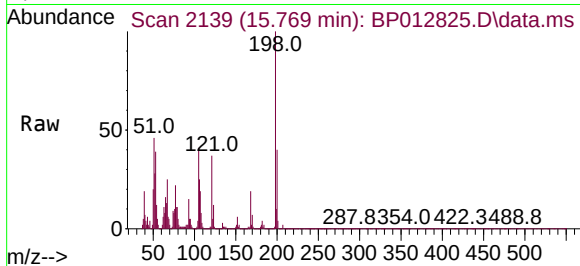

#67
N-Nitrosodiphenylamine
Concen: 28.148 ng/ul
RT: 15.904 min Scan# 2162
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion:169 Resp: 3182904
Ion Ratio Lower Upper
169 100
168 66.7 53.2 79.8
167 36.1 29.6 44.4

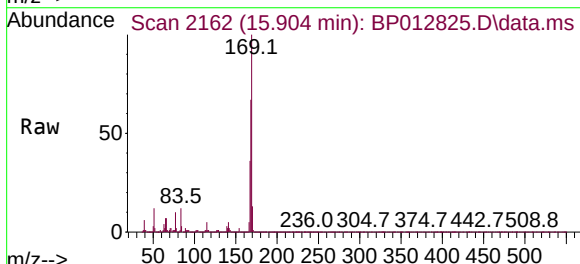



#68
4-Bromophenyl-phenylether
Concen: 29.496 ng/ul
RT: 16.592 min Scan# 2279
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200



Tgt Ion:248 Resp: 115507
Ion Ratio Lower Upper
248 100
250 98.5 78.6 118.0
141 59.9 48.7 73.1




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

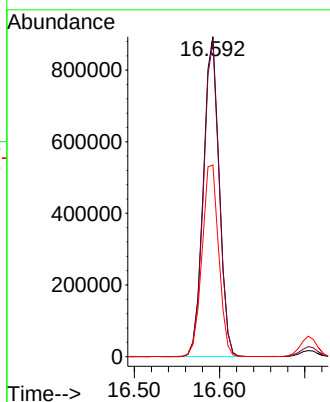

#69
Hexachlorobenzene
Concen: 28.136 ng/ul
RT: 16.704 min Scan# 2298
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion:284 Resp: 1404312
Ion Ratio Lower Upper
284 100
142 31.1 25.0 37.6
249 30.4 24.6 36.8

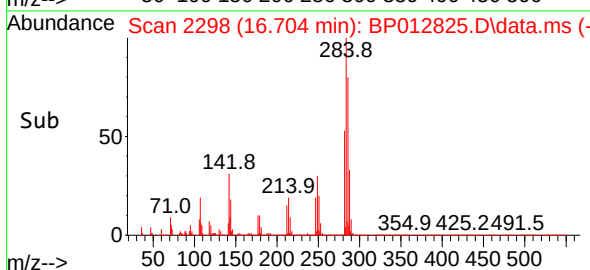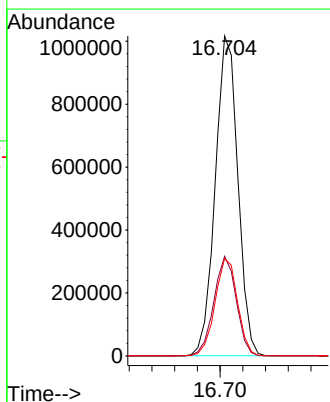



#70
Atrazine
Concen: 27.916 ng/ul
RT: 16.863 min Scan# 2325
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200



Tgt Ion:200 Resp: 1083060
Ion Ratio Lower Upper
200 100
173 25.3 20.3 30.5
215 49.7 40.1 60.1




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022



#71
Pentachlorophenol
Concen: 27.248 ng/ul
RT: 17.051 min Scan# 2357
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion:266 Resp: 835166
Ion Ratio Lower Upper
266 100
264 62.7 50.7 76.1
268 65.2 51.8 77.8

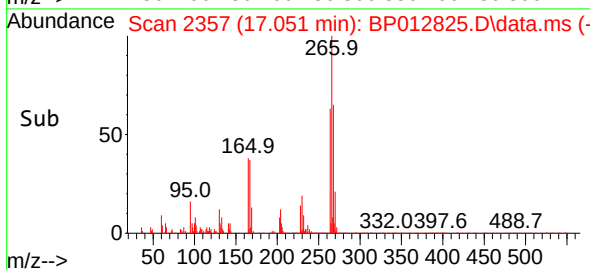



#72
Phenanthrene
Concen: 27.493 ng/ul
RT: 17.451 min Scan# 2425
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200



Tgt Ion:178 Resp: 5830127
Ion Ratio Lower Upper
178 100
179 15.8 12.3 18.5
176 19.5 15.4 23.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022



#74
Anthracene
Concen: 27.664 ng/ul
RT: 17.545 min Scan# 2441
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion:178 Resp: 5803530
Ion Ratio Lower Upper
178 100
179 15.5 12.4 18.6
176 18.7 14.8 22.2





#75
1,2,3,4-Tetrachlorobenzene
Concen: 26.854 ng/uL
RT: 13.451 min Scan# 1745
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200




Tgt Ion:216 Resp: 1651838
Ion Ratio Lower Upper
216 100
214 77.8 62.3 93.5
218 47.9 39.1 58.7

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022




#76
Pentachlorobenzene
Concen: 25.219 ng/uL
RT: 14.969 min Scan# 2003
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Tgt Ion:250 Resp: 1612537
Ion Ratio Lower Upper
250 100
248 62.2 50.6 76.0
252 62.9 50.5 75.7

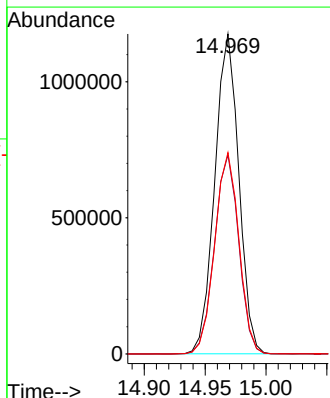



#77
 Carbazole
 Concen: 29.142 ng/ul
 RT: 17.804 min Scan# 2485
 Delta R.T. -0.006 min
 Lab File: BP012825.D
 Acq: 28 Nov 2022 19:56




Instrument : BNA_P
 ClientSampleId : SLCS200




Tgt Ion:167 Resp: 5171960
 Ion Ratio Lower Upper
 167 100
 166 21.5 17.1 25.7
 139 12.2 9.8 14.8

Manual Integrations
 APPROVED



Reviewed By :Jagrut Upadhyay 11/29/2022
 Supervised By :mohammad ahmed 11/30/2022




#78
 Di-n-butylphthalate
 Concen: 28.736 ng/ul
 RT: 18.351 min Scan# 2578
 Delta R.T. -0.006 min
 Lab File: BP012825.D
 Acq: 28 Nov 2022 19:56




Tgt Ion:149 Resp: 6037223
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.2 10.8
 104 4.6 3.7 5.5

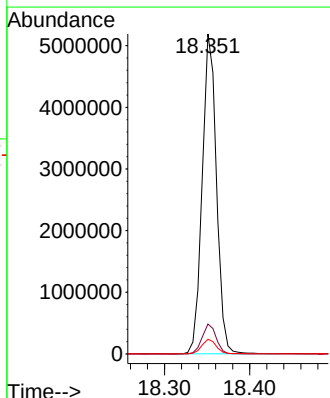



#80
Fluoranthene
Concen: 29.284 ng/ul
RT: 19.410 min Scan# 2758
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200




Tgt Ion:202 Resp: 6496200
Ion Ratio Lower Upper
202 100
101 10.4 8.7 13.1
100 8.0 6.9 10.3

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

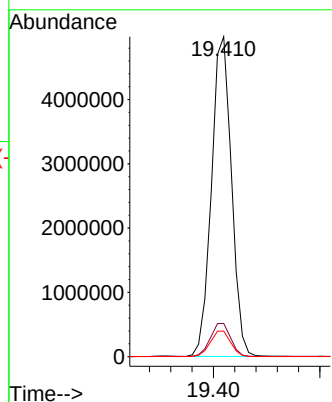


#82
Pyrene
Concen: 28.765 ng/ul
RT: 19.763 min Scan# 2818
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56



Tgt Ion:202 Resp: 6599735
Ion Ratio Lower Upper
202 100
101 12.1 10.3 15.5
100 9.8 8.6 13.0





#83

Butylbenzylphthalate

Concen: 38.397 ng/ul

RT: 20.627 min Scan# 2966

Delta R.T. -0.006 min

Lab File: BP012825.D

Acq: 28 Nov 2022 19:56

Instrument :

BNA_P

ClientSampleId :

SLCS200

Tgt Ion:149 Resp: 2061563

Ion Ratio Lower Upper

149 100





91 69.2 58.2 87.2

206 21.9 16.5 24.7

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

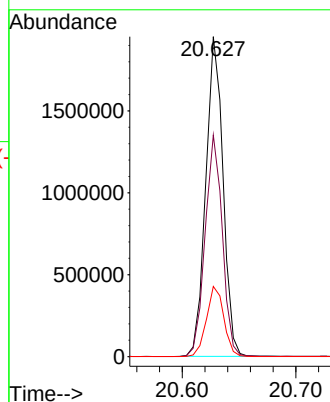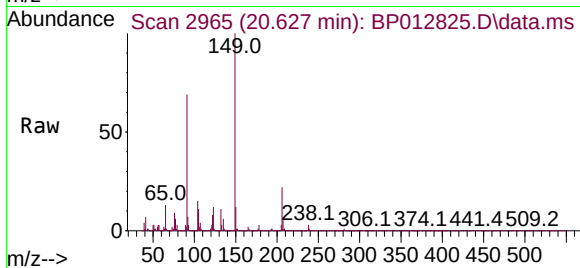

#84

3,3'-Dichlorobenzidine

Concen: 27.573 ng/ul

RT: 21.404 min Scan# 3097

Delta R.T. -0.000 min

Lab File: BP012825.D

Acq: 28 Nov 2022 19:56




Tgt Ion:252 Resp: 1554173


Ion Ratio Lower Upper

252 100

254 64.4 52.3 78.5


126 9.4 7.6 11.4

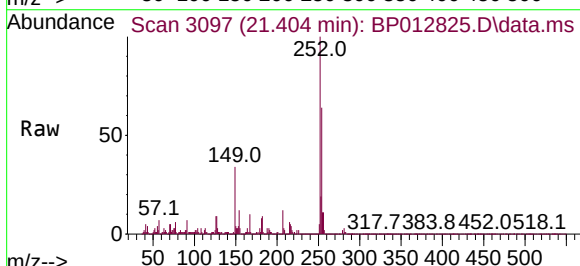



#85
Benzo(a)anthracene
Concen: 26.084 ng/ul
RT: 21.474 min Scan# 3110
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200

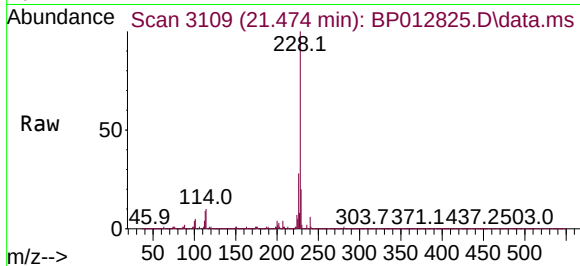

Tgt Ion:228 Resp: 5537427
Ion Ratio Lower Upper
228 100
229 20.0 16.2 24.2
226 27.5 22.2 33.2




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

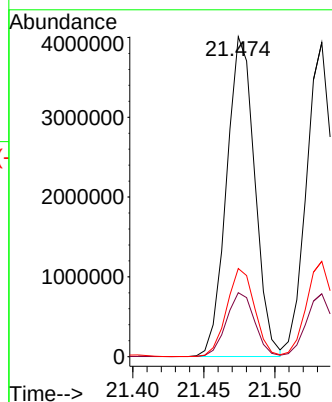

#86
Bis(2-ethylhexyl)phthalate
Concen: 33.337 ng/ul
RT: 21.392 min Scan# 3095
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56


Tgt Ion:149 Resp: 2737281
Ion Ratio Lower Upper
149 100
167 28.3 22.7 34.1
279 4.8 3.8 5.6

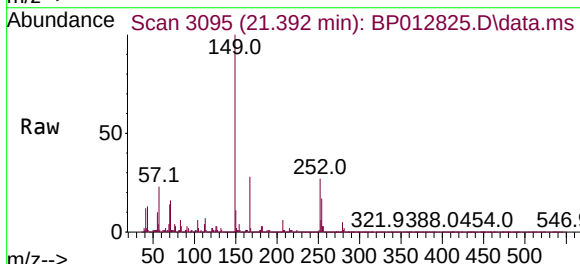



#87
Chrysene
Concen: 25.315 ng/ul
RT: 21.533 min Scan# 3119
Delta R.T. -0.000 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200



Tgt Ion:228 Resp: 5196093
Ion Ratio Lower Upper
228 100
226 30.3 24.3 36.5
229 20.0 15.9 23.9




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022



#89
Di-n-octyl phthalate
Concen: 28.979 ng/ul
RT: 22.357 min Scan# 3259
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56

Tgt Ion:149 Resp: 3702419

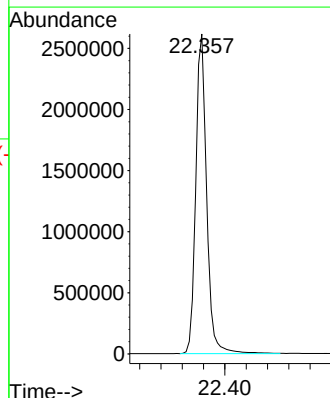



#90
Benzo(b)fluoranthene
Concen: 27.290 ng/ul
RT: 23.233 min Scan# 3409
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56

Instrument :

BNA_P

ClientSampleId :





SLCS200

Tgt Ion:252 Resp: 4521273
Ion Ratio Lower Upper
252 100
253 22.4 17.6 26.4
125 9.6 7.4 11.2

Manual Integrations




APPROVED


Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

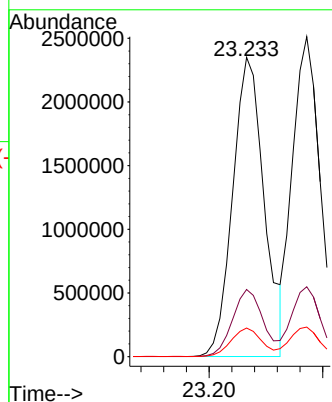

#91
Benzo(k)fluoranthene
Concen: 25.710 ng/ul
RT: 23.286 min Scan# 3417
Delta R.T. -0.006 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56

Tgt Ion:252 Resp: 4251702
Ion Ratio Lower Upper
252 100
253 21.8 17.8 26.8
125 9.2 7.8 11.8





#93

Benzo(a)pyrene

Concen: 27.192 ng/ul

RT: 23.892 min Scan# 31

Delta R.T. -0.006 min

Lab File: BP012825.D

Acq: 28 Nov 2022 19:56

Instrument :

BNA_P

ClientSampleId :

SLCS200

Tgt Ion:252 Resp: 3704528

Ion Ratio Lower Upper

252 100





253 21.9 17.6 26.4

125 10.7 8.5 12.7

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022



#94

Indeno(1,2,3-cd)pyrene

Concen: 30.965 ng/ul

RT: 26.645 min Scan# 3988

Delta R.T. -0.006 min

Lab File: BP012825.D

Acq: 28 Nov 2022 19:56




Tgt Ion:276 Resp: 4069937


Ion Ratio Lower Upper

276 100

138 23.2 18.3 27.5


277 25.2 19.8 29.8

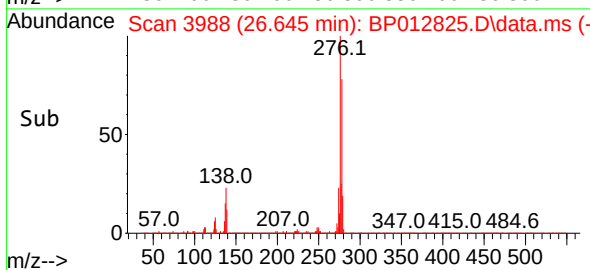



#95
Dibenzo(a,h)anthracene
Concen: 30.090 ng/ul
RT: 26.662 min Scan# 3992
Delta R.T. -0.012 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56




Instrument :
BNA_P
ClientSampleId :
SLCS200



Tgt Ion:278 Resp: 3588696
Ion Ratio Lower Upper
278 100
139 14.5 12.6 18.8
279 23.6 19.4 29.2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/29/2022
Supervised By :mohammad ahmed 11/30/2022

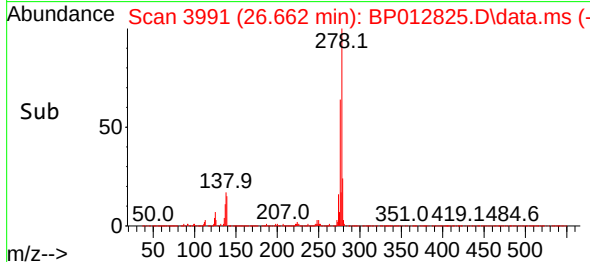

#96
Benzo(g,h,i)perylene
Concen: 31.724 ng/ul
RT: 27.445 min Scan# 4124
Delta R.T. -0.012 min
Lab File: BP012825.D
Acq: 28 Nov 2022 19:56

Tgt Ion:276 Resp: 3586532
Ion Ratio Lower Upper
276 100
138 20.0 16.7 25.1
277 23.7 19.1 28.7

