

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012834.D
 Acq On : 29 Nov 2022 01:37
 Operator : CG/JU
 Sample : N5666-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGXP5

Quant Time: Nov 29 02:14:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)


Internal Standards					
1) 1,4-Dichlorobenzene-d4	8.016	152	512242	20.000 ng/u1	0.00
20) Naphthalene-d8	10.828	136	2231295	20.000 ng/u1	0.00
38) Acenaphthene-d10	14.651	164	1384063	20.000 ng/u1	0.00
64) Phenanthrene-d10	17.404	188	2503881	20.000 ng/u1	0.00
79) Chrysene-d12	21.486	240	1584997	20.000 ng/u1	-0.01
88) Perylene-d12	23.998	264	1685722	20.000 ng/u1	-0.01
System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.399	96	61683	5.160 ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000 ng/u1	
7) Phenol-d5	7.163	99	467757	11.113 ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	1089209	41.994 ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	1146326	35.740 ng/u1	0.00
15) 4-Methylphenol-d8	8.716	113	780660	23.019 ng/u1	0.00
21) Nitrobenzene-d5	9.181	128	652207	47.757 ng/u1	0.00
24) 2-Nitrophenol-d4	9.904	143	704951	48.614 ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	1270718	37.557 ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	176212	3.803 ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	4051362	42.526 ng/u1	0.00
49) Acenaphthylene-d8	14.345	160	4753816	42.766 ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	89957	5.296 ng/u1	0.00
60) Fluorene-d10	15.639	176	3571793	42.811 ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	412600	34.477 ng/u1	0.00
73) Anthracene-d10	17.504	188	5102616	46.295 ng/u1	0.00
81) Pyrene-d10	19.727	212	4738052	51.446 ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	3897078	47.065 ng/u1	-0.01
Target Compounds					
2) 1,4-Dioxane	3.434	88	129129	10.058 ng/uL	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012834.D
Acq On : 29 Nov 2022 01:37
Operator : CG/JU
Sample : N5666-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGXP5

Quant Time: Nov 29 02:14:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

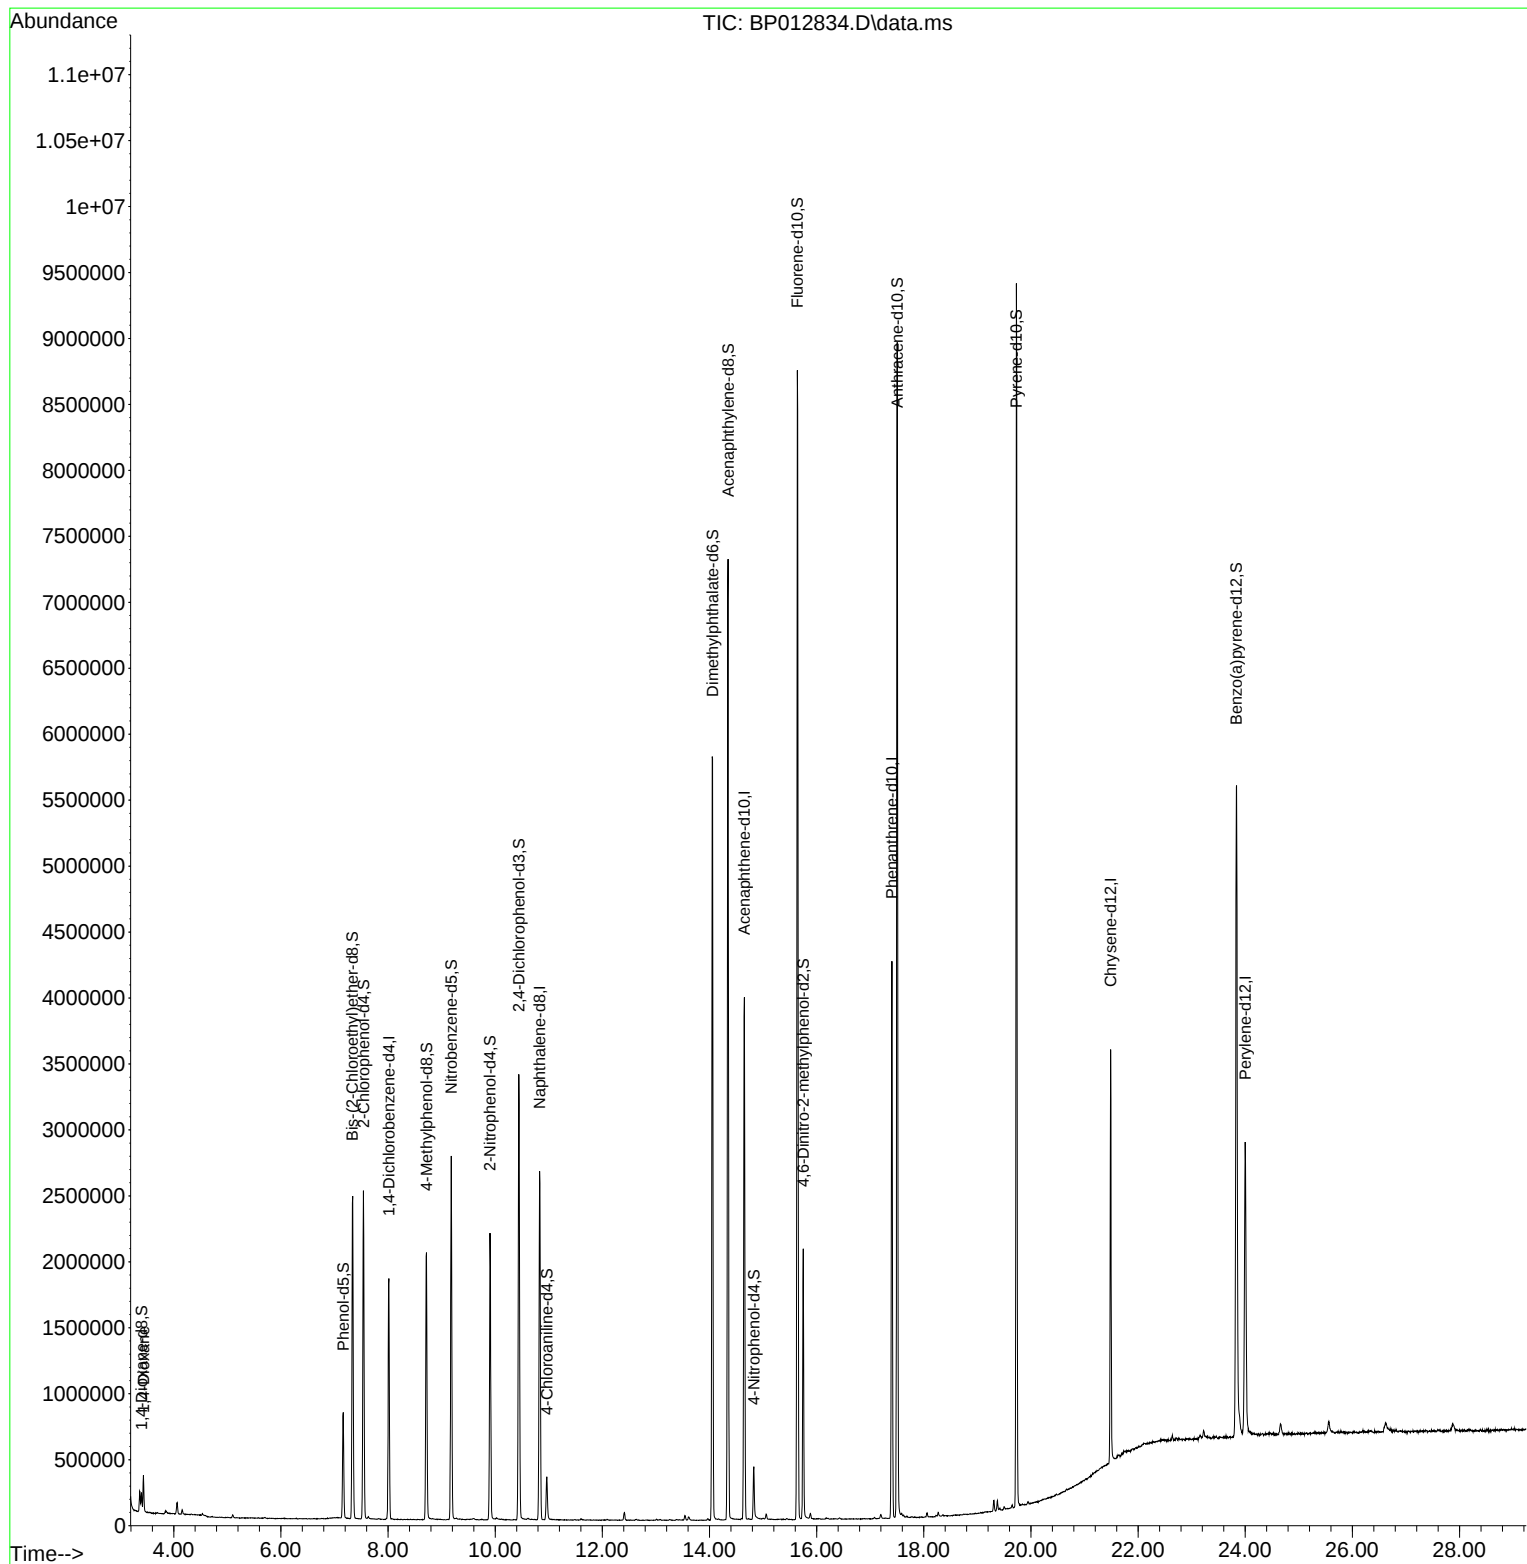

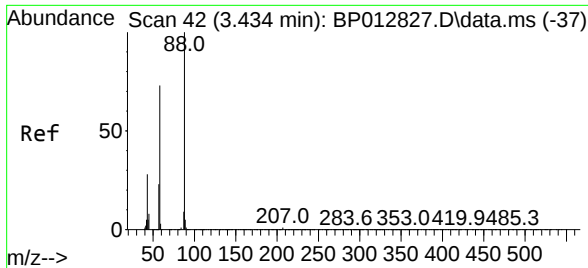

#2
 1,4-Dioxane
 Concen: 10.058 ng/uL
 RT: 3.434 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BP012834.D
 Acq: 29 Nov 2022 01:37

Instrument :
 BNA_P
 ClientSampleId :
 BGXP5

Tgt Ion: 88	Resp: 129129
Ion Ratio	Lower Upper
88	100
43	27.8 22.6 34.0
58	70.3 59.6 89.4

