

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012835.D
 Acq On : 29 Nov 2022 02:11
 Operator : CG/JU
 Sample : N5666-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGXP6

Quant Time: Nov 29 03:17:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	598293	20.000	ng/u1	0.00
20) Naphthalene-d8	10.828	136	2698960	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	1797894	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.404	188	3613152	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	2317043	20.000	ng/u1	-0.01
88) Perylene-d12	23.998	264	1981425	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	47550	3.406	ng/uL	0.00
4) Pyridine-d5	3.834	84	55505	1.328	ng/u1	0.01
7) Phenol-d5	7.163	99	306904	6.243	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	840305	27.738	ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	822022	21.943	ng/u1	0.00
15) 4-Methylphenol-d8	8.716	113	557928	14.085	ng/u1	0.00
21) Nitrobenzene-d5	9.181	128	497351	30.108	ng/u1	0.00
24) 2-Nitrophenol-d4	9.904	143	514897	29.355	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	964790	23.574	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	776994	13.864	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	3811791	30.802	ng/u1	0.00
49) Acenaphthylene-d8	14.345	160	4040751	27.984	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	83194	3.771	ng/u1	0.00
60) Fluorene-d10	15.639	176	3436157	31.705	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	409801	23.730	ng/u1	0.00
73) Anthracene-d10	17.504	188	5610543	35.276	ng/u1	0.00
81) Pyrene-d10	19.727	212	5663040	42.063	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.839	264	3384872	34.779	ng/u1	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.098	107	73132	1.703	ng/u1	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012835.D
Acq On : 29 Nov 2022 02:11
Operator : CG/JU
Sample : N5666-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGXP6

Quant Time: Nov 29 03:17:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

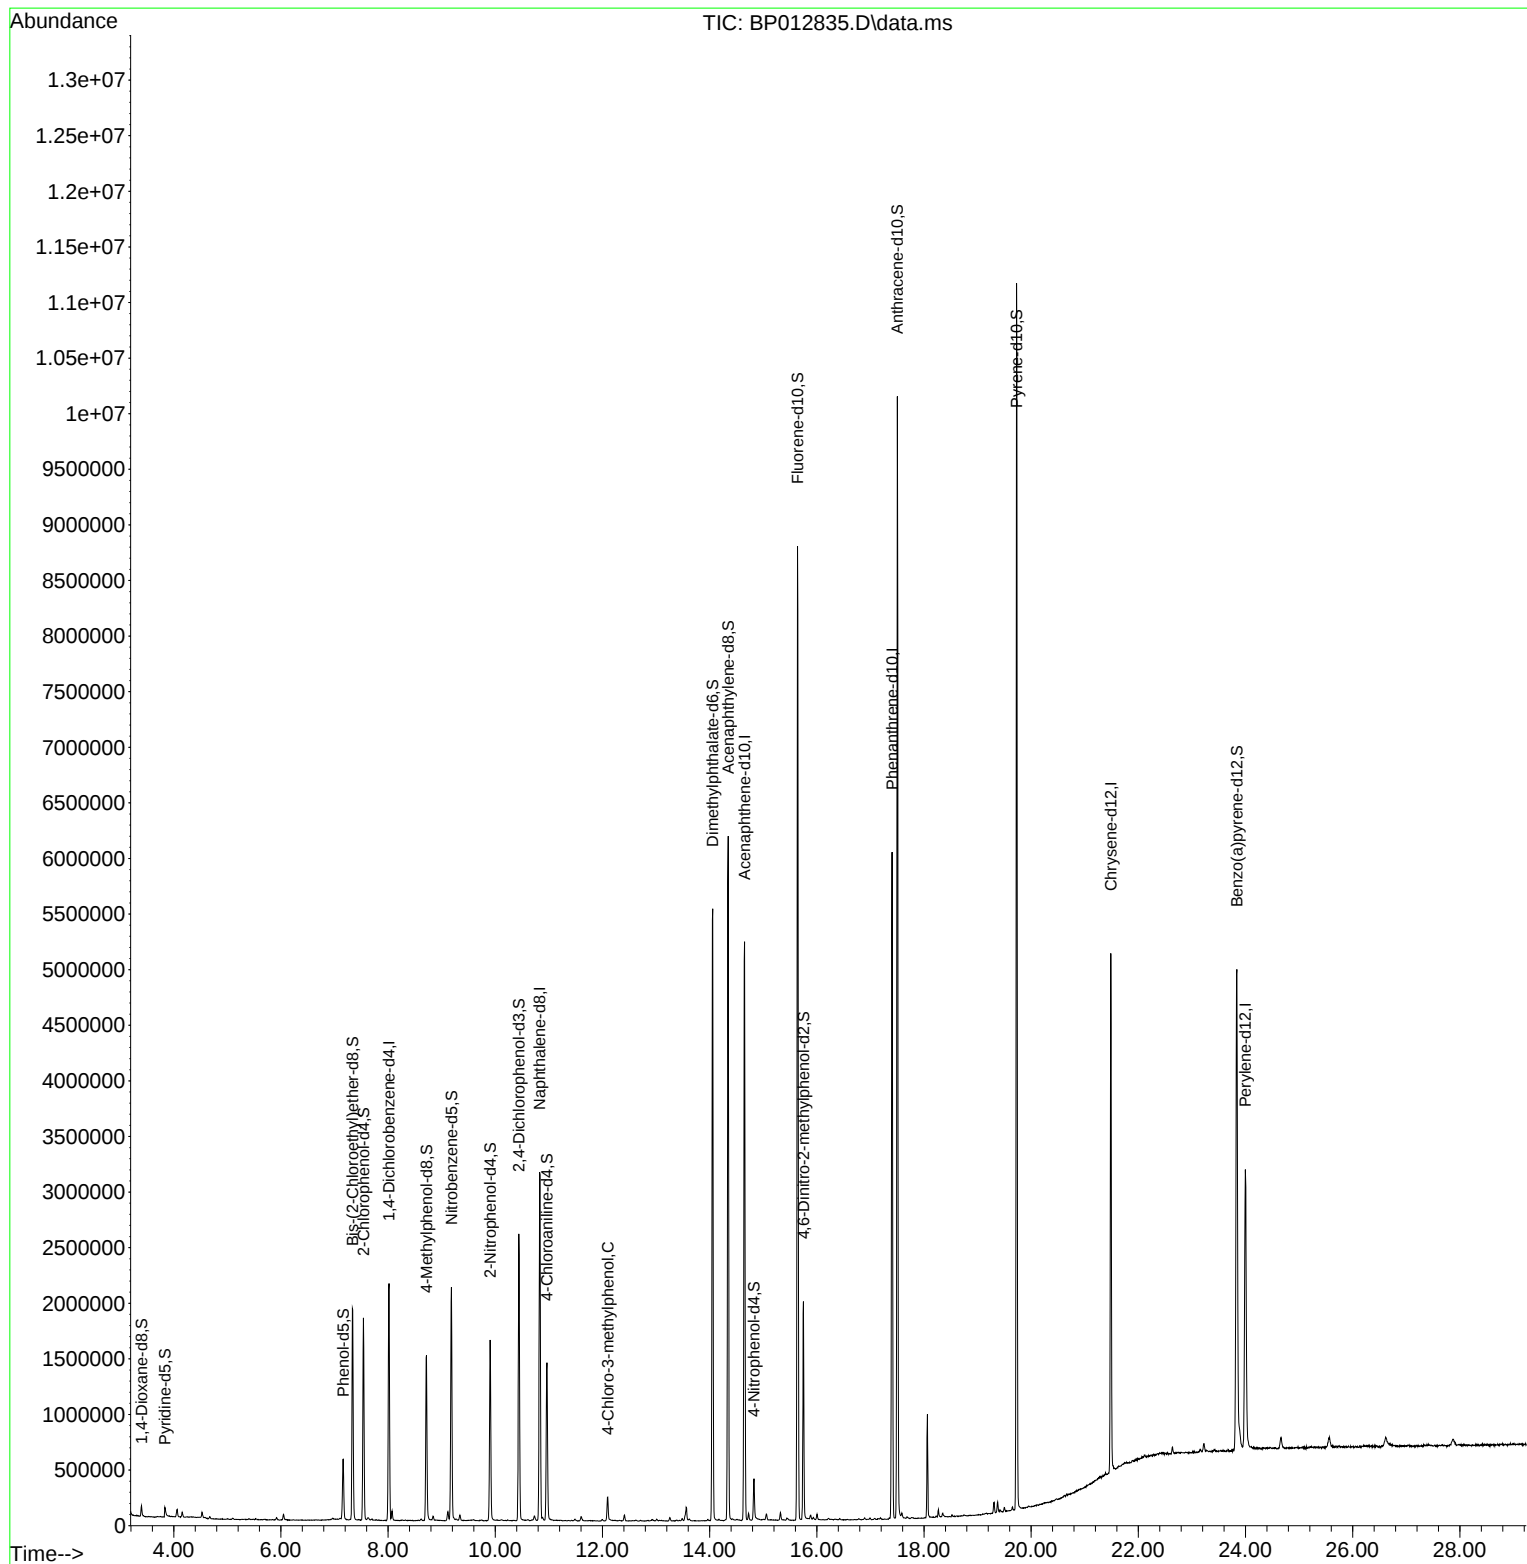

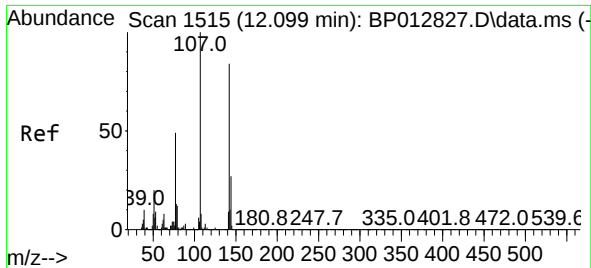

#35
 4-Chloro-3-methylphenol
 Concen: 1.703 ng/ul
 RT: 12.098 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BP012835.D
 Acq: 29 Nov 2022 02:11

Instrument :
 BNA_P
 ClientSampleId :
 BGXP6

Tgt Ion:107 Resp: 73132
 Ion Ratio Lower Upper
 107 100
 144 27.5 21.4 32.2
 142 83.2 66.6 100.0

