

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012836.D
 Acq On : 29 Nov 2022 02:46
 Operator : CG/JU
 Sample : N5666-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGXP7

Quant Time: Nov 29 03:17:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 27 22:55:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	562590	20.000	ng/u1	0.00
20) Naphthalene-d8	10.828	136	2501577	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	1656026	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.404	188	3192863	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	1907320	20.000	ng/u1	-0.01
88) Perylene-d12	23.998	264	1835655	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	73066	5.565	ng/uL	0.00
4) Pyridine-d5	3.828	84	187391	4.770	ng/u1	0.00
7) Phenol-d5	7.163	99	395994	8.566	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	1051946	36.928	ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	1019982	28.955	ng/u1	0.00
15) 4-Methylphenol-d8	8.716	113	703699	18.893	ng/u1	0.00
21) Nitrobenzene-d5	9.181	128	627273	40.969	ng/u1	0.00
24) 2-Nitrophenol-d4	9.905	143	624531	38.415	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	1180500	31.120	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	747079	14.382	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	4199059	36.838	ng/u1	0.00
49) Acenaphthylene-d8	14.345	160	4798244	36.077	ng/u1	0.00
54) 4-Nitrophenol-d4	14.828	143	88830	4.371	ng/u1	0.00
60) Fluorene-d10	15.640	176	3691255	36.977	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	402897	26.402	ng/u1	0.00
73) Anthracene-d10	17.504	188	5399859	38.420	ng/u1	0.00
81) Pyrene-d10	19.728	212	5125365	46.247	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	3408791	37.806	ng/u1	-0.01
Target Compounds						
35) 4-Chloro-3-methylphenol	12.093	107	80881	2.033	ng/u1	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012836.D
Acq On : 29 Nov 2022 02:46
Operator : CG/JU
Sample : N5666-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGXP7

Quant Time: Nov 29 03:17:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 27 22:55:08 2022
Response via : Initial Calibration

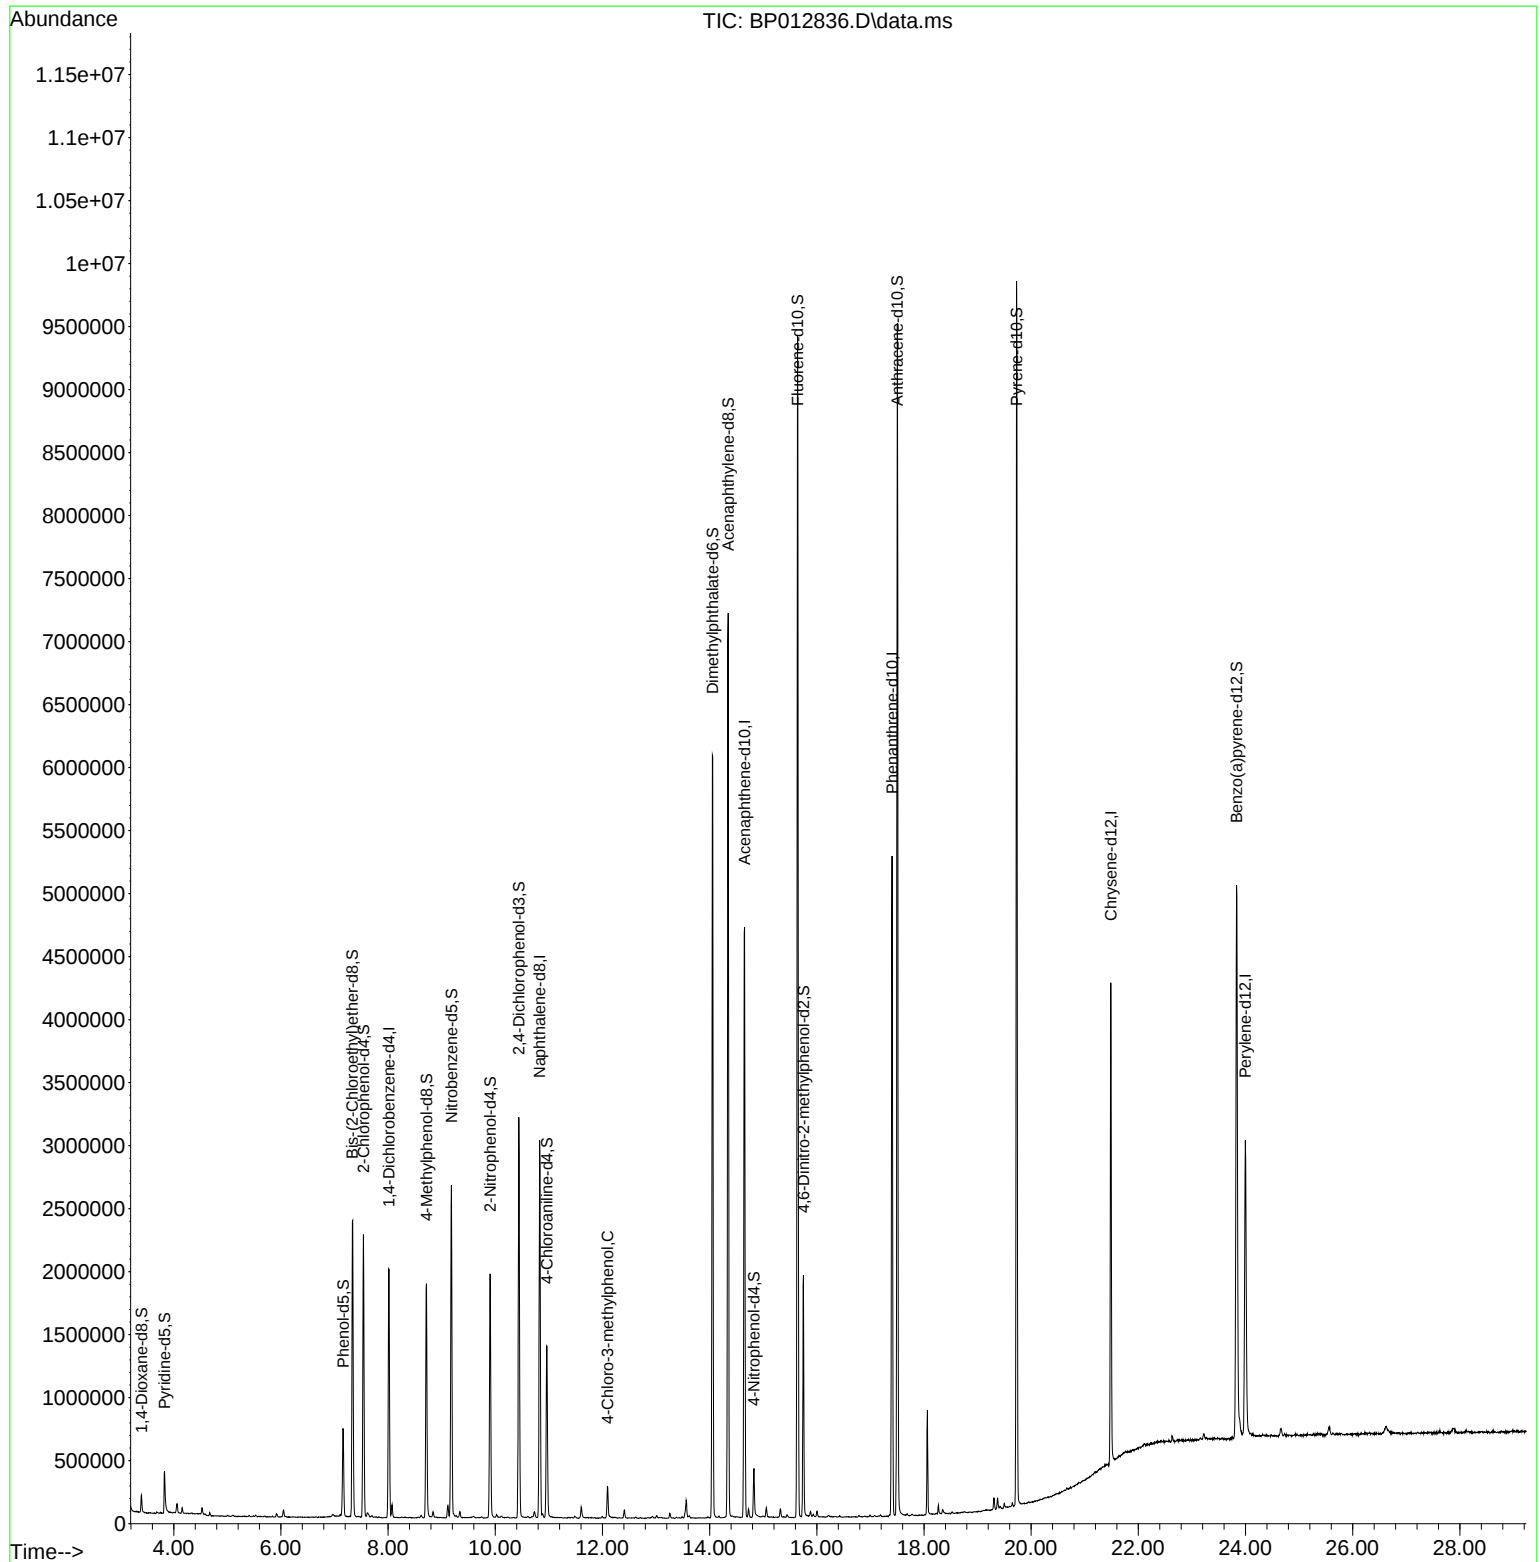

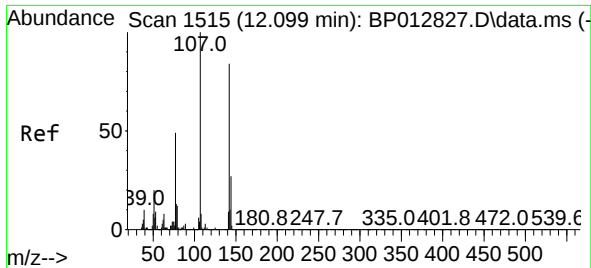

#35
 4-Chloro-3-methylphenol
 Concen: 2.033 ng/ul
 RT: 12.093 min Scan# 11
 Delta R.T. -0.012 min
 Lab File: BP012836.D
 Acq: 29 Nov 2022 02:46

Instrument :
 BNA_P
 ClientSampleId :
 BGXP7

Tgt Ion:107 Resp: 80881
 Ion Ratio Lower Upper
 107 100
 144 27.7 21.4 32.2
 142 87.9 66.6 100.0

