

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012810.D
 Acq On : 28 Nov 2022 11:19
 Operator : CG/JU
 Sample : PB149261BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK261

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012810.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	31	35	47	rVB	107097	163867	1.40%	0.135%
2	3.822	104	108	122	rBV	773565	1306199	11.19%	1.073%
3	4.158	162	165	170	rVB	28863	37477	0.32%	0.031%
4	7.163	669	676	688	rVB	1661712	2530799	21.69%	2.079%
5	7.340	699	706	716	rVB	1417501	2208217	18.92%	1.814%
6	7.540	732	740	752	rBV	1652139	2584071	22.14%	2.123%
7	8.016	814	821	836	rVB	1765430	2739273	23.47%	2.250%
8	8.716	932	940	948	rBV	2103839	3303692	28.31%	2.714%
9	9.181	1011	1019	1029	rBV	1504321	2418318	20.72%	1.987%
10	9.604	1087	1091	1099	rVB7	11532	26299	0.23%	0.022%
11	9.904	1135	1142	1155	rBV	1204190	1951509	16.72%	1.603%
12	10.446	1225	1234	1244	rBV	2026180	3458065	29.63%	2.841%
13	10.834	1292	1300	1309	rVB	2603911	4301871	36.87%	3.534%
14	10.963	1314	1322	1345	rBV	4137099	7234466	62.00%	5.944%
15	12.093	1510	1514	1519	rVB6	7573	12577	0.11%	0.010%
16	12.410	1561	1568	1574	rBV2	37016	63488	0.54%	0.052%
17	13.387	1729	1734	1739	rBV8	7785	14511	0.12%	0.012%
18	13.628	1771	1775	1780	rVB4	9440	13295	0.11%	0.011%
19	14.057	1840	1848	1861	rBV	4020423	5599911	47.99%	4.601%
20	14.345	1890	1897	1911	rBV	4734370	6714336	57.54%	5.516%
21	14.651	1940	1949	1958	rBV	4412091	6292915	53.93%	5.170%
22	14.828	1972	1979	1992	rBV	1631336	2391592	20.50%	1.965%
23	15.057	2013	2018	2025	rVB	10155	25150	0.22%	0.021%
24	15.645	2110	2118	2127	rBV	6090632	8846517	75.81%	7.268%
25	15.751	2130	2136	2152	rVV	1495437	1979069	16.96%	1.626%
26	15.887	2155	2159	2165	rVB3	27113	41109	0.35%	0.034%
27	17.192	2374	2381	2386	rBV4	12664	23230	0.20%	0.019%
28	17.404	2411	2417	2426	rBV	5295467	7668142	65.71%	6.300%
29	17.504	2428	2434	2454	rVV	6747763	9742920	83.49%	8.004%
30	18.281	2562	2566	2568	rBV4	12793	15626	0.13%	0.013%
31	19.310	2737	2741	2748	rBV3	79814	112816	0.97%	0.093%
32	19.380	2748	2753	2758	rBV	73070	112678	0.97%	0.093%
33	19.733	2807	2813	2824	rBV	9405238	11668980	100.00%	9.587%
34	21.492	3107	3112	3121	rBV	6213226	8464354	72.54%	6.954%
35	23.845	3505	3512	3520	rBV2	4973084	9843636	84.36%	8.087%
36	24.010	3533	3540	3557	rVB2	3679248	7809441	66.92%	6.416%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012810.D
Acq On : 28 Nov 2022 11:19
Operator : CG/JU
Sample : PB149261BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 121720416

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012810.D
Acq On : 28 Nov 2022 11:19
Operator : CG/JU
Sample : PB149261BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

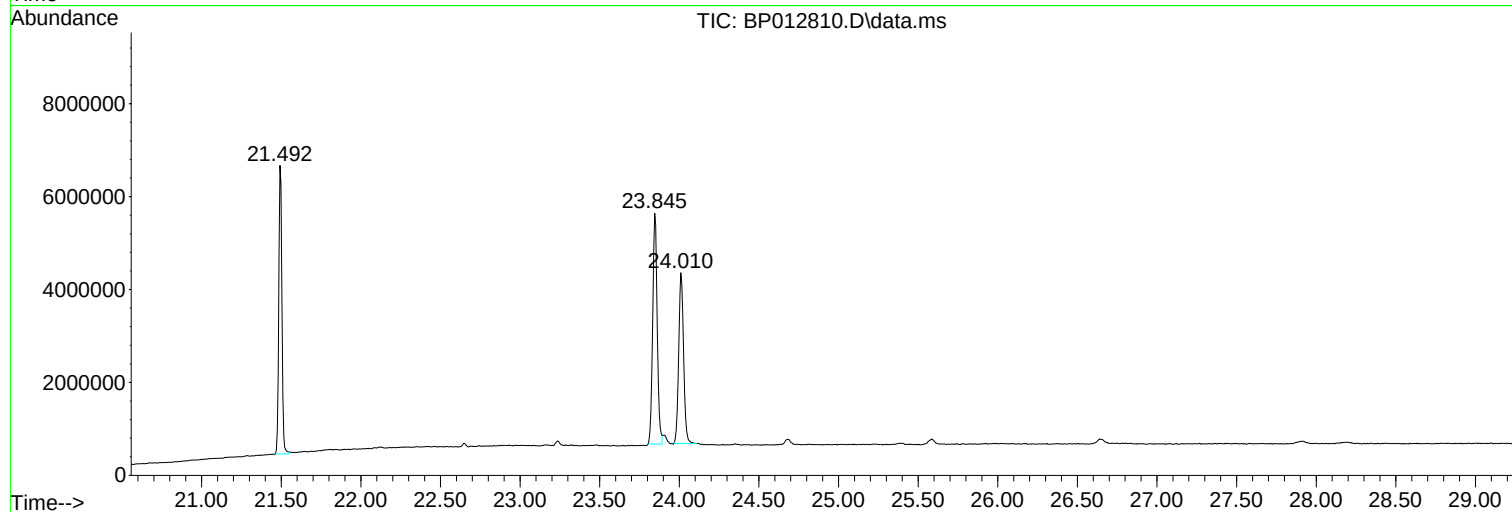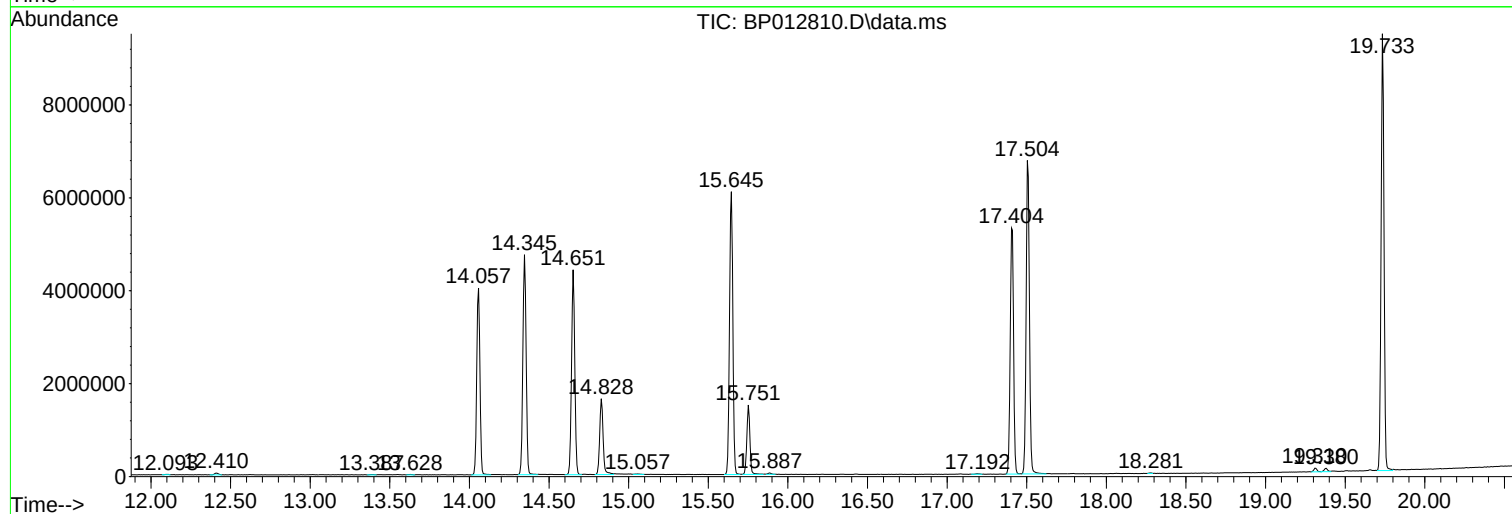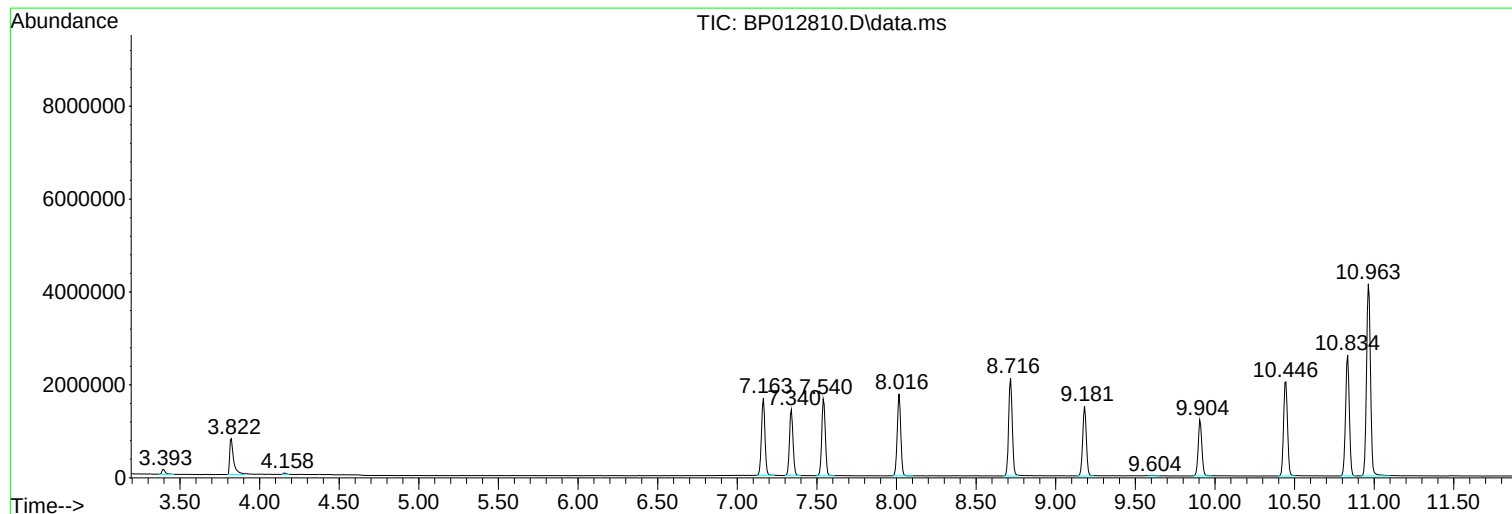

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012810.D
Acq On : 28 Nov 2022 11:19
Operator : CG/JU
Sample : PB149261BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012810.D
Acq On : 28 Nov 2022 11:19
Operator : CG/JU
Sample : PB149261BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc