

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012813.D
 Acq On : 28 Nov 2022 13:02
 Operator : CG/JU
 Sample : N5710-09DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KY8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012813.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	25	30	38	rBV	3690306	5837832	65.24%	9.351%
2	3.428	38	41	53	rVB	426552	687541	7.68%	1.101%
3	4.158	161	165	171	rBV2	30960	41709	0.47%	0.067%
4	4.699	251	257	266	rVB	247472	383334	4.28%	0.614%
5	4.946	294	299	303	rBV5	11671	18086	0.20%	0.029%
6	5.434	378	382	387	rVB3	10669	17364	0.19%	0.028%
7	7.164	670	676	684	rVB	78239	140279	1.57%	0.225%
8	7.340	700	706	715	rBV	339622	536770	6.00%	0.860%
9	7.540	735	740	750	rVV	288170	454934	5.08%	0.729%
10	8.016	812	821	828	rBV	1752324	2764304	30.89%	4.428%
11	8.075	828	831	835	rVB5	8562	11811	0.13%	0.019%
12	8.716	931	940	949	rBV	205208	348971	3.90%	0.559%
13	9.181	1012	1019	1028	rBV	295908	489535	5.47%	0.784%
14	9.346	1042	1047	1051	rBV6	9399	14145	0.16%	0.023%
15	9.605	1083	1091	1096	rVB6	12855	27921	0.31%	0.045%
16	9.905	1136	1142	1150	rBV	200146	329303	3.68%	0.527%
17	10.446	1227	1234	1244	rBV	381978	664795	7.43%	1.065%
18	10.834	1292	1300	1309	rBV	2571192	4281161	47.84%	6.858%
19	10.969	1315	1323	1332	rBV	108652	208245	2.33%	0.334%
20	11.499	1406	1413	1416	rBV8	6809	15372	0.17%	0.025%
21	11.605	1427	1431	1440	rVB8	11566	22303	0.25%	0.036%
22	12.093	1508	1514	1518	rBV9	6069	12455	0.14%	0.020%
23	12.246	1533	1540	1544	rVB5	12903	20323	0.23%	0.033%
24	12.310	1544	1551	1555	rBV9	5356	11506	0.13%	0.018%
25	12.410	1564	1568	1573	rVB6	9401	15178	0.17%	0.024%
26	13.010	1666	1670	1674	rBV7	4990	10901	0.12%	0.017%
27	13.387	1730	1734	1738	rBV4	7114	10441	0.12%	0.017%
28	13.475	1744	1749	1755	rBV4	21618	31798	0.36%	0.051%
29	13.546	1757	1761	1764	rBV6	9922	12522	0.14%	0.020%
30	14.057	1840	1848	1857	rBV	872481	1276830	14.27%	2.045%
31	14.346	1891	1897	1904	rBV	773325	1107143	12.37%	1.773%
32	14.540	1925	1930	1936	rBV9	6065	11219	0.13%	0.018%
33	14.651	1941	1949	1957	rBV	4326216	6136052	68.57%	9.829%
34	14.834	1974	1980	1991	rBV4	31429	80791	0.90%	0.129%
35	15.057	2013	2018	2025	rVB10	15016	28370	0.32%	0.045%
36	15.457	2079	2086	2089	rBV9	6988	15942	0.18%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012813.D
 Acq On : 28 Nov 2022 13:02
 Operator : CG/JU
 Sample : N5710-09DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KY8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	15.640	2111	2117	2130	rBV	1397595	2079771	23.24%	3.331%
38	15.751	2130	2136	2144	rVV	177670	268261	3.00%	0.430%
39	15.887	2154	2159	2163	rVB7	7994	12962	0.14%	0.021%
40	16.004	2176	2179	2187	rBV2	20661	33395	0.37%	0.053%
41	16.787	2309	2312	2317	rVB7	9439	15673	0.18%	0.025%
42	17.192	2378	2381	2387	rVB4	11365	18146	0.20%	0.029%
43	17.404	2411	2417	2428	rBV	5402498	7625662	85.22%	12.215%
44	17.504	2428	2434	2444	rVV2	1545485	2231265	24.93%	3.574%
45	17.587	2445	2448	2454	rVB2	34500	51437	0.57%	0.082%
46	18.275	2560	2565	2574	rBV	209234	269368	3.01%	0.431%
47	18.692	2632	2636	2643	rBV5	47796	65049	0.73%	0.104%
48	19.310	2738	2741	2746	rBV5	18670	24003	0.27%	0.038%
49	19.504	2770	2774	2779	rBV	210380	268948	3.01%	0.431%
50	19.651	2797	2799	2806	rVB6	22150	24242	0.27%	0.039%
51	19.733	2807	2813	2824	rVV	2141874	2845811	31.80%	4.558%
52	21.186	3056	3060	3067	rBV2	162194	258918	2.89%	0.415%
53	21.492	3107	3112	3120	rBV	6736214	8948681	100.00%	14.334%
54	23.839	3505	3511	3518	rBV2	1169248	2398343	26.80%	3.842%
55	24.010	3532	3540	3556	rVB2	4263777	8912262	99.59%	14.276%




Sum of corrected areas: 62429383

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012813.D
Acq On : 28 Nov 2022 13:02
Operator : CG/JU
Sample : N5710-09DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY8DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

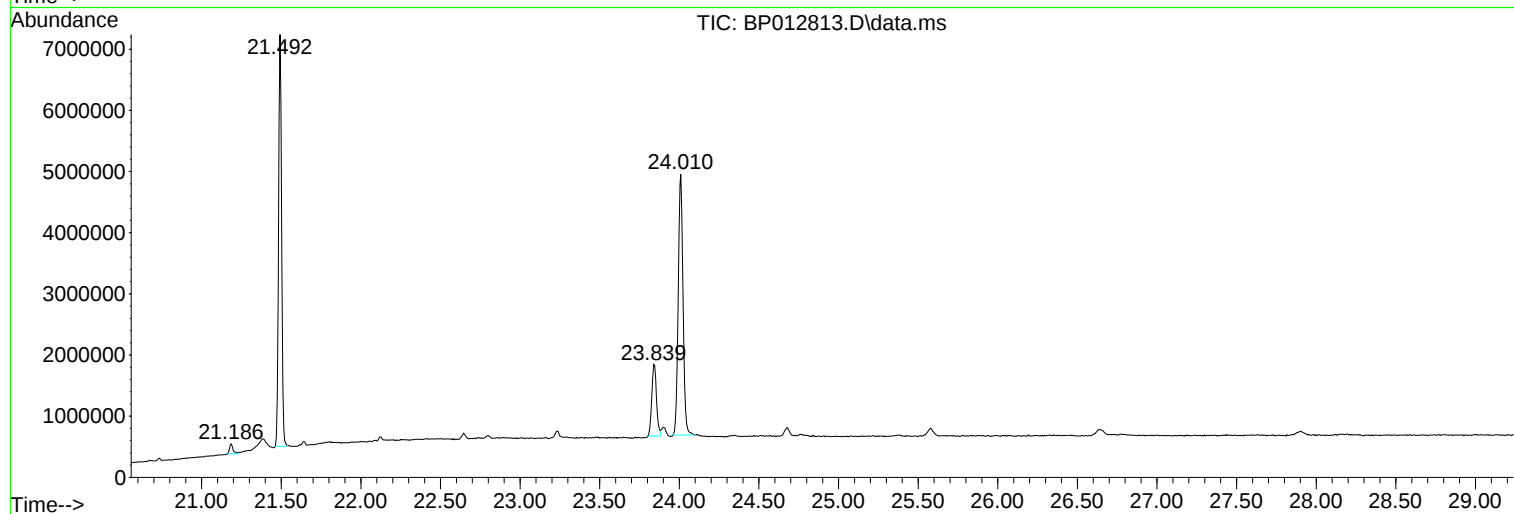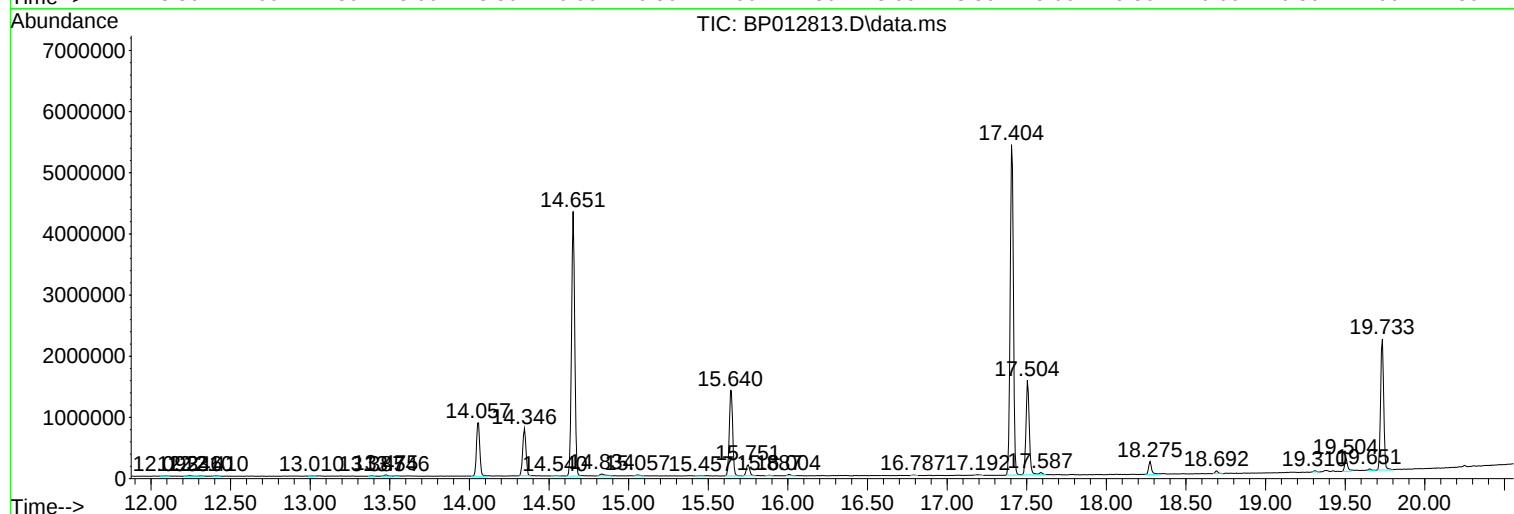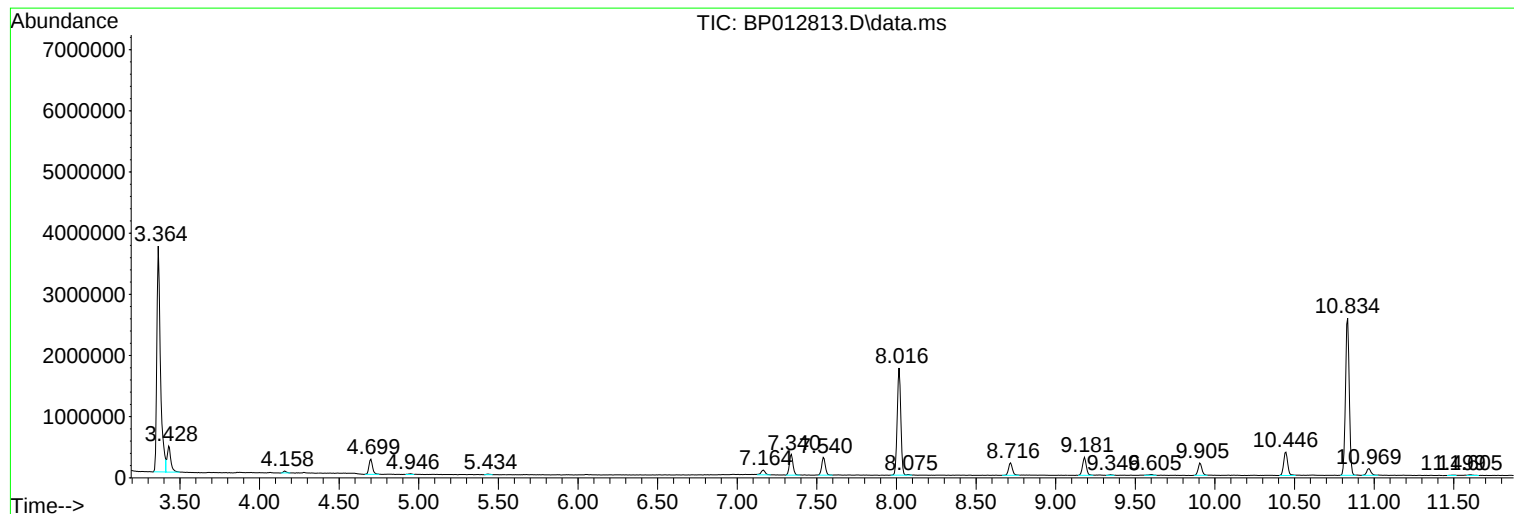

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012813.D
Acq On : 28 Nov 2022 13:02
Operator : CG/JU
Sample : N5710-09DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY8DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012813.D
Acq On : 28 Nov 2022 13:02
Operator : CG/JU
Sample : N5710-09DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY8DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc