

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012814.D
 Acq On : 28 Nov 2022 13:36
 Operator : CG/JU
 Sample : N5710-10DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KY9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012814.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	25	30	38	rBV	1092210	1675301	20.72%	3.501%
2	3.428	38	41	50	rVB	289059	399295	4.94%	0.835%
3	3.840	108	111	119	rBV2	41425	68098	0.84%	0.142%
4	4.158	162	165	169	rVB	19944	25468	0.31%	0.053%
5	4.699	250	257	269	rVV	5227619	8085594	100.00%	16.899%
6	4.793	269	273	278	rVB6	6273	13016	0.16%	0.027%
7	5.434	380	382	388	rVB4	10915	15141	0.19%	0.032%
8	7.164	671	676	681	rVB	53755	86724	1.07%	0.181%
9	7.340	700	706	716	rBV	209433	343452	4.25%	0.718%
10	7.540	734	740	747	rVB	171506	270752	3.35%	0.566%
11	7.705	761	768	771	rBV7	10559	19141	0.24%	0.040%
12	8.016	812	821	827	rBV	1164317	1843300	22.80%	3.853%
13	8.075	827	831	840	rVB	78573	119363	1.48%	0.249%
14	8.716	933	940	947	rBV	140459	234225	2.90%	0.490%
15	8.840	958	961	965	rVB7	7045	11176	0.14%	0.023%
16	9.181	1013	1019	1029	rBV	172480	297015	3.67%	0.621%
17	9.275	1033	1035	1038	rVV4	7537	8724	0.11%	0.018%
18	9.599	1087	1090	1095	rVB6	8063	13917	0.17%	0.029%
19	9.905	1132	1142	1150	rBV2	113096	206184	2.55%	0.431%
20	10.446	1227	1234	1241	rBV	234464	392281	4.85%	0.820%
21	10.834	1292	1300	1308	rBV	1690261	2842122	35.15%	5.940%
22	10.963	1316	1322	1332	rBV	162693	303440	3.75%	0.634%
23	11.487	1406	1411	1416	rVB8	6534	12343	0.15%	0.026%
24	11.604	1427	1431	1437	rVB8	5421	8225	0.10%	0.017%
25	12.240	1536	1539	1543	rVB5	5976	9057	0.11%	0.019%
26	12.410	1565	1568	1572	rBV5	7341	8465	0.10%	0.018%
27	12.593	1594	1599	1605	rVV9	5434	14653	0.18%	0.031%
28	13.475	1744	1749	1752	rBV4	7424	10492	0.13%	0.022%
29	13.540	1755	1760	1765	rVB7	7170	12233	0.15%	0.026%
30	14.057	1841	1848	1858	rBV	579189	831013	10.28%	1.737%
31	14.181	1864	1869	1872	rBV7	6166	8317	0.10%	0.017%
32	14.251	1875	1881	1890	rBV	143062	265091	3.28%	0.554%
33	14.345	1891	1897	1905	rVB	603711	881068	10.90%	1.841%
34	14.651	1941	1949	1964	rBV	2875091	4061733	50.23%	8.489%
35	14.828	1973	1979	1983	rBV3	31183	51797	0.64%	0.108%
36	15.051	2013	2017	2022	rVB7	8928	17487	0.22%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012814.D
 Acq On : 28 Nov 2022 13:36
 Operator : CG/JU
 Sample : N5710-10DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0KY9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	15.392	2070	2075	2078	rVB5	6446	9332	0.12%	0.020%
38	15.640	2111	2117	2128	rBV	906564	1365295	16.89%	2.854%
39	15.751	2130	2136	2142	rVV	120919	181248	2.24%	0.379%
40	16.010	2175	2180	2184	rBV5	9097	15692	0.19%	0.033%
41	17.187	2378	2380	2386	rVB4	7809	11129	0.14%	0.023%
42	17.404	2411	2417	2426	rBV	3515540	4990279	61.72%	10.430%
43	17.504	2428	2434	2443	rVV	1024577	1490713	18.44%	3.116%
44	17.581	2445	2447	2454	rVB6	22697	35291	0.44%	0.074%
45	17.692	2461	2466	2469	rBV6	6954	10824	0.13%	0.023%
46	18.275	2561	2565	2572	rBV2	54908	72175	0.89%	0.151%
47	18.692	2634	2636	2639	rVB3	12258	9179	0.11%	0.019%
48	19.375	2749	2752	2756	rBV3	16305	26684	0.33%	0.056%
49	19.504	2771	2774	2779	rBV4	39637	55700	0.69%	0.116%
50	19.733	2807	2813	2821	rBV	1442578	1927743	23.84%	4.029%
51	21.492	3107	3112	3122	rBV	4695503	6155051	76.12%	12.864%
52	23.839	3506	3511	3518	rBV2	827688	1606516	19.87%	3.358%
53	24.010	3533	3540	3554	rVB2	3100135	6416796	79.36%	13.412%




Sum of corrected areas: 47845350

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012814.D
Acq On : 28 Nov 2022 13:36
Operator : CG/JU
Sample : N5710-10DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

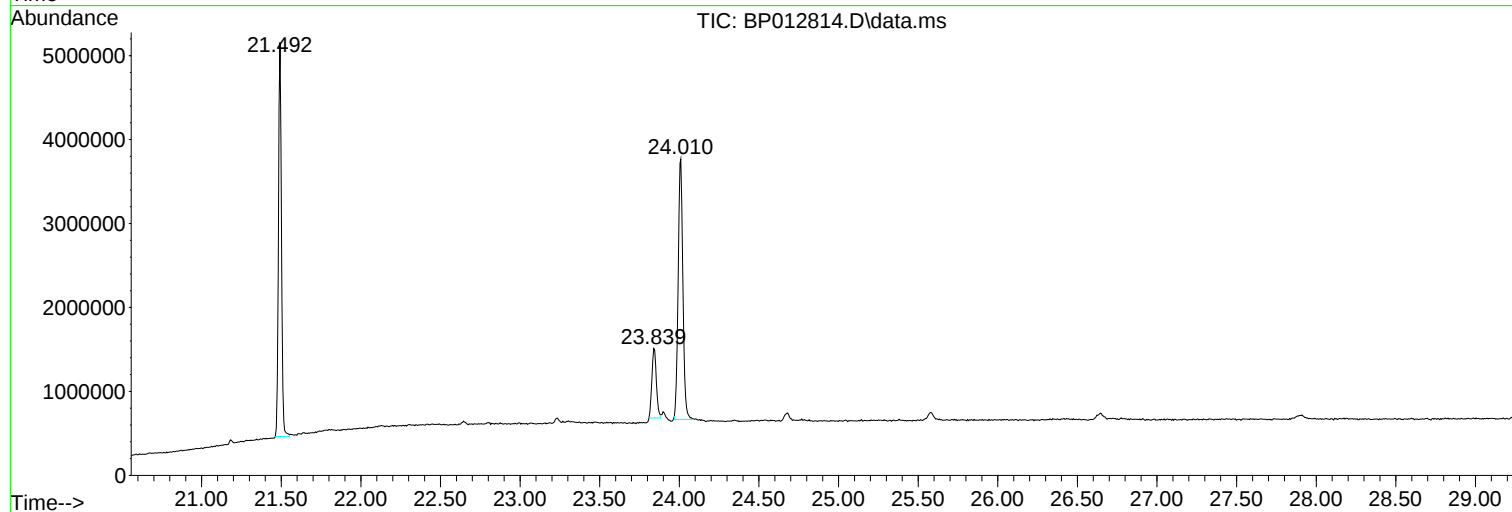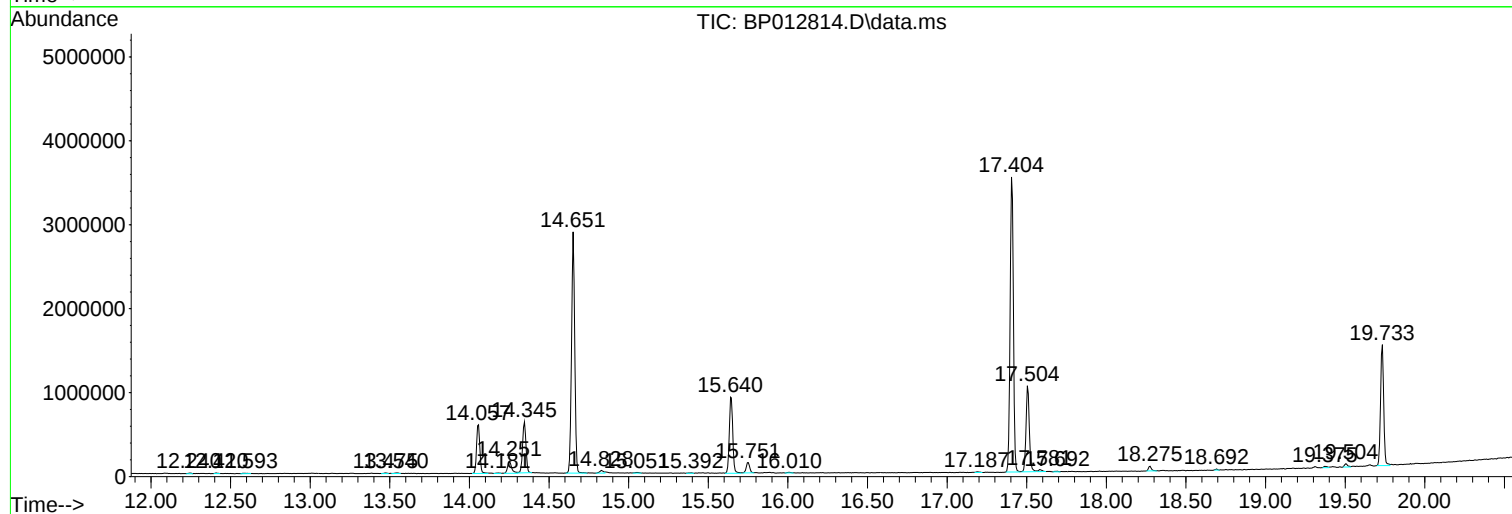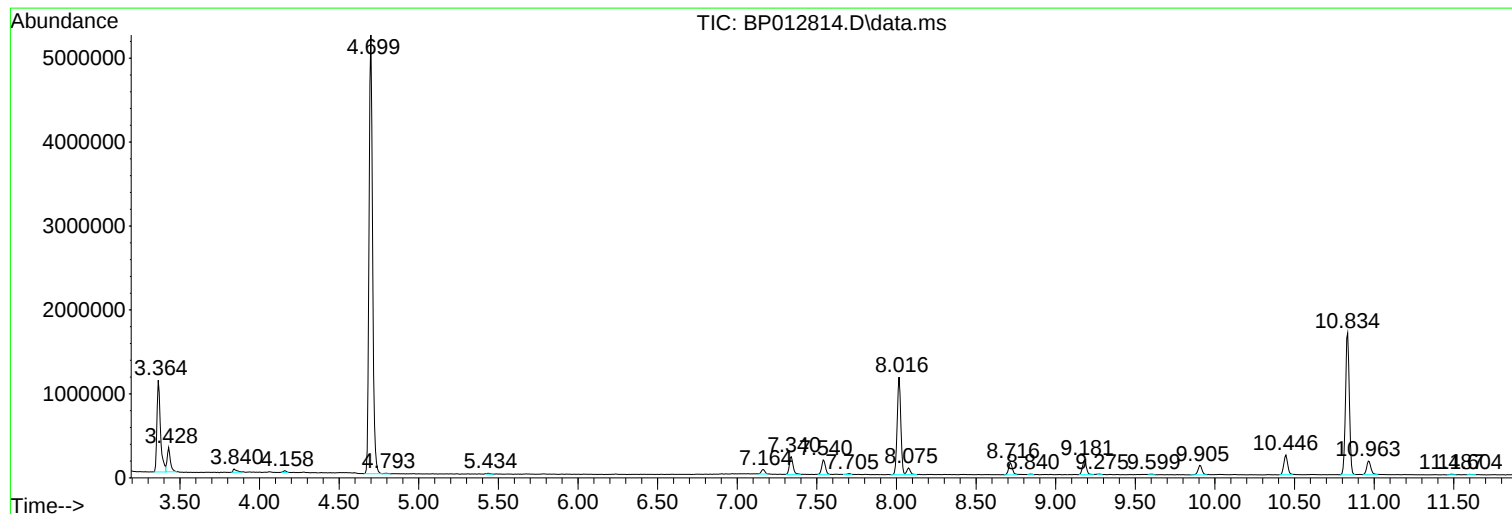

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012814.D
Acq On : 28 Nov 2022 13:36
Operator : CG/JU
Sample : N5710-10DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012814.D
Acq On : 28 Nov 2022 13:36
Operator : CG/JU
Sample : N5710-10DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KY9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc