

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012815.D
 Acq On : 28 Nov 2022 14:13
 Operator : CG/JU
 Sample : N5710-11DL 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COKZODL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012815.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	25	30	37	rBV	527101	834098	8.63%	1.499%
2	3.428	37	41	53	rVB	641638	953150	9.86%	1.713%
3	3.840	108	111	121	rBV	43122	78561	0.81%	0.141%
4	4.157	161	165	170	rBV	37248	52992	0.55%	0.095%
5	4.210	172	174	178	rVB4	9076	10574	0.11%	0.019%
6	4.281	182	186	190	rVB	18738	23812	0.25%	0.043%
7	4.699	251	257	267	rBV	1112645	1715606	17.75%	3.084%
8	5.357	366	369	375	rVB4	13778	22808	0.24%	0.041%
9	5.440	378	383	389	rVB	19268	29145	0.30%	0.052%
10	5.781	436	441	446	rBV6	10639	18022	0.19%	0.032%
11	6.246	514	520	525	rBV10	9877	20650	0.21%	0.037%
12	6.757	602	607	614	rVB4	17780	28337	0.29%	0.051%
13	6.904	627	632	637	rBV2	22006	35075	0.36%	0.063%
14	7.163	667	676	683	rVB	39514	75252	0.78%	0.135%
15	7.340	701	706	711	rBV	204095	326712	3.38%	0.587%
16	7.546	734	741	747	rBV	153953	252571	2.61%	0.454%
17	8.016	814	821	828	rBV	1949109	3084617	31.92%	5.545%
18	8.716	933	940	949	rBV	100666	175787	1.82%	0.316%
19	8.975	978	984	988	rBV9	5550	10447	0.11%	0.019%
20	9.181	1012	1019	1028	rBV	158980	270249	2.80%	0.486%
21	9.604	1087	1091	1098	rVB4	13371	22859	0.24%	0.041%
22	9.910	1135	1143	1155	rBV	109623	197964	2.05%	0.356%
23	10.445	1228	1234	1243	rBV	211797	364797	3.77%	0.656%
24	10.834	1292	1300	1308	rBV	2827831	4750158	49.15%	8.539%
25	10.969	1316	1323	1335	rBV	171398	316898	3.28%	0.570%
26	11.563	1420	1424	1430	rBV	21733	36388	0.38%	0.065%
27	12.098	1508	1515	1519	rBV7	9020	20767	0.21%	0.037%
28	13.481	1742	1750	1751	rBV8	14439	23331	0.24%	0.042%
29	13.510	1751	1755	1759	rVV	61044	94841	0.98%	0.170%
30	13.545	1759	1761	1767	rVB3	22850	29988	0.31%	0.054%
31	13.980	1830	1835	1840	rBV9	5708	10117	0.10%	0.018%
32	14.057	1842	1848	1854	rBV	532028	732945	7.58%	1.317%
33	14.257	1875	1882	1890	rBV	127656	246066	2.55%	0.442%
34	14.345	1891	1897	1905	rVB	545192	812654	8.41%	1.461%
35	14.651	1942	1949	1958	rBV	4499713	6716901	69.50%	12.074%
36	14.833	1976	1980	1986	rBV6	16619	26883	0.28%	0.048%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012815.D
 Acq On : 28 Nov 2022 14:13
 Operator : CG/JU
 Sample : N5710-11DL 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 COKZ0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	15.051	2011	2017	2023	rBV6	10242	18423	0.19%	0.033%
38	15.645	2112	2118	2130	rBV	866257	1227033	12.70%	2.206%
39	15.751	2130	2136	2144	rVV	106603	158150	1.64%	0.284%
40	16.004	2177	2179	2184	rBV5	7860	11319	0.12%	0.020%
41	17.192	2378	2381	2384	rBV3	9196	9668	0.10%	0.017%
42	17.410	2411	2418	2428	rBV	6136551	8333214	86.23%	14.979%
43	17.510	2429	2435	2443	rVV	849133	1281775	13.26%	2.304%
44	17.592	2447	2449	2456	rVB7	17567	25605	0.26%	0.046%
45	18.274	2561	2565	2575	rBV	120683	160759	1.66%	0.289%
46	18.357	2575	2579	2583	rVV5	9023	14031	0.15%	0.025%
47	18.692	2634	2636	2639	rVB4	16532	14358	0.15%	0.026%
48	19.510	2771	2775	2784	rBV2	127233	182653	1.89%	0.328%
49	19.733	2808	2813	2824	rBV	1236311	1598484	16.54%	2.873%
50	21.498	3107	3113	3122	rBV	6962219	9664146	100.00%	17.372%
51	23.845	3507	3512	3518	rBV2	535916	1024075	10.60%	1.841%
52	24.009	3533	3540	3560	rVB2	4628472	9486188	98.16%	17.052%




Sum of corrected areas: 55631903

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012815.D
Acq On : 28 Nov 2022 14:13
Operator : CG/JU
Sample : N5710-11DL 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KZ0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

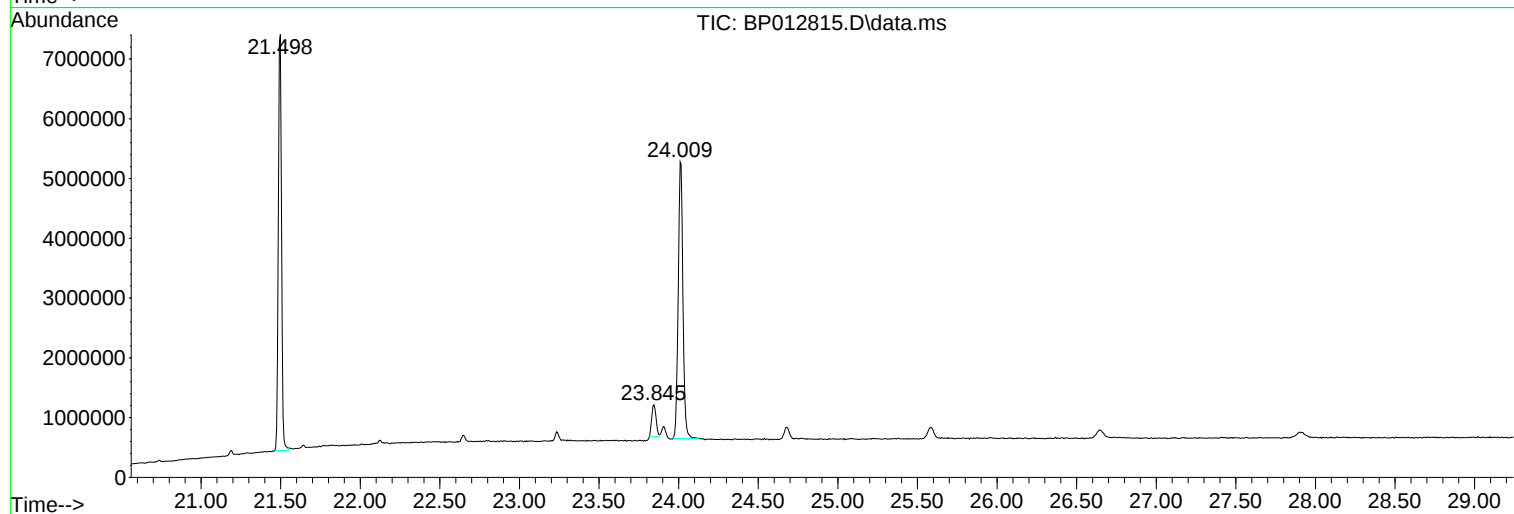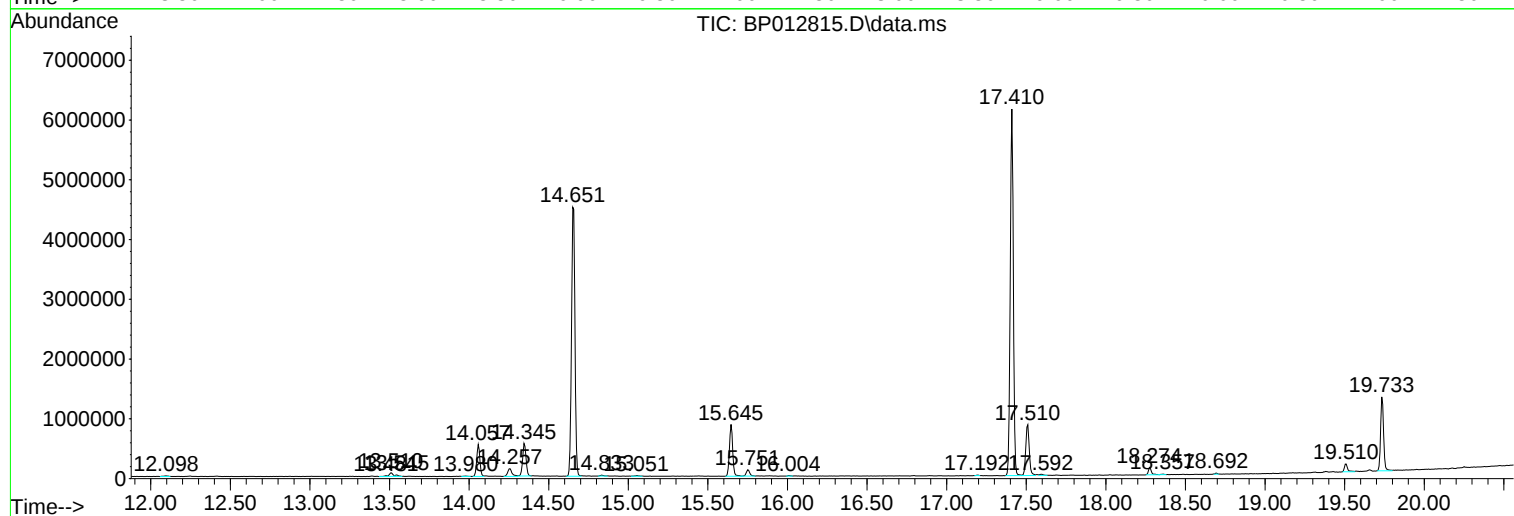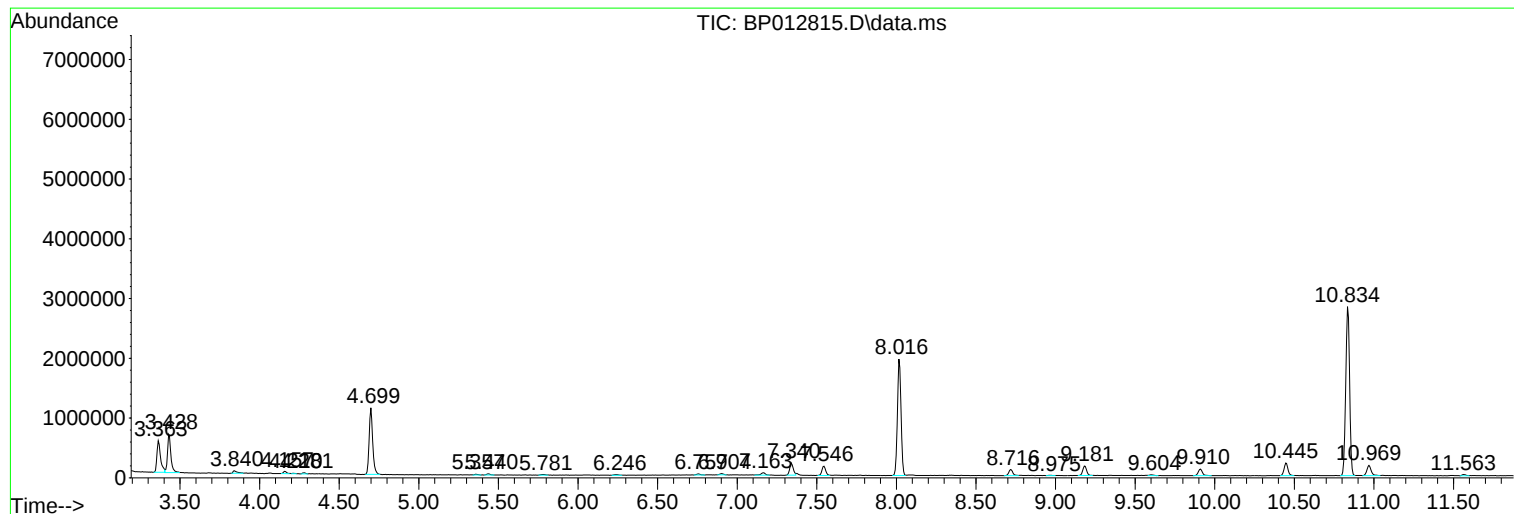

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012815.D
Acq On : 28 Nov 2022 14:13
Operator : CG/JU
Sample : N5710-11DL 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KZ0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012815.D
Acq On : 28 Nov 2022 14:13
Operator : CG/JU
Sample : N5710-11DL 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0KZ0DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
