

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012822.D
 Acq On : 28 Nov 2022 18:13
 Operator : CG/JU
 Sample : N5666-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012822.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	41	rBV	130100	164322	1.35%	0.138%
2	3.828	106	109	121	rBV	235380	390646	3.20%	0.328%
3	4.058	145	148	155	rVB	33486	52985	0.43%	0.044%
4	4.158	161	165	171	rVB	39591	56914	0.47%	0.048%
5	4.381	201	203	210	rVB6	10940	13077	0.11%	0.011%
6	4.493	218	222	229	rVB3	20922	30086	0.25%	0.025%
7	4.611	239	242	249	rVB2	26818	47367	0.39%	0.040%
8	6.405	542	547	554	rVB6	9778	17313	0.14%	0.015%
9	7.164	668	676	684	rVB	607513	957229	7.85%	0.804%
10	7.340	699	706	714	rBV	2138246	3296446	27.03%	2.768%
11	7.540	732	740	750	rBV	1982906	3111141	25.51%	2.612%
12	7.622	750	754	763	rVB3	22727	52052	0.43%	0.044%
13	8.016	813	821	828	rBV	2014569	3121508	25.60%	2.621%
14	8.075	828	831	835	rVB3	15600	21292	0.17%	0.018%
15	8.716	931	940	950	rBV	1569931	2486209	20.39%	2.088%
16	9.181	1009	1019	1032	rBV	2310132	3715623	30.47%	3.120%
17	9.605	1085	1091	1097	rVB	38435	67102	0.55%	0.056%
18	9.905	1134	1142	1155	rBV	1760359	2872350	23.55%	2.412%
19	10.028	1158	1163	1167	rVB8	7953	16679	0.14%	0.014%
20	10.116	1174	1178	1184	rVB9	8633	16136	0.13%	0.014%
21	10.346	1212	1217	1225	rVB10	10720	19859	0.16%	0.017%
22	10.446	1225	1234	1249	rBV	2771856	4685431	38.42%	3.934%
23	10.834	1290	1300	1308	rBV	2919702	4867225	39.91%	4.087%
24	10.963	1317	1322	1332	rBV2	85666	162792	1.33%	0.137%
25	11.487	1407	1411	1416	rBV5	7456	16824	0.14%	0.014%
26	11.604	1426	1431	1436	rBV8	17184	28062	0.23%	0.024%
27	11.857	1466	1474	1478	rBV8	15472	26942	0.22%	0.023%
28	12.093	1506	1514	1521	rBV9	9765	23080	0.19%	0.019%
29	12.240	1533	1539	1547	rVB	43667	69986	0.57%	0.059%
30	12.410	1561	1568	1573	rBV	52952	85774	0.70%	0.072%
31	12.675	1608	1613	1619	rVB8	10747	19320	0.16%	0.016%
32	12.875	1641	1647	1650	rBV5	12416	18988	0.16%	0.016%
33	13.051	1673	1677	1683	rVB6	13314	25568	0.21%	0.021%
34	13.134	1686	1691	1696	rBV5	13346	21629	0.18%	0.018%
35	13.187	1696	1700	1706	rVV6	15396	26236	0.22%	0.022%
36	13.387	1730	1734	1738	rBV7	11156	14247	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012822.D
 Acq On : 28 Nov 2022 18:13
 Operator : CG/JU
 Sample : N5666-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	13.475	1744	1749	1756	rVV	67480	93066	0.76%	0.078%
38	13.546	1756	1761	1768	rVB3	32503	58172	0.48%	0.049%
39	13.628	1768	1775	1780	rVB7	14064	29940	0.25%	0.025%
40	14.057	1841	1848	1857	rBV	5582120	7700204	63.14%	6.466%

41	14.122	1857	1859	1864	rVV6	14432	22979	0.19%	0.019%
42	14.169	1864	1867	1873	rVB8	9678	14690	0.12%	0.012%
43	14.287	1883	1887	1890	rBV4	23014	29988	0.25%	0.025%
44	14.346	1890	1897	1910	rVB	5989553	8549624	70.11%	7.179%
45	14.540	1926	1930	1936	rVB3	18501	29429	0.24%	0.025%

46	14.651	1940	1949	1957	rBV	4429724	6583704	53.99%	5.528%
47	14.828	1972	1979	1990	rBV	403296	657395	5.39%	0.552%
48	15.051	2013	2017	2022	rVB7	22099	36807	0.30%	0.031%
49	15.281	2051	2056	2062	rBV9	14732	24671	0.20%	0.021%
50	15.445	2079	2084	2088	rVV	21862	31524	0.26%	0.026%

51	15.493	2088	2092	2098	rVB6	14658	19493	0.16%	0.016%
52	15.645	2111	2118	2128	rBV	8414969	12175043	99.84%	10.223%
53	15.751	2130	2136	2148	rVV	2147743	2803165	22.99%	2.354%
54	15.881	2152	2158	2165	rVB2	41280	72539	0.59%	0.061%
55	16.004	2173	2179	2185	rBV	150072	211059	1.73%	0.177%

56	16.428	2248	2251	2256	rVB7	14055	19307	0.16%	0.016%
57	16.787	2307	2312	2320	rVB7	14954	26811	0.22%	0.023%
58	16.881	2325	2328	2332	rVV6	8932	16025	0.13%	0.013%
59	16.934	2335	2337	2342	rVB5	12028	13409	0.11%	0.011%
60	17.081	2359	2362	2366	rBV5	10707	17183	0.14%	0.014%

61	17.198	2378	2382	2388	rVB5	17025	32016	0.26%	0.027%
62	17.404	2410	2417	2427	rBV	4902783	6777405	55.58%	5.691%
63	17.504	2427	2434	2446	rVV	8758201	12194552	100.00%	10.240%
64	17.587	2446	2448	2453	rVB3	37353	49208	0.40%	0.041%
65	17.687	2462	2465	2468	rBV2	9603	12349	0.10%	0.010%

66	18.063	2525	2529	2534	rVB4	41146	54684	0.45%	0.046%
67	18.275	2560	2565	2575	rBV	242358	340225	2.79%	0.286%
68	18.692	2632	2636	2639	rBV5	25415	36295	0.30%	0.030%
69	18.751	2643	2646	2650	rVB4	24990	30107	0.25%	0.025%
70	19.310	2737	2741	2746	rBV3	99619	133110	1.09%	0.112%

71	19.375	2747	2752	2758	rBV	94542	158196	1.30%	0.133%
72	19.504	2770	2774	2780	rBV2	100050	130959	1.07%	0.110%
73	19.733	2807	2813	2824	rBV	9036208	11812161	96.86%	9.919%
74	21.180	3056	3059	3063	rBV	138244	181067	1.48%	0.152%
75	21.492	3107	3112	3126	rBV	3119484	4225846	34.65%	3.548%

76	23.839	3504	3511	3529	rVB2	4146395	8688282	71.25%	7.295%
----	--------	------	------	------	------	---------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012822.D
Acq On : 28 Nov 2022 18:13
Operator : CG/JU
Sample : N5666-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB32

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION

77	24.004	3532	3539	3555	rVB2	2006455	4380909	35.93%	3.679%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 119092038

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012822.D
Acq On : 28 Nov 2022 18:13
Operator : CG/JU
Sample : N5666-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

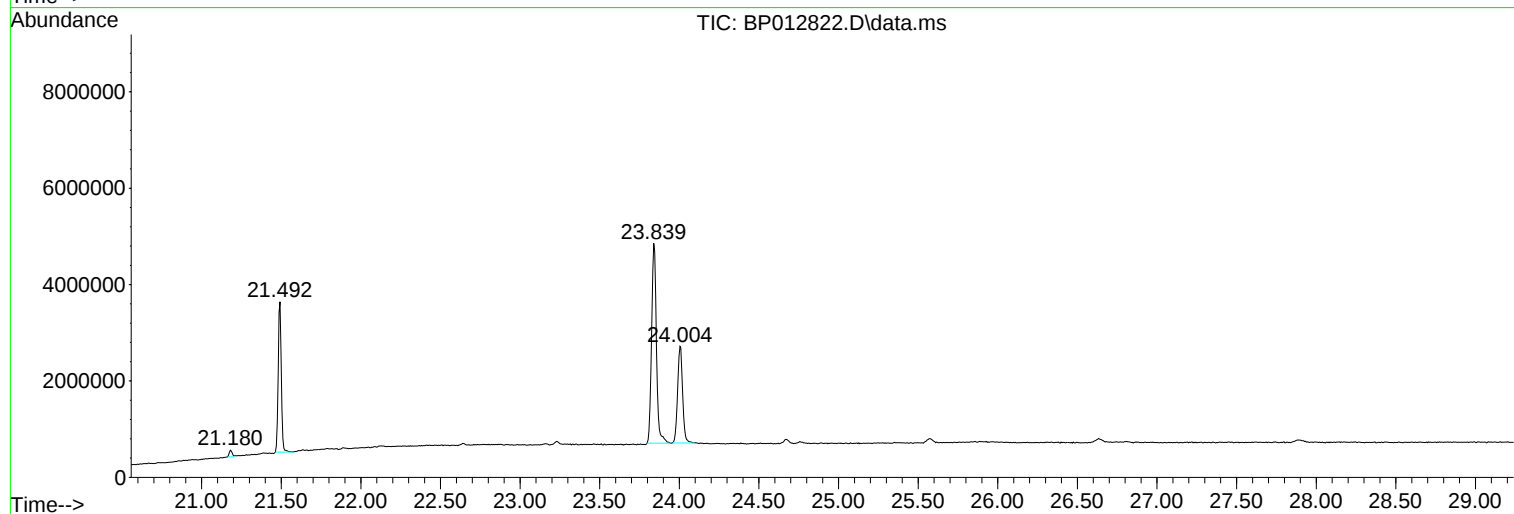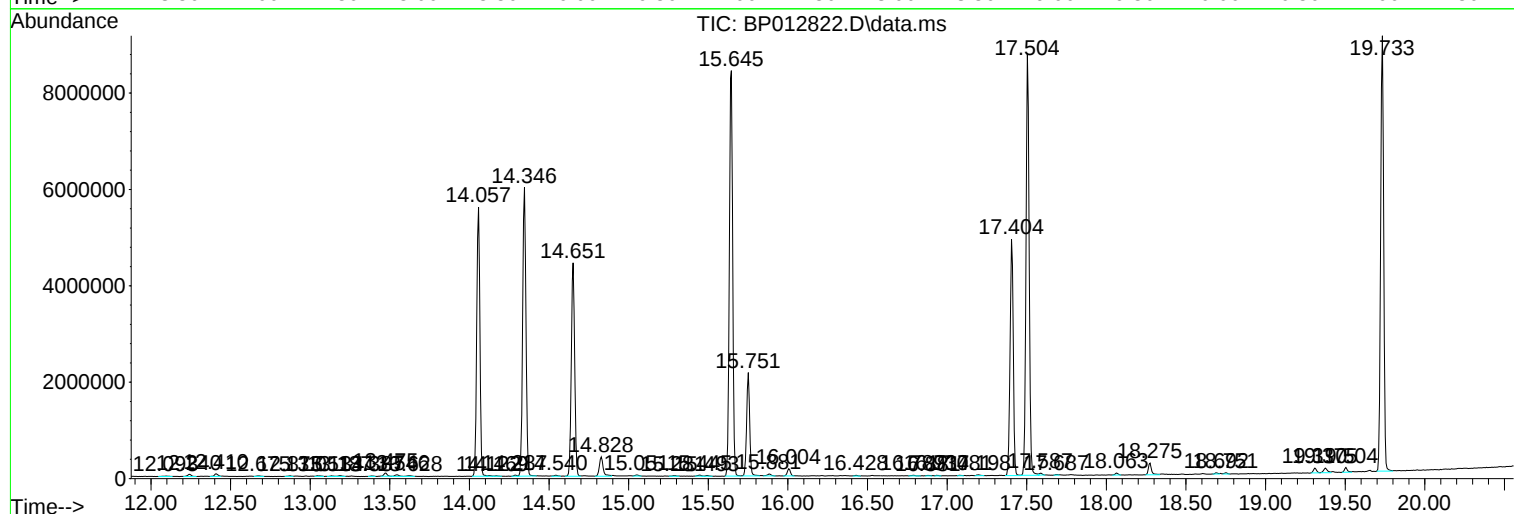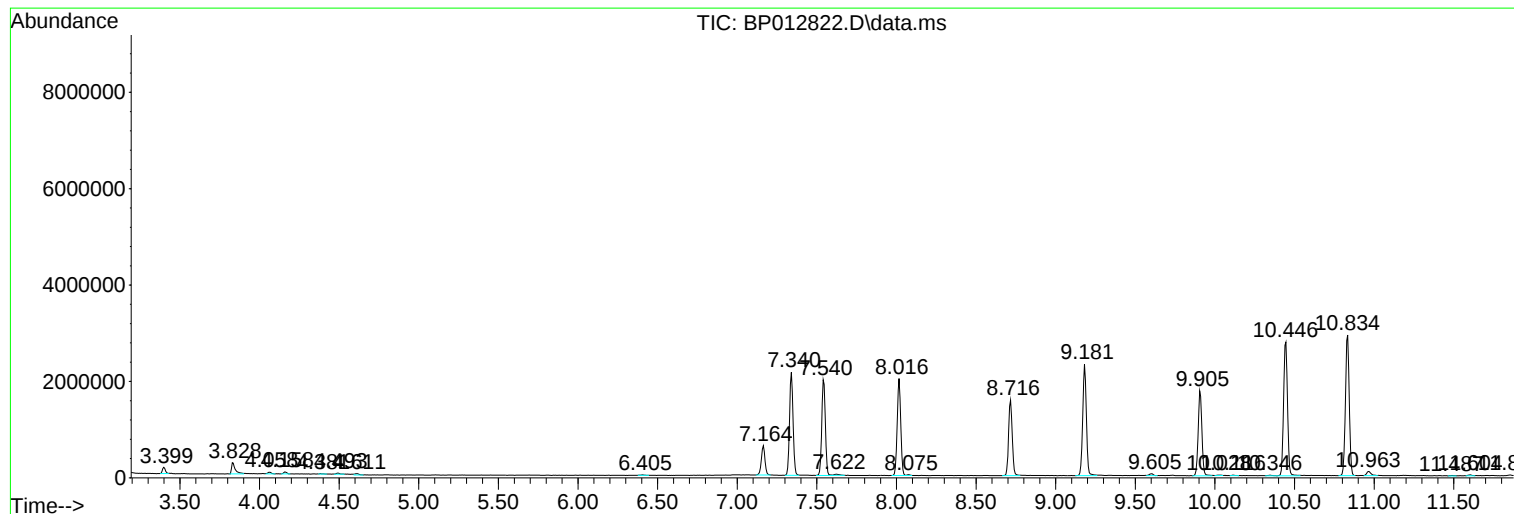

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012822.D
Acq On : 28 Nov 2022 18:13
Operator : CG/JU
Sample : N5666-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012822.D
Acq On : 28 Nov 2022 18:13
Operator : CG/JU
Sample : N5666-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB32

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc