

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012828.D
 Acq On : 28 Nov 2022 22:13
 Operator : CG/JU
 Sample : PB149261BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK261

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012828.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	48	rVB	161436	220088	1.88%	0.165%
2	3.822	105	108	126	rBV	1108555	1697662	14.53%	1.270%
3	4.158	161	165	170	rVB	44072	58964	0.50%	0.044%
4	7.163	667	676	688	rBV	2205065	3404968	29.13%	2.547%
5	7.340	699	706	717	rVB	1912876	2992650	25.61%	2.239%
6	7.540	733	740	748	rBV	2255978	3485666	29.82%	2.608%
7	8.016	813	821	829	rBV	2328706	3682883	31.51%	2.755%
8	8.716	932	940	949	rBV	2817742	4427596	37.88%	3.312%
9	9.181	1011	1019	1031	rBV	2094602	3365305	28.79%	2.518%
10	9.904	1134	1142	1154	rBV	1698516	2740245	23.45%	2.050%
11	10.440	1226	1233	1246	rBV	2802066	4648100	39.77%	3.477%
12	10.834	1288	1300	1310	rBV	3409092	5755812	49.25%	4.306%
13	10.963	1314	1322	1335	rBV	2083910	3561524	30.47%	2.664%
14	12.410	1560	1568	1575	rBV2	52845	94010	0.80%	0.070%
15	13.381	1730	1733	1739	rBV6	7023	11770	0.10%	0.009%
16	13.540	1756	1760	1765	rVB5	10552	16958	0.15%	0.013%
17	13.616	1769	1773	1780	rVB4	10326	17773	0.15%	0.013%
18	14.051	1840	1847	1860	rBV	5150675	7313448	62.58%	5.471%
19	14.345	1889	1897	1908	rBV	6035824	8908480	76.22%	6.664%
20	14.651	1941	1949	1956	rBV	5521330	8213797	70.28%	6.145%
21	14.828	1972	1979	1996	rBV	2004552	2878939	24.63%	2.154%
22	15.057	2013	2018	2023	rVB9	12731	21143	0.18%	0.016%
23	15.639	2110	2117	2129	rBV	7747576	11295504	96.65%	8.450%
24	15.751	2129	2136	2145	rBV	1885762	2522011	21.58%	1.887%
25	15.881	2153	2158	2165	rVB3	34053	60325	0.52%	0.045%
26	16.210	2211	2214	2218	rVB5	9482	13231	0.11%	0.010%
27	16.428	2248	2251	2258	rVB8	11262	14940	0.13%	0.011%
28	17.075	2359	2361	2366	rVB6	9750	12510	0.11%	0.009%
29	17.186	2376	2380	2386	rBV3	12720	19976	0.17%	0.015%
30	17.404	2410	2417	2427	rBV	6558229	9206548	78.77%	6.887%
31	17.504	2427	2434	2449	rVV	8352282	11566087	98.96%	8.653%
32	18.063	2526	2529	2533	rBV6	10667	15407	0.13%	0.012%
33	18.269	2561	2564	2572	rVB9	14701	24957	0.21%	0.019%
34	19.310	2736	2741	2746	rBV	85701	129805	1.11%	0.097%
35	19.375	2748	2752	2758	rVV	82593	112189	0.96%	0.084%
36	19.733	2806	2813	2828	rBV	8648278	11687410	100.00%	8.743%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012828.D
Acq On : 28 Nov 2022 22:13
Operator : CG/JU
Sample : PB149261BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION

37	21.486	3106	3111	3123	rBV	4861176	6571514	56.23%	4.916%
38	23.839	3503	3511	3518	rBV	3456565	7196641	61.58%	5.384%
39	23.998	3531	3538	3551	rBV2	2725181	5704357	48.81%	4.267%


Sum of corrected areas: 133671193

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012828.D
Acq On : 28 Nov 2022 22:13
Operator : CG/JU
Sample : PB149261BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

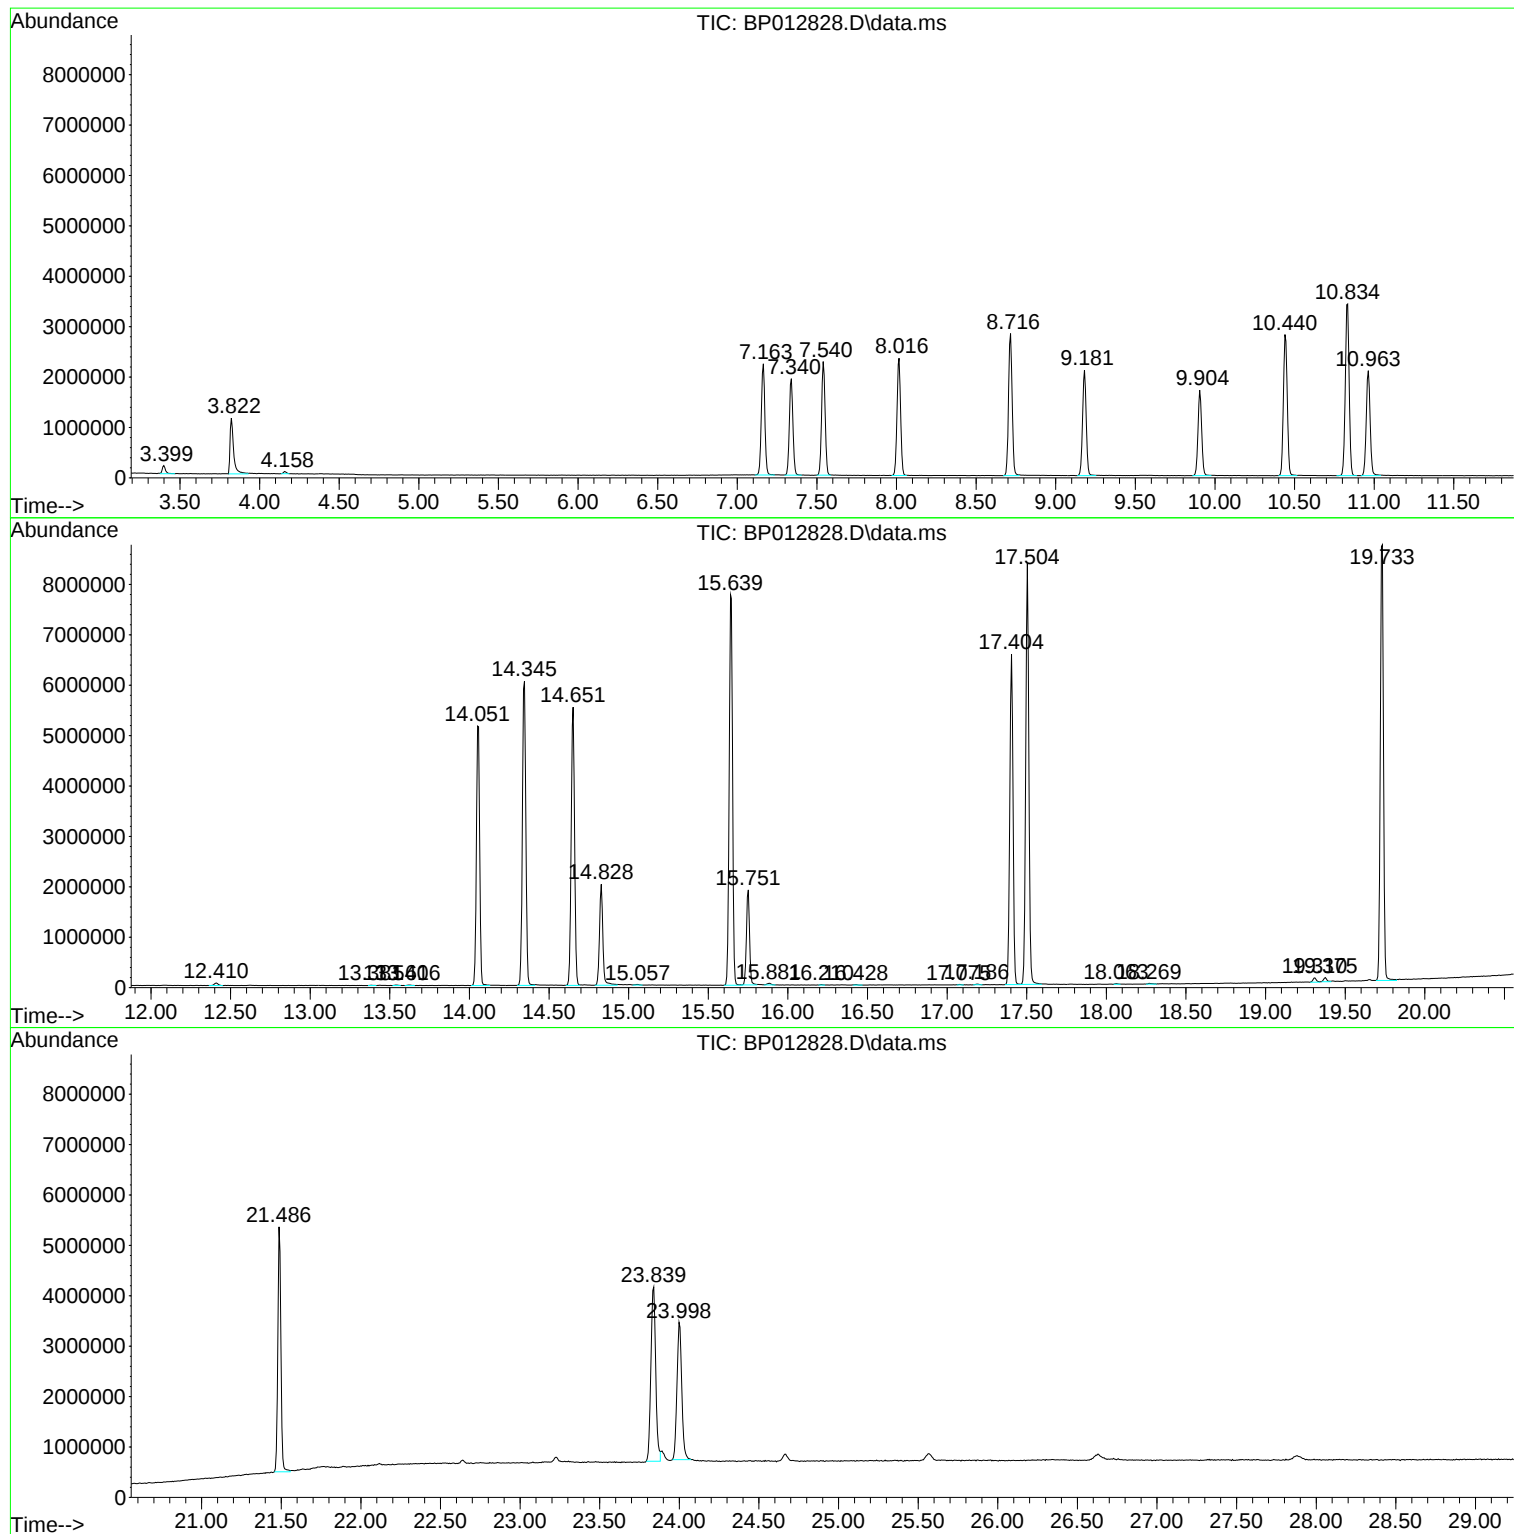

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012828.D
Acq On : 28 Nov 2022 22:13
Operator : CG/JU
Sample : PB149261BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012828.D
Acq On : 28 Nov 2022 22:13
Operator : CG/JU
Sample : PB149261BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK261

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc