

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012829.D
 Acq On : 28 Nov 2022 22:47
 Operator : CG/JU
 Sample : PB149199BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK199

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012829.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	46	rVB	203374	266215	2.32%	0.187%
2	3.822	104	108	126	rBV	2361880	3502828	30.51%	2.460%
3	4.158	162	165	171	rVB	49999	66072	0.58%	0.046%
4	7.163	669	676	690	rBV	2682721	4189182	36.49%	2.942%
5	7.340	699	706	716	rVB	2367958	3671773	31.98%	2.579%
6	7.540	733	740	755	rBV	2794096	4315167	37.59%	3.031%
7	8.016	812	821	829	rBV	2617349	4174824	36.37%	2.932%
8	8.716	932	940	955	rBV	3303049	5312184	46.27%	3.731%
9	9.181	1011	1019	1030	rBV	2516734	4036299	35.16%	2.835%
10	9.904	1131	1142	1153	rBV	2014614	3287211	28.63%	2.309%
11	10.440	1224	1233	1244	rBV	3347975	5466721	47.62%	3.839%
12	10.828	1292	1299	1312	rVB	3732148	6376300	55.54%	4.478%
13	10.963	1314	1322	1337	rBV	3249312	5464280	47.60%	3.838%
14	12.410	1562	1568	1575	rBV2	58189	93164	0.81%	0.065%
15	13.539	1756	1760	1767	rVB2	34068	48411	0.42%	0.034%
16	13.628	1771	1775	1778	rVB6	10927	17602	0.15%	0.012%
17	14.057	1839	1848	1862	rBV	5310722	7477885	65.14%	5.252%
18	14.345	1887	1897	1906	rBV	6591612	9578543	83.44%	6.727%
19	14.651	1942	1949	1958	rBV	5601282	8261266	71.96%	5.802%
20	14.828	1972	1979	1998	rBV	1830215	2712738	23.63%	1.905%
21	15.057	2014	2018	2023	rVB6	13220	19796	0.17%	0.014%
22	15.639	2110	2117	2129	rBV	7739405	11480027	100.00%	8.062%
23	15.751	2129	2136	2149	rVV	1671725	2247216	19.58%	1.578%
24	15.881	2154	2158	2163	rVB2	34751	51426	0.45%	0.036%
25	16.428	2248	2251	2256	rVB7	8466	13367	0.12%	0.009%
26	17.080	2358	2362	2366	rBV6	10445	12952	0.11%	0.009%
27	17.404	2410	2417	2426	rBV	5457420	7858422	68.45%	5.519%
28	17.504	2426	2434	2447	rBV	7388992	10511803	91.57%	7.382%
29	19.310	2737	2741	2745	rBV2	67849	86247	0.75%	0.061%
30	19.374	2748	2752	2756	rBV2	58134	82811	0.72%	0.058%
31	19.727	2807	2812	2825	rBV	7265327	9644620	84.01%	6.773%
32	21.486	3106	3111	3125	rBV	4318094	5830804	50.79%	4.095%
33	23.833	3503	3510	3529	rBV2	4507797	9500962	82.76%	6.672%
34	23.998	3531	3538	3551	rVV2	3267499	6730811	58.63%	4.727%

Sum of corrected areas: 142389929




Instrument :
BNA_P
ClientSampleId :
SBLK199

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012829.D
Acq On : 28 Nov 2022 22:47
Operator : CG/JU
Sample : PB149199BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK199

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

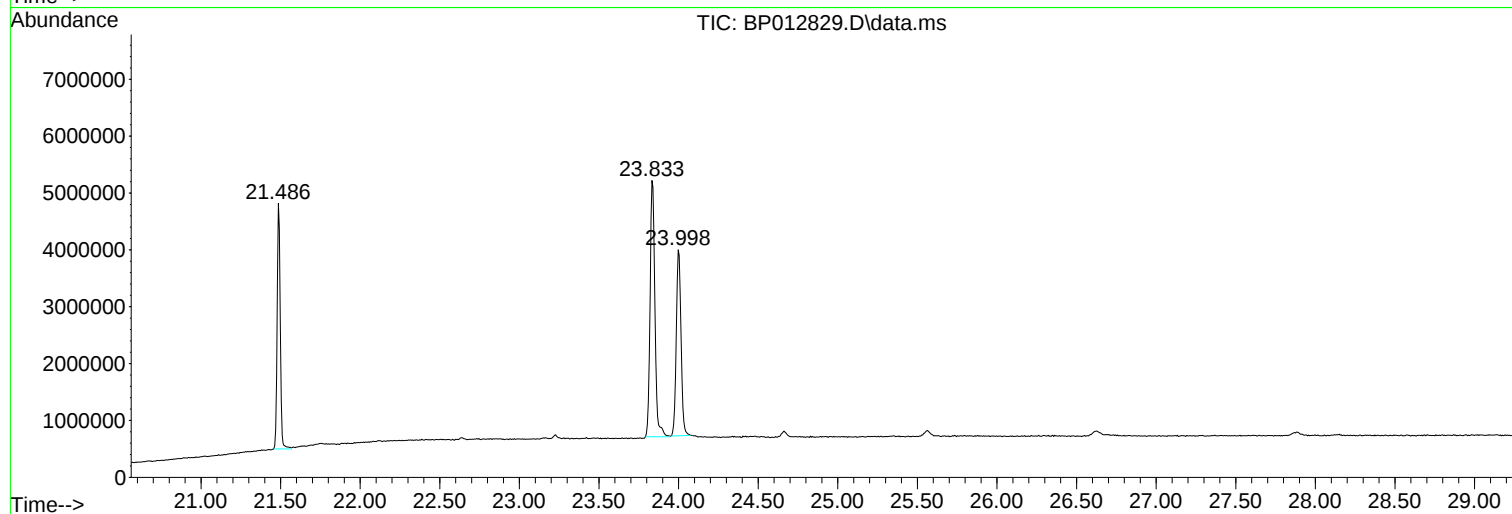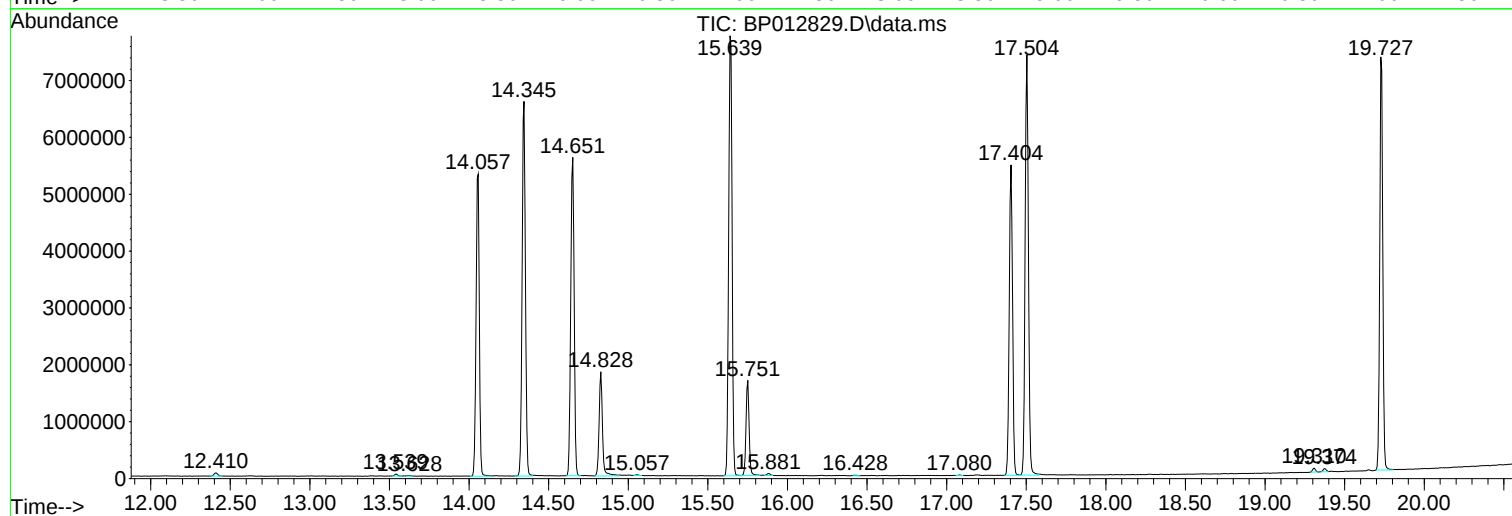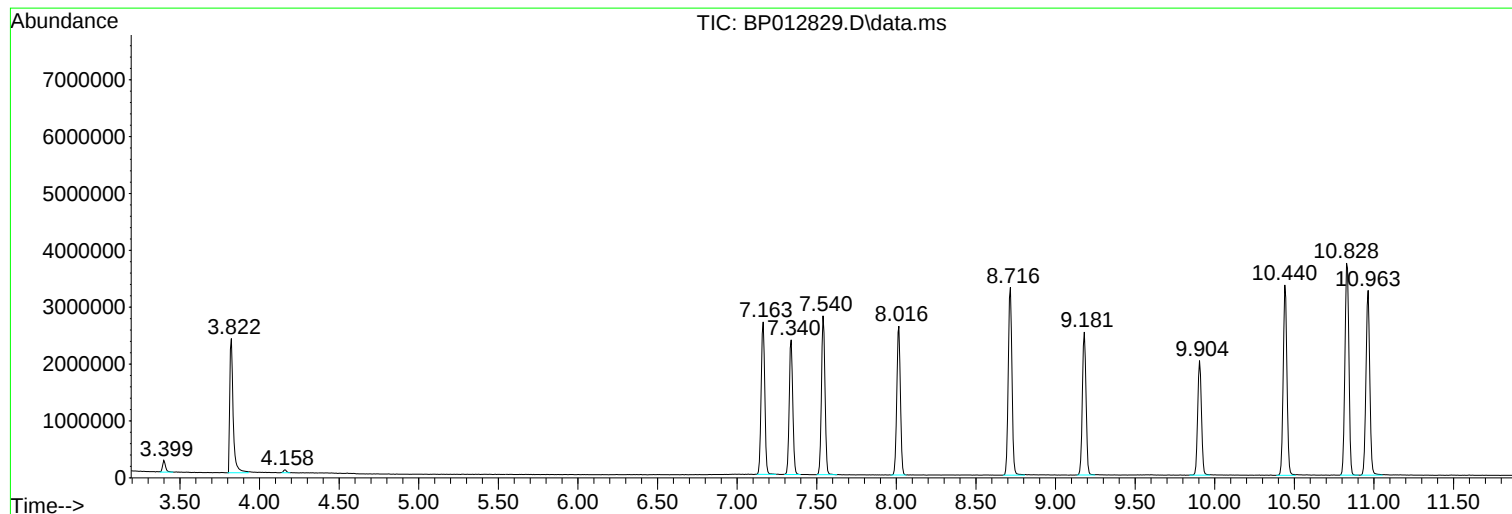

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012829.D
Acq On : 28 Nov 2022 22:47
Operator : CG/JU
Sample : PB149199BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK199

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012829.D
Acq On : 28 Nov 2022 22:47
Operator : CG/JU
Sample : PB149199BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK199

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc