

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012830.D
 Acq On : 28 Nov 2022 23:21
 Operator : CG/JU
 Sample : PB149200BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK200

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012830.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	45	rVB	177168	229267	1.83%	0.157%
2	3.822	104	108	125	rBV	2038989	3101654	24.71%	2.124%
3	4.158	161	165	172	rVB	46680	67076	0.53%	0.046%
4	7.163	669	676	688	rBV	2393003	3689830	29.39%	2.527%
5	7.340	699	706	715	rVB	2095866	3249969	25.89%	2.226%
6	7.540	733	740	748	rBV	2456446	3757100	29.93%	2.573%
7	8.016	810	821	830	rBV	2470075	3954271	31.50%	2.708%
8	8.716	931	940	953	rBV	2953435	4782623	38.10%	3.276%
9	9.181	1011	1019	1031	rBV	2258030	3620694	28.84%	2.480%
10	9.904	1134	1142	1152	rBV	1835036	2924768	23.30%	2.003%
11	10.440	1225	1233	1247	rBV	3029404	4971545	39.60%	3.405%
12	10.828	1291	1299	1308	rBV	3608286	6184534	49.26%	4.236%
13	10.963	1313	1322	1336	rBV	3007016	5109415	40.70%	3.499%
14	12.410	1561	1568	1576	rBV2	52474	89948	0.72%	0.062%
15	12.628	1600	1605	1610	rVB7	7238	13378	0.11%	0.009%
16	13.387	1730	1734	1739	rVB7	9731	15244	0.12%	0.010%
17	13.545	1753	1761	1767	rBV	63328	107621	0.86%	0.074%
18	13.622	1770	1774	1781	rVB3	12721	21731	0.17%	0.015%
19	14.057	1840	1848	1859	rBV	5549332	7783843	62.00%	5.331%
20	14.345	1889	1897	1910	rBV	6576079	9514161	75.78%	6.516%
21	14.651	1941	1949	1959	rBV	6074333	8838840	70.41%	6.054%
22	14.828	1972	1979	2000	rBV	2139913	3103398	24.72%	2.126%
23	15.057	2013	2018	2024	rVB9	13530	19559	0.16%	0.013%
24	15.639	2110	2117	2129	rBV	8290843	12051590	96.00%	8.254%
25	15.751	2129	2136	2152	rVV	1992900	2704106	21.54%	1.852%
26	15.881	2154	2158	2164	rVB2	37556	61326	0.49%	0.042%
27	17.080	2358	2362	2366	rVB7	9878	13560	0.11%	0.009%
28	17.186	2376	2380	2385	rBV2	13099	21310	0.17%	0.015%
29	17.404	2409	2417	2427	rBV	6879152	9827782	78.28%	6.731%
30	17.504	2427	2434	2452	rVV	8914216	12366651	98.51%	8.470%
31	19.304	2736	2740	2746	rBV	86375	125615	1.00%	0.086%
32	19.374	2748	2752	2757	rVB	81870	108980	0.87%	0.075%
33	19.727	2806	2812	2822	rBV	9298550	12554228	100.00%	8.599%
34	21.486	3106	3111	3125	rBV	5161391	6957098	55.42%	4.765%
35	23.839	3503	3511	3528	rBV	3866964	7973610	63.51%	5.461%
36	23.998	3532	3538	3558	rVB2	2831319	6088122	48.49%	4.170%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012830.D
Acq On : 28 Nov 2022 23:21
Operator : CG/JU
Sample : PB149200BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK200

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 146004447

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012830.D
Acq On : 28 Nov 2022 23:21
Operator : CG/JU
Sample : PB149200BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK200

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

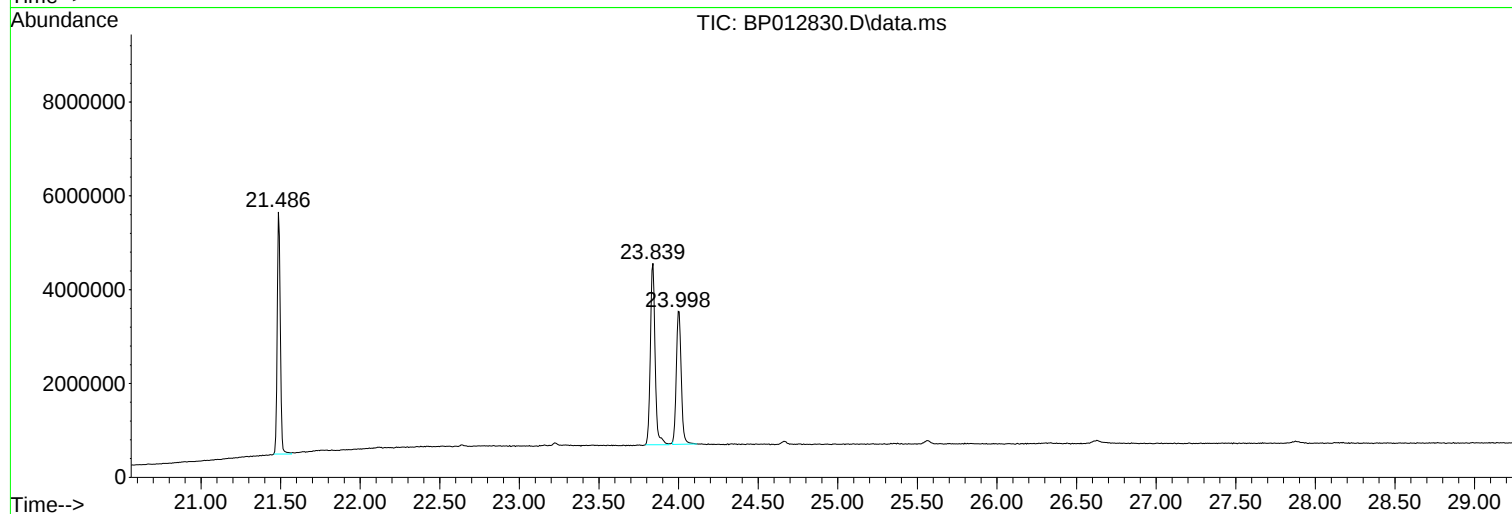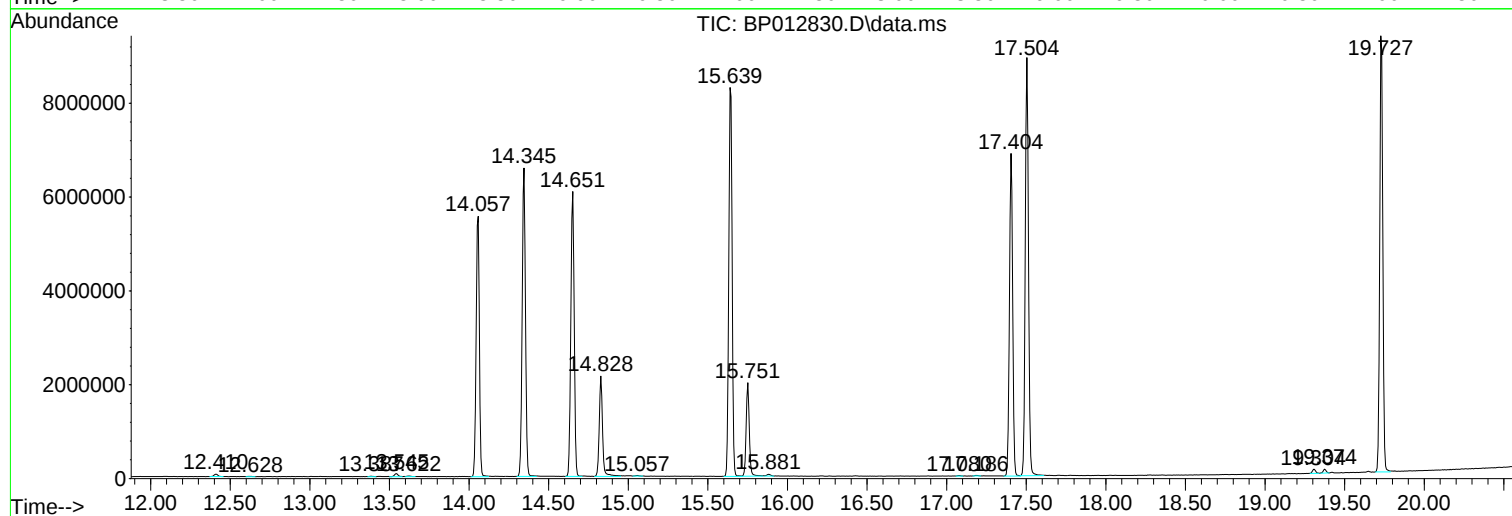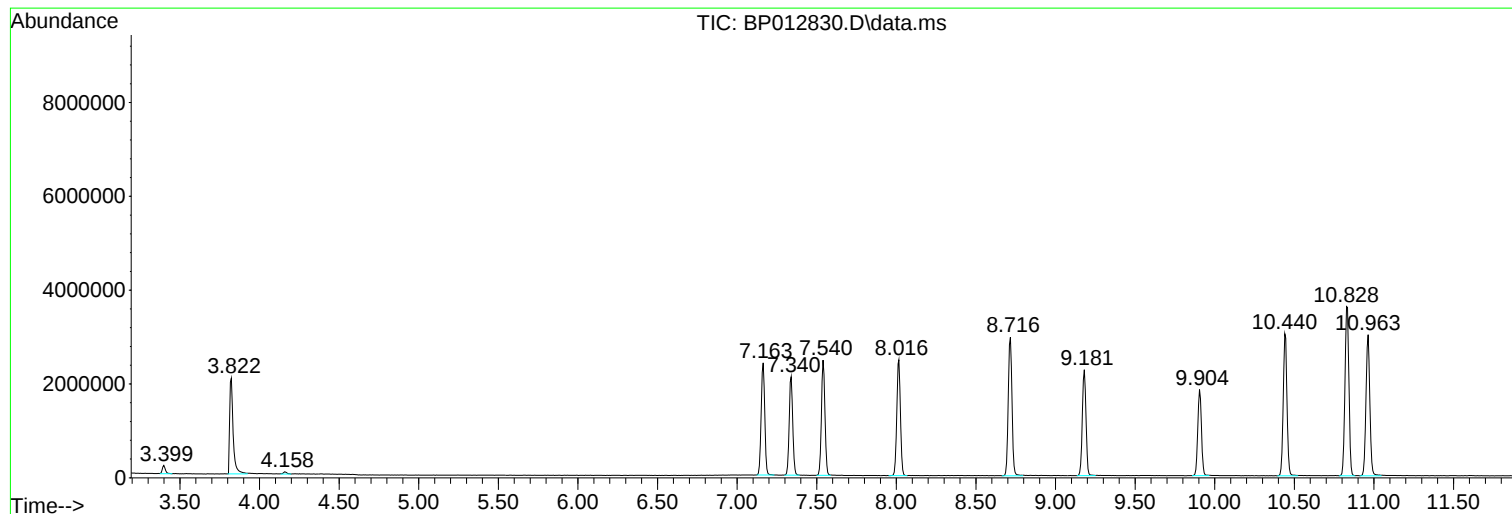

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012830.D
Acq On : 28 Nov 2022 23:21
Operator : CG/JU
Sample : PB149200BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK200

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012830.D
Acq On : 28 Nov 2022 23:21
Operator : CG/JU
Sample : PB149200BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK200

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------