

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012831.D
 Acq On : 28 Nov 2022 23:55
 Operator : CG/JU
 Sample : N5666-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012831.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	44	rVB	134387	177050	1.40%	0.140%
2	3.822	106	108	122	rBV	698776	1031099	8.14%	0.813%
3	4.064	144	149	154	rVB	84019	123646	0.98%	0.097%
4	4.158	161	165	172	rVB	37158	50712	0.40%	0.040%
5	5.099	320	325	331	rVB	25946	36676	0.29%	0.029%
6	7.163	669	676	685	rVB	745852	1167777	9.21%	0.920%
7	7.340	696	706	714	rBV	2351556	3748894	29.58%	2.954%
8	7.540	732	740	749	rBV	2335898	3576482	28.22%	2.818%
9	7.622	749	754	761	rVB5	21616	51296	0.40%	0.040%
10	8.016	813	821	828	rBV	1870260	2984891	23.55%	2.352%
11	8.716	930	940	953	rBV	1987387	3216950	25.38%	2.535%
12	8.834	956	960	966	rVB5	12762	25918	0.20%	0.020%
13	9.181	1011	1019	1030	rBV	2542540	4118457	32.49%	3.245%
14	9.275	1031	1035	1043	rVB5	21515	39888	0.31%	0.031%
15	9.593	1084	1089	1096	rVB9	12980	31954	0.25%	0.025%
16	9.904	1134	1142	1157	rBV	2012697	3250509	25.65%	2.562%
17	10.028	1158	1163	1167	rVB3	11656	21518	0.17%	0.017%
18	10.440	1226	1233	1243	rBV	3254772	5326807	42.03%	4.198%
19	10.610	1256	1262	1265	rBV7	9832	14874	0.12%	0.012%
20	10.828	1291	1299	1309	rBV	2715608	4611498	36.38%	3.634%
21	10.963	1313	1322	1337	rBV	2486497	4237165	33.43%	3.339%
22	11.481	1405	1410	1415	rBV4	14260	25219	0.20%	0.020%
23	11.598	1425	1430	1436	rBV4	17581	32600	0.26%	0.026%
24	12.410	1562	1568	1574	rBV	59052	93684	0.74%	0.074%
25	13.010	1665	1670	1676	rBV10	11032	20894	0.16%	0.016%
26	13.257	1709	1712	1716	rVB4	8163	12900	0.10%	0.010%
27	13.387	1728	1734	1739	rBV9	7554	13697	0.11%	0.011%
28	13.545	1754	1761	1765	rBV	47711	77417	0.61%	0.061%
29	13.622	1768	1774	1777	rVB3	9455	16291	0.13%	0.013%
30	14.057	1840	1848	1860	rBV	5662850	8148172	64.29%	6.421%
31	14.298	1882	1889	1890	rBV7	12801	22785	0.18%	0.018%
32	14.345	1890	1897	1909	rVV	7157596	10251003	80.88%	8.078%
33	14.651	1940	1949	1956	rBV	4134935	6165408	48.64%	4.859%
34	14.828	1973	1979	1993	rBV	384280	634132	5.00%	0.500%
35	14.987	2001	2006	2012	rBV10	10300	26927	0.21%	0.021%
36	15.057	2014	2018	2023	rVB8	26007	41868	0.33%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012831.D
 Acq On : 28 Nov 2022 23:55
 Operator : CG/JU
 Sample : N5666-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	15.445	2080	2084	2089	rBV5	7987	14123	0.11%	0.011%
38	15.639	2110	2117	2129	rBV	8784730	12674544	100.00%	9.988%
39	15.751	2129	2136	2147	rBV	1954334	2648973	20.90%	2.087%
40	15.881	2153	2158	2168	rVB2	36982	64877	0.51%	0.051%
41	16.316	2229	2232	2237	rBV6	12458	20054	0.16%	0.016%
42	16.422	2247	2250	2254	rVB5	10686	14321	0.11%	0.011%
43	17.075	2358	2361	2367	rVB7	12453	19901	0.16%	0.016%
44	17.192	2378	2381	2387	rVB3	20080	30374	0.24%	0.024%
45	17.404	2410	2417	2427	rBV	4593292	6314993	49.82%	4.976%
46	17.504	2427	2434	2451	rVV	8694339	12174689	96.06%	9.594%
47	18.269	2560	2564	2569	rBV4	44300	56470	0.45%	0.045%
48	19.304	2736	2740	2746	rBV	85229	121470	0.96%	0.096%
49	19.375	2748	2752	2757	rVV	73510	99748	0.79%	0.079%
50	19.498	2771	2773	2777	rBV4	32021	38967	0.31%	0.031%
51	19.727	2806	2812	2826	rBV	8431886	11550125	91.13%	9.102%
52	21.486	3106	3111	3122	rBV	3249864	4252844	33.55%	3.351%
53	23.839	3503	3511	3529	rVB	4386705	9040838	71.33%	7.124%
54	23.998	3532	3538	3553	rVB2	1991478	4334042	34.19%	3.415%




Sum of corrected areas: 126898411

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012831.D
Acq On : 28 Nov 2022 23:55
Operator : CG/JU
Sample : N5666-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

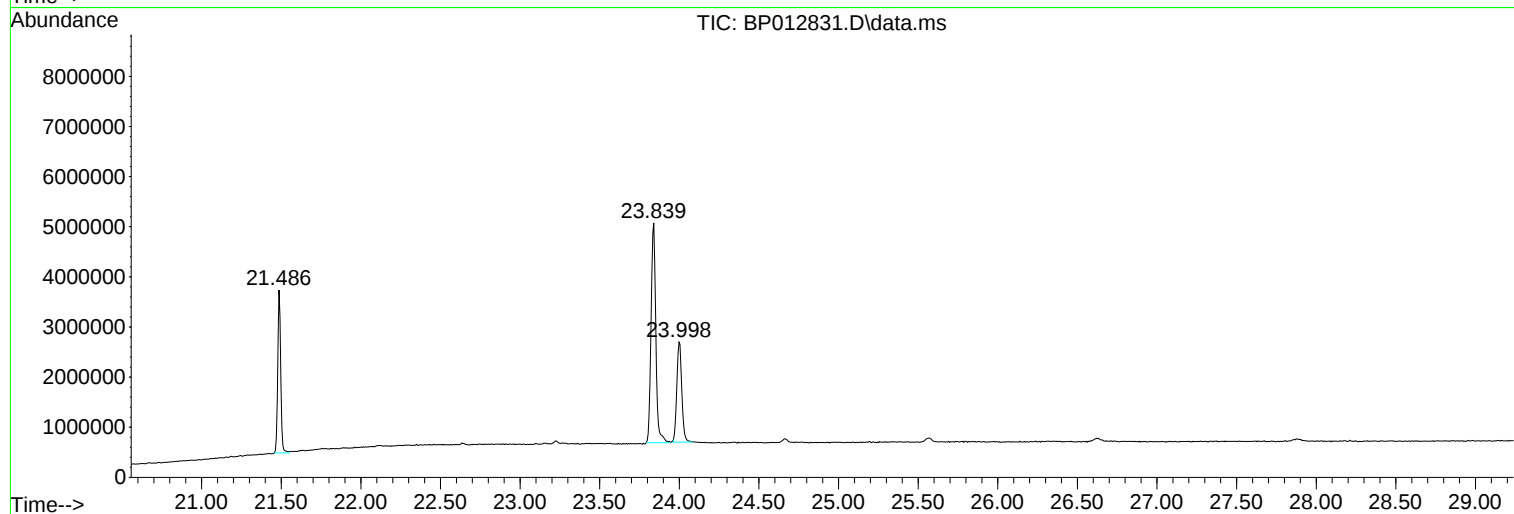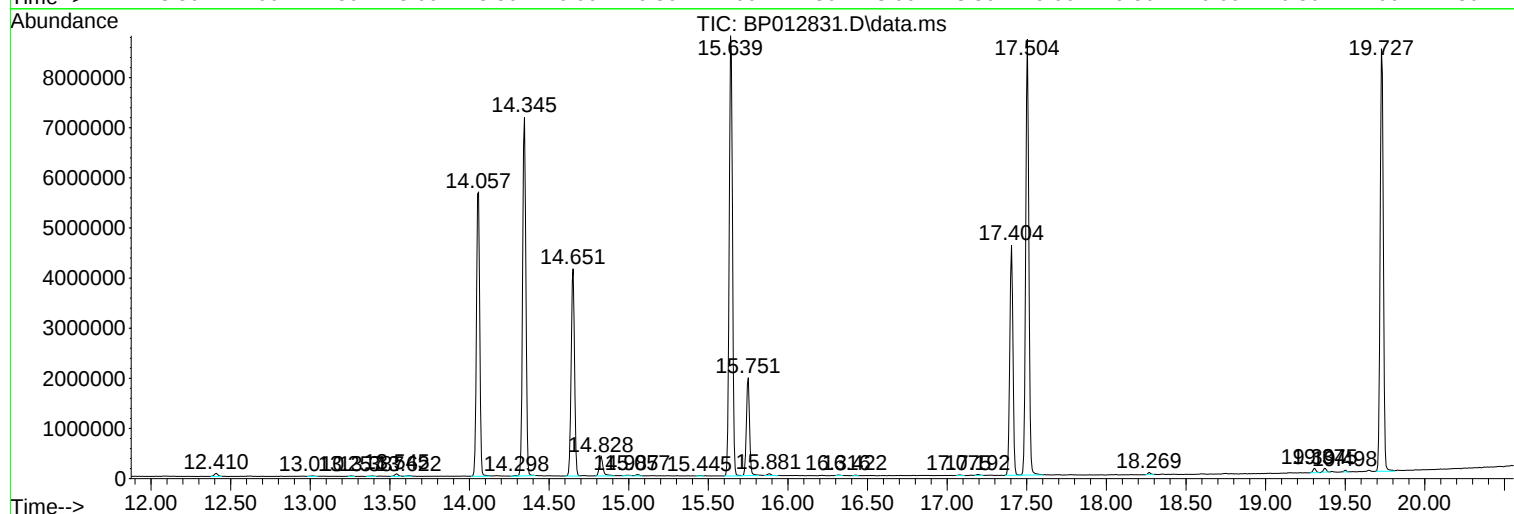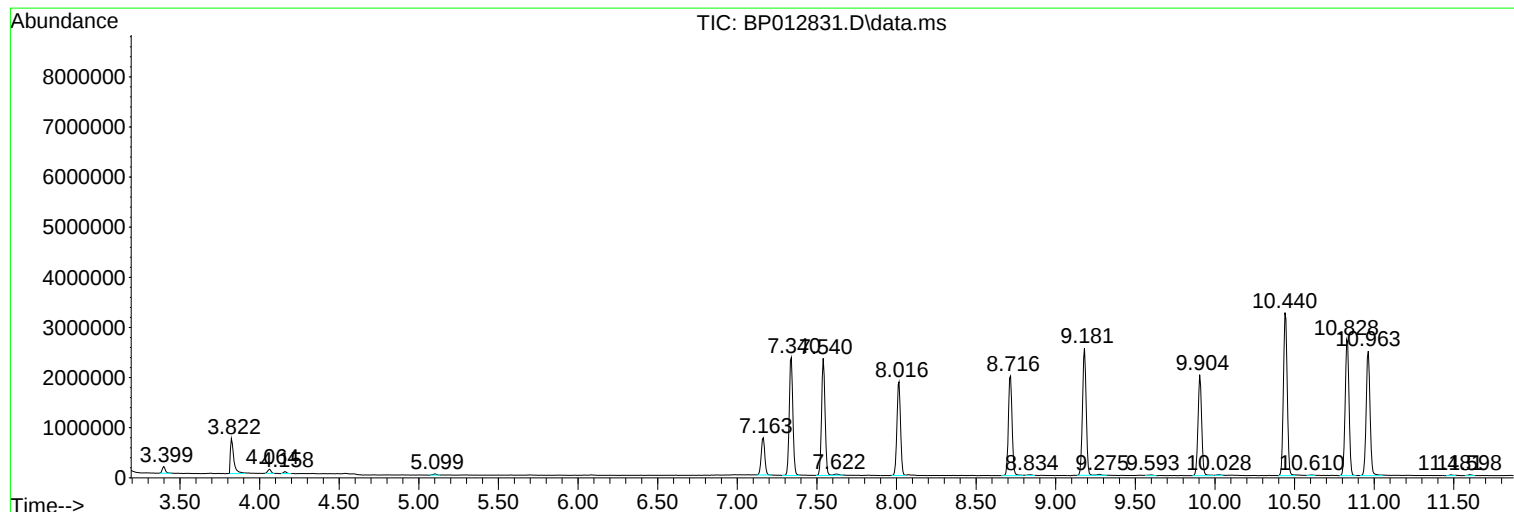

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012831.D
Acq On : 28 Nov 2022 23:55
Operator : CG/JU
Sample : N5666-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012831.D
Acq On : 28 Nov 2022 23:55
Operator : CG/JU
Sample : N5666-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
