

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012832.D
 Acq On : 29 Nov 2022 00:29
 Operator : CG/JU
 Sample : N5666-13
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012832.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	41	rBV	132640	171910	1.92%	0.184%
2	3.822	106	108	127	rBV	690946	1076837	12.03%	1.154%
3	4.058	146	148	153	rVB2	16661	22228	0.25%	0.024%
4	4.158	161	165	170	rVB	43386	60744	0.68%	0.065%
5	4.587	236	238	243	rVB4	11018	15965	0.18%	0.017%
6	5.105	320	326	328	rBV7	6217	10243	0.11%	0.011%
7	7.163	669	676	688	rVB	871123	1368483	15.29%	1.467%
8	7.334	697	705	716	rBV	1188094	1886719	21.08%	2.022%
9	7.540	733	740	750	rBV	1250131	1897246	21.20%	2.033%
10	7.622	750	754	760	rVB6	11666	23747	0.27%	0.025%
11	8.016	812	821	828	rBV	2219777	3568776	39.87%	3.825%
12	8.069	828	830	840	rVB9	11831	21997	0.25%	0.024%
13	8.716	929	940	949	rBV	1326362	2163036	24.17%	2.318%
14	9.122	1003	1009	1011	rBV6	9834	15215	0.17%	0.016%
15	9.181	1011	1019	1030	rVV	1234987	1992233	22.26%	2.135%
16	9.346	1043	1047	1052	rVB8	7030	10583	0.12%	0.011%
17	9.599	1081	1090	1095	rVB7	11985	27765	0.31%	0.030%
18	9.904	1134	1142	1151	rBV	919904	1476194	16.49%	1.582%
19	10.440	1225	1233	1246	rBV	1602405	2632585	29.41%	2.821%
20	10.598	1255	1260	1273	rBV	106893	207414	2.32%	0.222%
21	10.828	1291	1299	1307	rBV	3362243	5623904	62.84%	6.027%
22	10.963	1314	1322	1336	rBV	1376390	2319326	25.91%	2.486%
23	11.487	1404	1411	1416	rBV10	5306	12851	0.14%	0.014%
24	12.087	1508	1513	1518	rBV9	6366	11816	0.13%	0.013%
25	12.240	1535	1539	1543	rVB5	8526	10234	0.11%	0.011%
26	12.410	1561	1568	1573	rBV2	32016	57274	0.64%	0.061%
27	12.869	1642	1646	1650	rBV7	5420	9510	0.11%	0.010%
28	13.392	1726	1735	1738	rBV10	10712	22478	0.25%	0.024%
29	13.475	1744	1749	1751	rBV5	10684	16424	0.18%	0.018%
30	13.539	1755	1760	1768	rVB2	48911	81647	0.91%	0.088%
31	13.622	1768	1774	1777	rBV8	9811	16880	0.19%	0.018%
32	14.051	1841	1847	1861	rBV	3318900	4486220	50.12%	4.808%
33	14.287	1883	1887	1889	rBV5	8649	12477	0.14%	0.013%
34	14.345	1889	1897	1907	rVV	3703272	5383423	60.15%	5.769%
35	14.651	1941	1949	1960	rBV	5484460	8035473	89.78%	8.612%
36	14.828	1973	1979	1990	rBV	455108	747493	8.35%	0.801%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012832.D
 Acq On : 29 Nov 2022 00:29
 Operator : CG/JU
 Sample : N5666-13
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	15.051	2014	2017	2024	rVB9	15130	25747	0.29%	0.028%
38	15.492	2090	2092	2097	rVB6	7647	9290	0.10%	0.010%
39	15.639	2109	2117	2126	rBV	4966378	7068426	78.98%	7.575%
40	15.745	2129	2135	2148	rVV	463419	712502	7.96%	0.764%
41	15.881	2154	2158	2166	rVB3	21527	37603	0.42%	0.040%
42	16.004	2175	2179	2184	rBV4	16935	25452	0.28%	0.027%
43	16.333	2230	2235	2236	rBV4	9491	11827	0.13%	0.013%
44	16.357	2236	2239	2242	rVB5	6520	9040	0.10%	0.010%
45	16.428	2248	2251	2256	rVB7	9298	13710	0.15%	0.015%
46	16.539	2266	2270	2272	rBV5	6848	9568	0.11%	0.010%
47	17.151	2372	2374	2377	rBV3	7781	12471	0.14%	0.013%
48	17.186	2377	2380	2387	rVB4	26953	42749	0.48%	0.046%
49	17.404	2410	2417	2427	rBV	6648886	8950115	100.00%	9.592%
50	17.504	2427	2434	2446	rBV	5381658	7469097	83.45%	8.005%
51	18.063	2525	2529	2534	rVB5	29716	37750	0.42%	0.040%
52	18.269	2560	2564	2573	rBV2	94345	130419	1.46%	0.140%
53	19.192	2718	2721	2727	rVB7	24729	29229	0.33%	0.031%
54	19.310	2737	2741	2747	rBV4	57313	84028	0.94%	0.090%
55	19.374	2748	2752	2757	rVV	49692	69740	0.78%	0.075%
56	19.498	2770	2773	2777	rBV4	40368	53481	0.60%	0.057%
57	19.651	2796	2799	2803	rVB3	35197	40831	0.46%	0.044%
58	19.727	2807	2812	2822	rVV	5541903	7402804	82.71%	7.934%
59	21.486	3106	3111	3121	rBV	4604209	6162784	68.86%	6.605%
60	23.833	3504	3510	3518	rBV2	2063024	4160791	46.49%	4.459%
61	23.998	3531	3538	3554	rVB	2464562	5242220	58.57%	5.618%




Sum of corrected areas: 93309024

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012832.D
Acq On : 29 Nov 2022 00:29
Operator : CG/JU
Sample : N5666-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB35

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

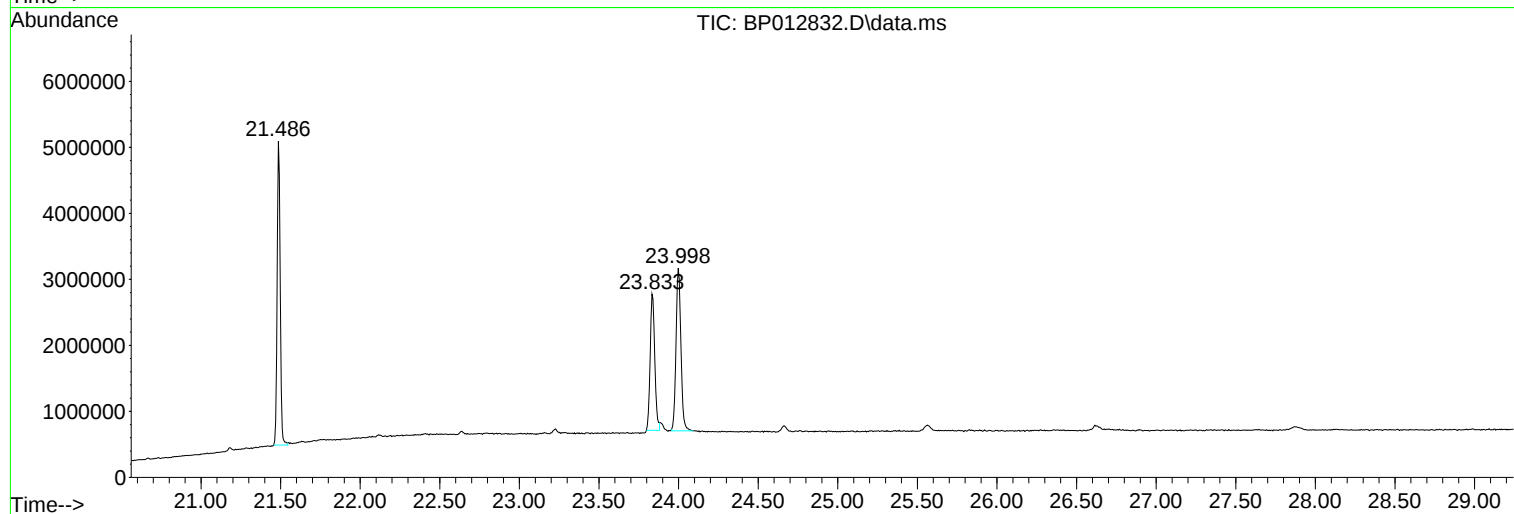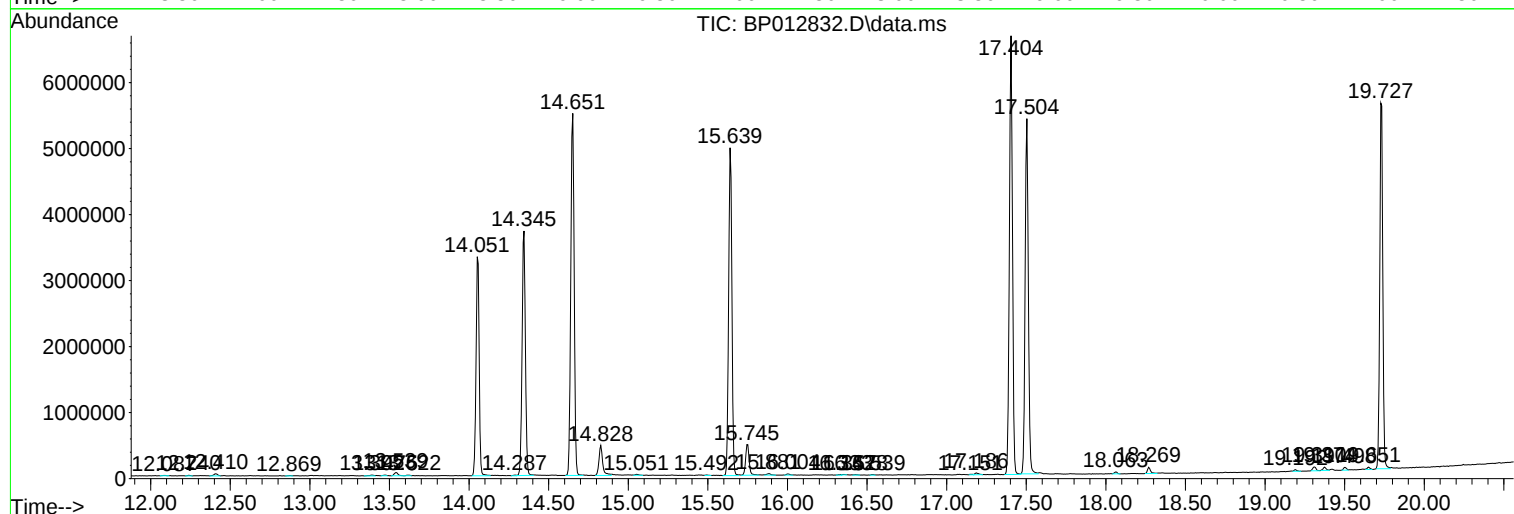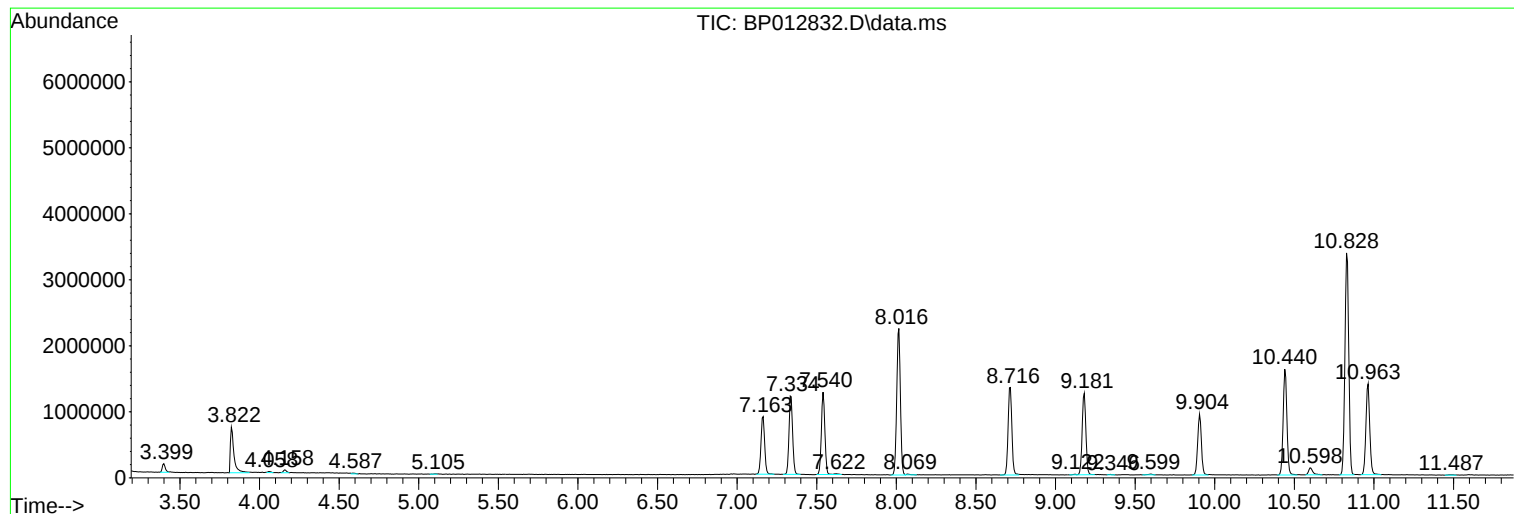

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012832.D
Acq On : 29 Nov 2022 00:29
Operator : CG/JU
Sample : N5666-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB35

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012832.D
Acq On : 29 Nov 2022 00:29
Operator : CG/JU
Sample : N5666-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB35

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc