

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012833.D
 Acq On : 29 Nov 2022 01:03
 Operator : CG/JU
 Sample : N5666-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGXP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012833.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	26	31	33	rBV	93116	135478	1.01%	0.099%
2	3.399	33	36	39	rVV	149183	190107	1.41%	0.139%
3	3.434	39	42	48	rVB	99969	130798	0.97%	0.095%
4	3.681	82	84	91	rBV2	18667	22485	0.17%	0.016%
5	3.822	105	108	126	rBV	865824	1339581	9.97%	0.976%
6	4.064	143	149	154	rVB	72604	115581	0.86%	0.084%
7	4.158	161	165	171	rVB	46784	66355	0.49%	0.048%
8	7.163	668	676	684	rVB	535424	855381	6.36%	0.623%
9	7.334	699	705	717	rBV	2137790	3385243	25.18%	2.467%
10	7.540	732	740	750	rBV	1965114	3032539	22.56%	2.210%
11	7.622	750	754	763	rVB5	19393	42548	0.32%	0.031%
12	8.016	811	821	828	rBV	2237978	3610031	26.86%	2.630%
13	8.075	828	831	835	rVB3	19745	27941	0.21%	0.020%
14	8.710	932	939	951	rBV	1586583	2562872	19.07%	1.867%
15	9.181	1011	1019	1031	rVV	2395715	3813918	28.37%	2.779%
16	9.263	1031	1033	1040	rVB8	10044	18309	0.14%	0.013%
17	9.599	1084	1090	1095	rVB2	57253	94720	0.70%	0.069%
18	9.904	1134	1142	1156	rBV	1771519	2859577	21.27%	2.084%
19	10.440	1225	1233	1247	rBV	2904774	4726015	35.16%	3.444%
20	10.828	1290	1299	1307	rBV	3430280	5693942	42.36%	4.149%
21	10.963	1312	1322	1332	rBV	2738447	4544511	33.81%	3.311%
22	11.493	1404	1412	1415	rBV9	6779	14552	0.11%	0.011%
23	11.598	1425	1430	1437	rBV10	7929	18501	0.14%	0.013%
24	11.846	1467	1472	1476	rBV6	11557	17335	0.13%	0.013%
25	12.240	1531	1539	1544	rBV	66960	107172	0.80%	0.078%
26	12.410	1561	1568	1573	rBV2	54508	92745	0.69%	0.068%
27	12.869	1641	1646	1649	rBV5	16579	26141	0.19%	0.019%
28	13.045	1668	1676	1684	rVB5	23723	44071	0.33%	0.032%
29	13.128	1688	1690	1696	rVB5	14676	20590	0.15%	0.015%
30	13.187	1696	1700	1706	rBV3	22276	32653	0.24%	0.024%
31	13.381	1728	1733	1739	rVV9	8879	16587	0.12%	0.012%
32	13.469	1739	1748	1755	rVV	101537	165096	1.23%	0.120%
33	13.540	1755	1760	1768	rVV	70352	130772	0.97%	0.095%
34	13.622	1770	1774	1780	rVV5	17395	36645	0.27%	0.027%
35	13.704	1784	1788	1794	rVB9	7400	14129	0.11%	0.010%
36	14.051	1841	1847	1854	rBV	5894834	8181959	60.87%	5.962%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012833.D
 Acq On : 29 Nov 2022 01:03
 Operator : CG/JU
 Sample : N5666-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGXP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

37	14.128	1858	1860	1863	rVV4	17920	18524	0.14%	0.013%
38	14.169	1863	1867	1875	rVB9	14423	23567	0.18%	0.017%
39	14.287	1883	1887	1890	rBV6	15867	25121	0.19%	0.018%
40	14.345	1890	1897	1915	rVB	6637125	9915172	73.76%	7.225%
41	14.539	1926	1930	1935	rVB2	31980	42122	0.31%	0.031%
42	14.651	1941	1949	1956	rBV	5475782	7908901	58.84%	5.763%
43	14.728	1958	1962	1971	rVB	9730	21769	0.16%	0.016%
44	14.828	1973	1979	1995	rBV	316552	521981	3.88%	0.380%
45	15.057	2013	2018	2022	rVB5	31277	51419	0.38%	0.037%
46	15.151	2032	2034	2043	rVB10	6586	13815	0.10%	0.010%
47	15.434	2078	2082	2088	rBV7	10152	17783	0.13%	0.013%
48	15.492	2088	2092	2096	rVB3	18399	25105	0.19%	0.018%
49	15.639	2110	2117	2129	rBV	9178314	12989145	96.63%	9.464%
50	15.751	2129	2136	2145	rBV	2033240	2735336	20.35%	1.993%
51	15.881	2154	2158	2165	rVB3	40914	71628	0.53%	0.052%
52	16.004	2174	2179	2184	rBV	324798	439496	3.27%	0.320%
53	16.210	2210	2214	2219	rVB8	8142	14600	0.11%	0.011%
54	16.422	2247	2250	2254	rVB6	10995	15623	0.12%	0.011%
55	16.569	2272	2275	2281	rVB5	11556	16282	0.12%	0.012%
56	16.875	2325	2327	2333	rVB7	9934	16587	0.12%	0.012%
57	17.075	2355	2361	2370	rBV7	12755	29704	0.22%	0.022%
58	17.151	2371	2374	2376	rVV4	11832	14013	0.10%	0.010%
59	17.192	2377	2381	2388	rVB5	15875	32719	0.24%	0.024%
60	17.404	2410	2417	2426	rBV	6266109	8608710	64.04%	6.273%
61	17.504	2427	2434	2444	rVV	9632839	13442205	100.00%	9.795%
62	17.586	2445	2448	2453	rVB2	55770	70557	0.52%	0.051%
63	17.710	2467	2469	2475	rVB7	13111	15331	0.11%	0.011%
64	17.775	2477	2480	2484	rVV4	13578	15892	0.12%	0.012%
65	18.063	2526	2529	2534	rVB7	11712	14491	0.11%	0.011%
66	18.269	2560	2564	2574	rBV	284301	379923	2.83%	0.277%
67	18.686	2632	2635	2639	rBV3	31279	34976	0.26%	0.025%
68	19.304	2736	2740	2746	rBV	95450	128945	0.96%	0.094%
69	19.375	2747	2752	2756	rBV	93074	148726	1.11%	0.108%
70	19.498	2770	2773	2777	rBV3	69609	86138	0.64%	0.063%
71	19.651	2796	2799	2802	rBV	33986	37985	0.28%	0.028%
72	19.727	2806	2812	2824	rVV	9820405	13228820	98.41%	9.639%
73	21.180	3055	3059	3065	rBV2	258056	364756	2.71%	0.266%
74	21.486	3106	3111	3120	rBV	4395090	5839388	43.44%	4.255%
75	23.833	3503	3510	3528	rBV2	4164850	8503811	63.26%	6.196%
76	23.998	3531	3538	3551	rVB2	2489452	5173033	38.48%	3.769%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012833.D
Acq On : 29 Nov 2022 01:03
Operator : CG/JU
Sample : N5666-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGXP4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 137240979

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012833.D
Acq On : 29 Nov 2022 01:03
Operator : CG/JU
Sample : N5666-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGXP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

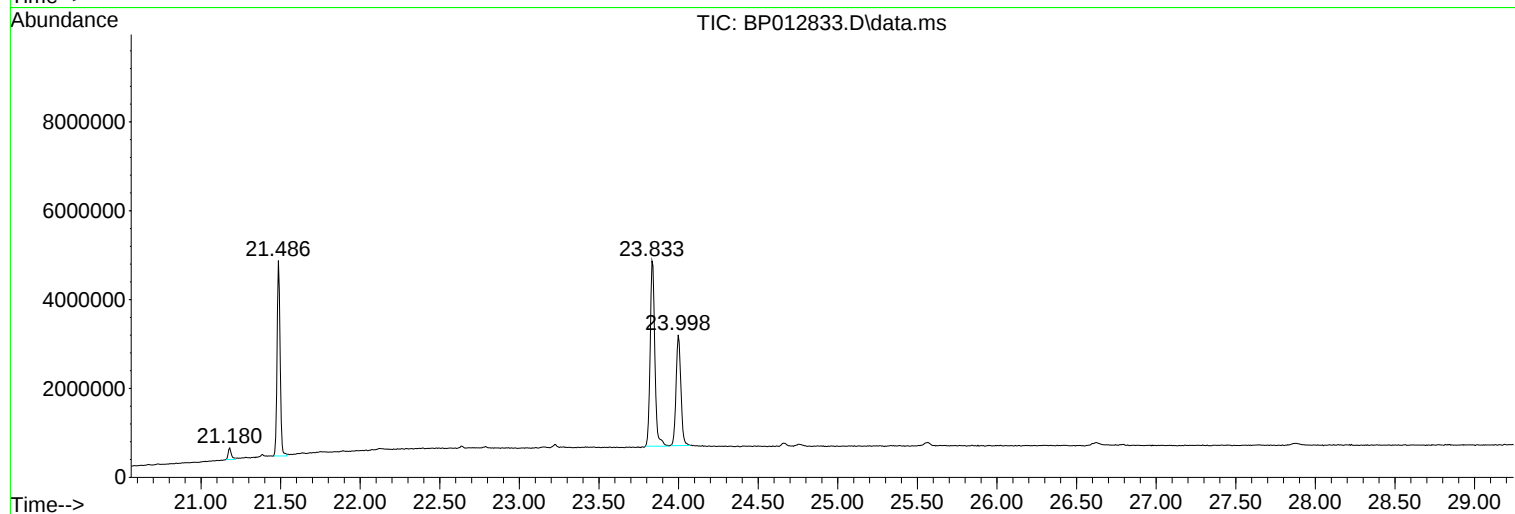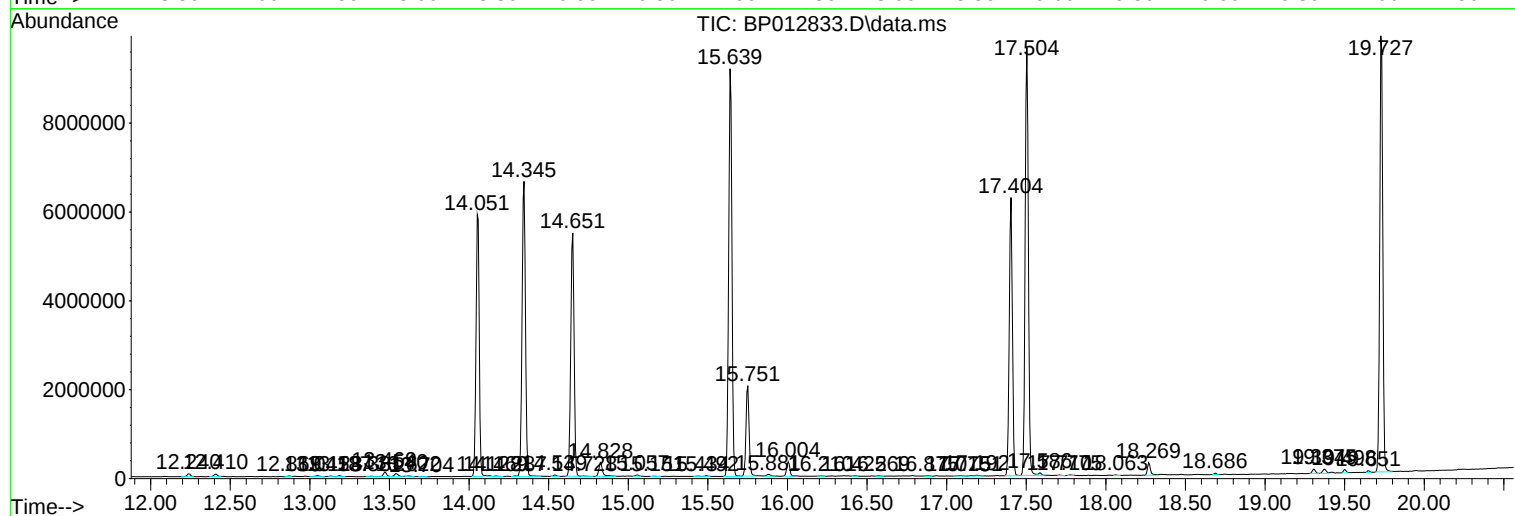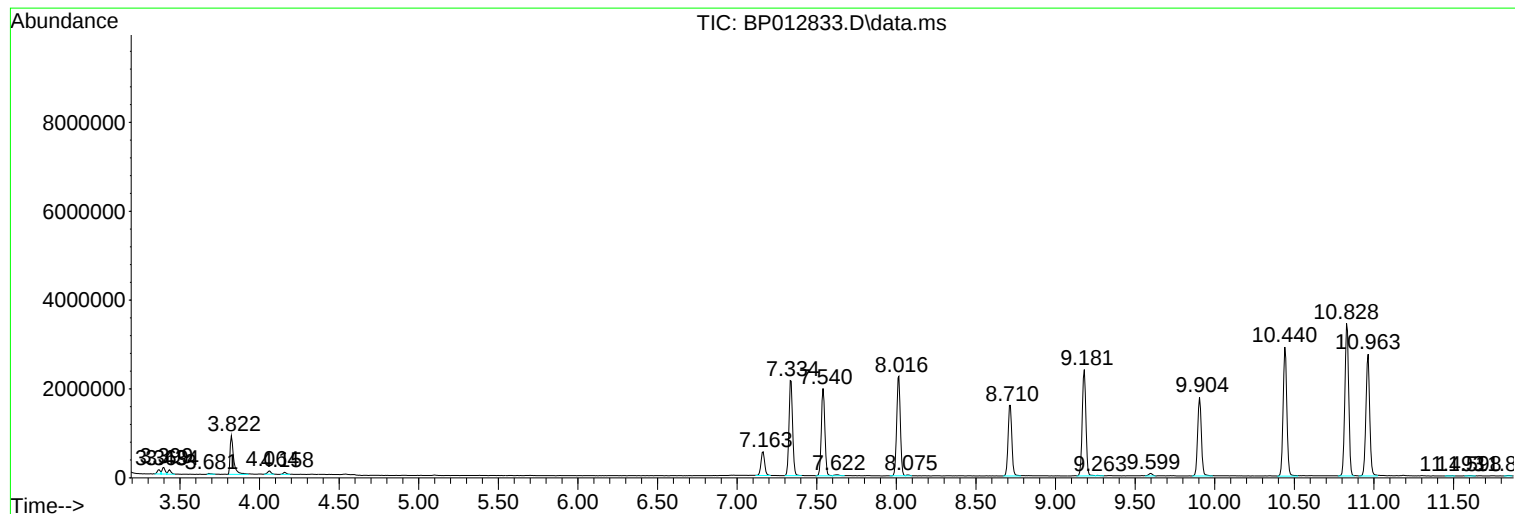

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012833.D
Acq On : 29 Nov 2022 01:03
Operator : CG/JU
Sample : N5666-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGXP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012833.D
Acq On : 29 Nov 2022 01:03
Operator : CG/JU
Sample : N5666-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGXP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc