

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
 Data File : BP012837.D
 Acq On : 29 Nov 2022 03:20
 Operator : CG/JU
 Sample : N5666-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHB26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
 Title : SVOA CALIBRATION

Signal : TIC: BP012837.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	32	36	38	rBV	123952	151491	1.08%	0.114%
2	3.434	38	42	50	rVB	339165	446156	3.17%	0.336%
3	3.823	105	108	123	rBV	555136	869797	6.18%	0.654%
4	4.064	144	149	157	rVB	65416	104532	0.74%	0.079%
5	4.158	161	165	169	rBV	36024	54794	0.39%	0.041%
6	5.105	320	326	329	rBV6	15771	27383	0.19%	0.021%
7	7.164	669	676	686	rVB	590472	931123	6.62%	0.701%
8	7.340	699	706	719	rVB	1975866	3161818	22.48%	2.379%
9	7.540	733	740	748	rBV	1954220	2991456	21.26%	2.251%
10	7.616	749	753	763	rVB2	24291	58053	0.41%	0.044%
11	8.016	812	821	827	rBV	2005276	3271890	23.26%	2.462%
12	8.069	827	830	835	rVB7	10607	16500	0.12%	0.012%
13	8.716	930	940	950	rBV	1623491	2645091	18.80%	1.990%
14	9.181	1010	1019	1029	rBV	2181267	3519748	25.02%	2.648%
15	9.275	1031	1035	1043	rVB8	13605	28600	0.20%	0.022%
16	9.593	1082	1089	1097	rVB2	20048	40989	0.29%	0.031%
17	9.905	1134	1142	1153	rBV	1696224	2715064	19.30%	2.043%
18	10.440	1226	1233	1246	rBV	2786097	4512334	32.08%	3.395%
19	10.605	1255	1261	1273	rBV	63855	119459	0.85%	0.090%
20	10.828	1291	1299	1306	rBV	3089188	5184772	36.86%	3.901%
21	10.887	1306	1309	1313	rVB4	24243	29112	0.21%	0.022%
22	10.963	1314	1322	1335	rBV	2251722	3798630	27.00%	2.858%
23	11.487	1405	1411	1418	rBV	6960	17897	0.13%	0.013%
24	11.599	1423	1430	1435	rVV9	13105	23883	0.17%	0.018%
25	12.087	1508	1513	1517	rBV6	9982	17579	0.12%	0.013%
26	12.240	1535	1539	1543	rVB2	18655	27238	0.19%	0.020%
27	12.410	1562	1568	1577	rVB2	49641	84401	0.60%	0.064%
28	13.257	1706	1712	1717	rVB10	7119	14905	0.11%	0.011%
29	13.469	1744	1748	1755	rVB3	23892	35323	0.25%	0.027%
30	13.546	1755	1761	1767	rBV2	40224	64930	0.46%	0.049%
31	13.616	1769	1773	1778	rVV3	11912	17496	0.12%	0.013%
32	14.051	1840	1847	1864	rBV	5620334	8062935	57.32%	6.067%
33	14.340	1883	1896	1909	rBV	6334515	9490709	67.47%	7.141%
34	14.651	1942	1949	1958	rVV	4934424	7315471	52.00%	5.504%
35	14.722	1958	1961	1967	rVB8	8949	16003	0.11%	0.012%
36	14.828	1973	1979	1992	rBV	414381	672917	4.78%	0.506%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012837.D
Acq On : 29 Nov 2022 03:20
Operator : CG/JU
Sample : N5666-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Title : SVOA CALIBRATION

37	15.057	2012	2018	2024	rVB4	42607	67097	0.48%	0.050%
38	15.640	2109	2117	2128	rBV	8696739	12878312	91.55%	9.690%
39	15.751	2129	2136	2153	rVV	2205972	3074238	21.85%	2.313%
40	15.881	2153	2158	2164	rVB4	43793	79362	0.56%	0.060%
41	16.004	2174	2179	2184	rVB	86331	114652	0.82%	0.086%
42	16.204	2209	2213	2219	rVB5	11008	18226	0.13%	0.014%
43	16.422	2246	2250	2254	rBV7	10876	16984	0.12%	0.013%
44	17.187	2377	2380	2387	rVB3	17080	33098	0.24%	0.025%
45	17.263	2387	2393	2398	rBV4	20334	43691	0.31%	0.033%
46	17.404	2410	2417	2426	rBV	5678653	8144562	57.90%	6.128%
47	17.504	2427	2434	2445	rBV	9817775	14049130	99.87%	10.571%
48	17.781	2475	2481	2484	rBV4	14214	27387	0.19%	0.021%
49	18.063	2525	2529	2534	rVB6	25281	34754	0.25%	0.026%
50	18.269	2560	2564	2569	rBV	118809	141502	1.01%	0.106%
51	18.686	2632	2635	2639	rBV6	17202	23336	0.17%	0.018%
52	19.304	2736	2740	2746	rBV	104424	138208	0.98%	0.104%
53	19.375	2747	2752	2757	rBV	91277	137964	0.98%	0.104%
54	19.498	2770	2773	2779	rBV3	62538	74175	0.53%	0.056%
55	19.645	2796	2798	2804	rVB6	31401	38538	0.27%	0.029%
56	19.728	2806	2812	2823	rBV	10696788	14067527	100.00%	10.585%
57	21.486	3106	3111	3118	rBV	4038212	5540268	39.38%	4.169%
58	23.833	3503	3510	3527	rBV2	4234852	8749688	62.20%	6.584%
59	23.998	3531	3538	3552	rVB2	2339931	4869366	34.61%	3.664%




Sum of corrected areas: 132902544

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012837.D
Acq On : 29 Nov 2022 03:20
Operator : CG/JU
Sample : N5666-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB26

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

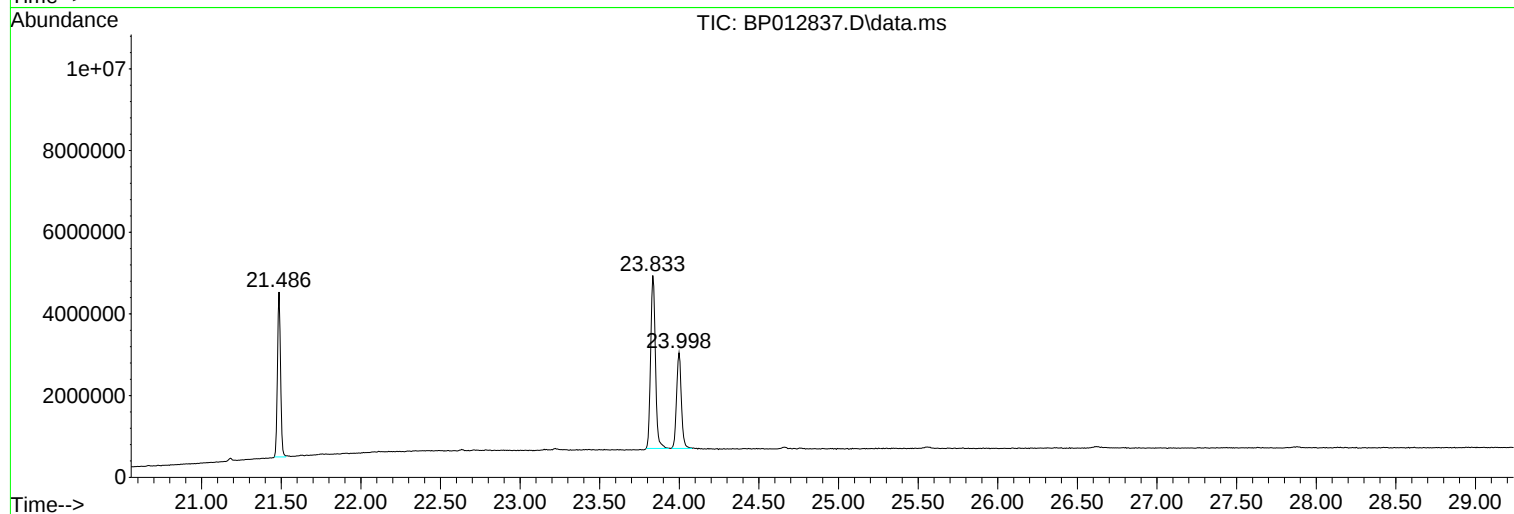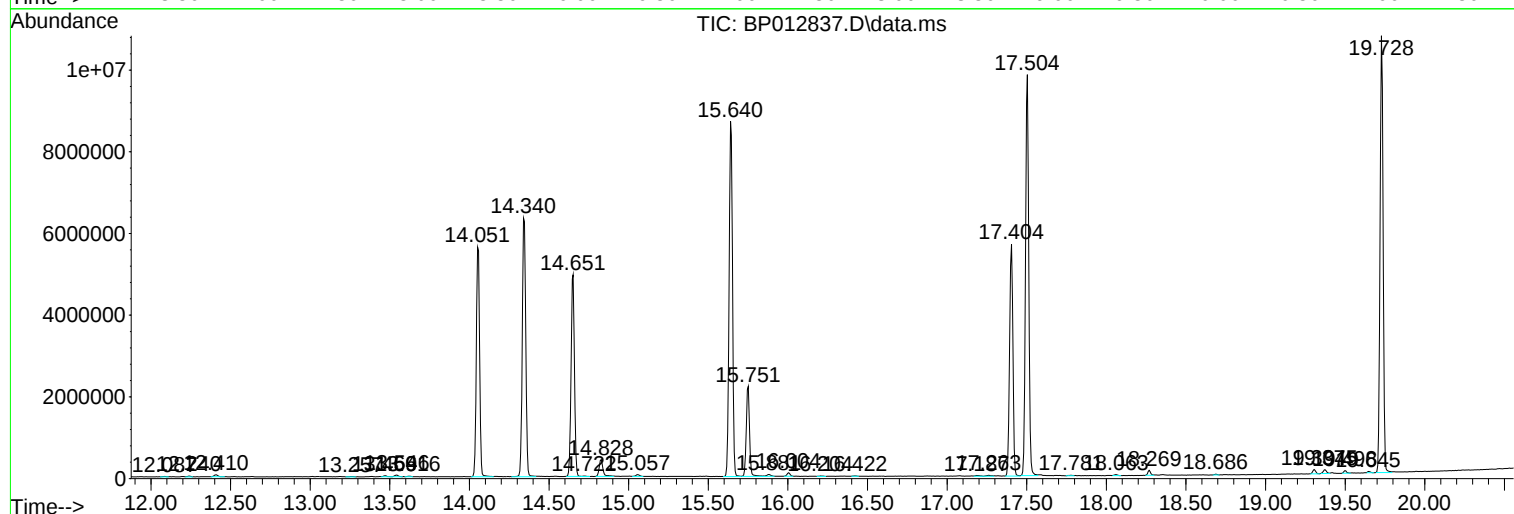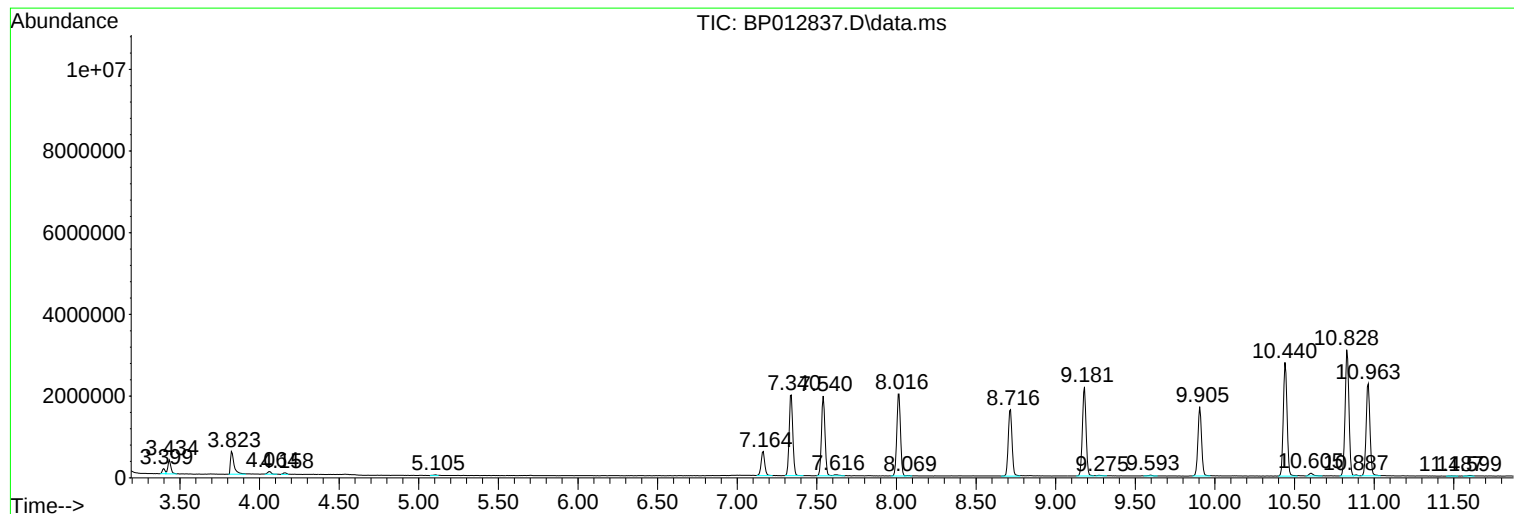

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012837.D
Acq On : 29 Nov 2022 03:20
Operator : CG/JU
Sample : N5666-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB26

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP112822\
Data File : BP012837.D
Acq On : 29 Nov 2022 03:20
Operator : CG/JU
Sample : N5666-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHB26

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc